

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
 Data File : PD055723.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 23:24
 Operator : SG\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 06:35:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:31:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.963	66831057	84592290	74.452	73.199
28)	SA Decachlor...	7.964	8.998	64852894	93539965	71.369	71.071
Target Compounds							
23)	Chlordane-1	4.130	4.951	19344743	33063747	731.233	730.863
24)	Chlordane-2	4.621	5.416	22851551	35102366	747.077	703.770
25)	Chlordane-3	5.176	6.059	69981341	157.0E6	737.549	734.102
26)	Chlordane-4	5.232	6.133	61815956	185.3E6	743.819	728.305
27)	Chlordane-5	6.056	6.933	22558463	34113382	732.978	742.242



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
Data File : PD055723.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 23:24
Operator : SG\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 06:35:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:31:17 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

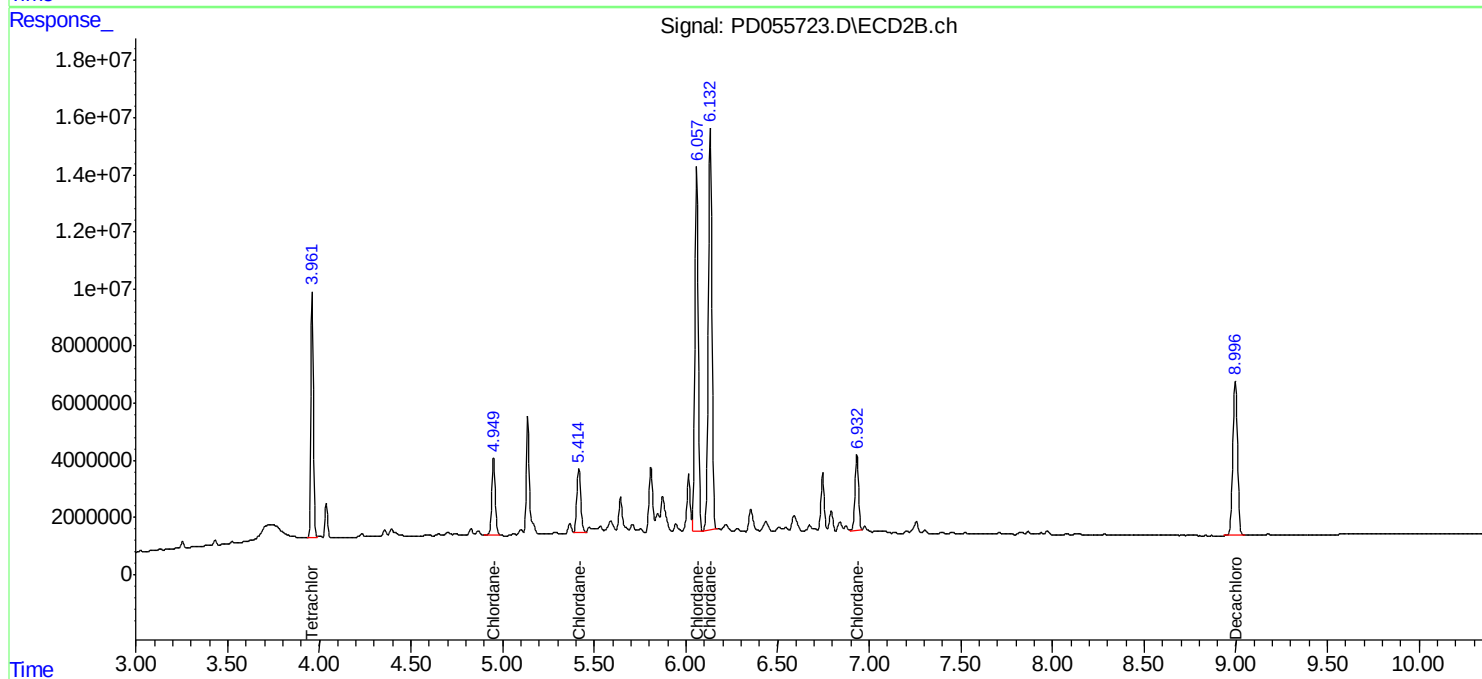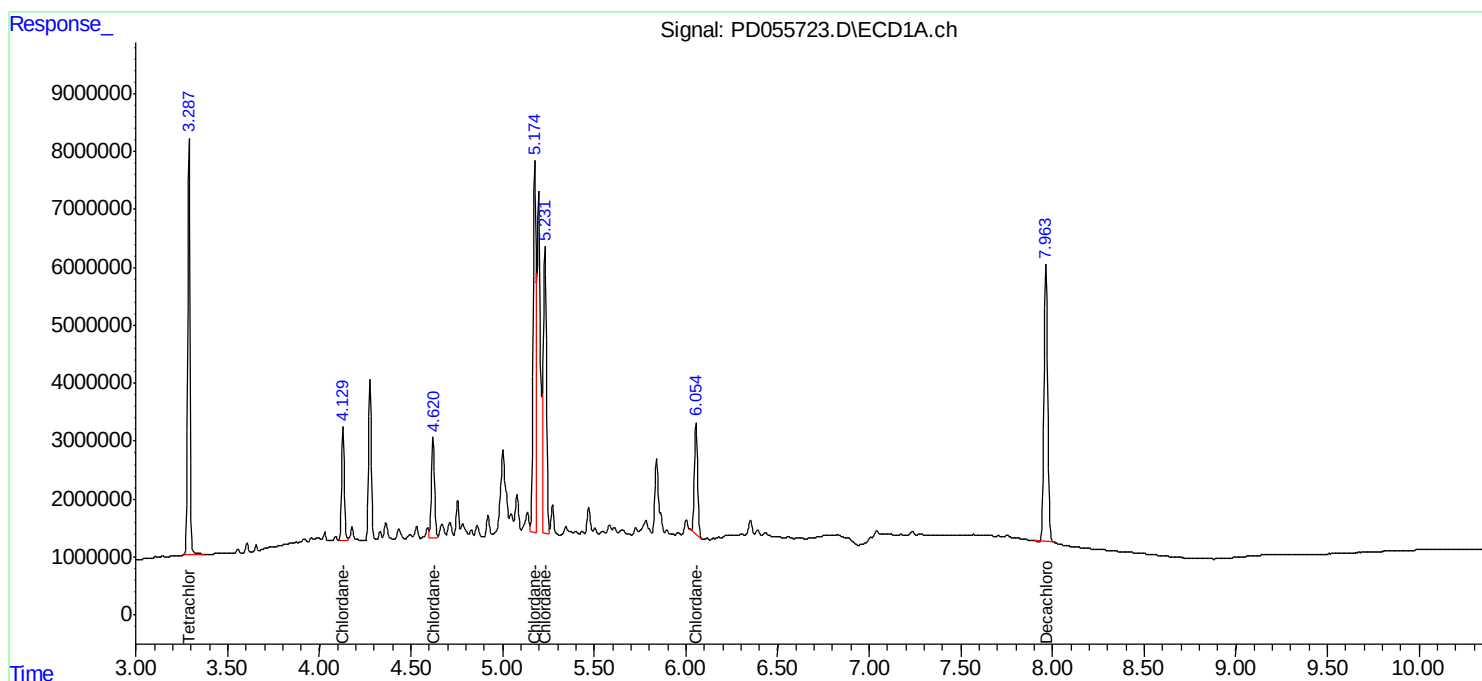


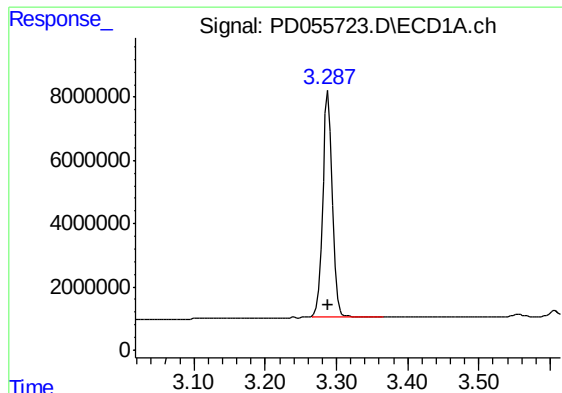

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 66831057
Conc: 74.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

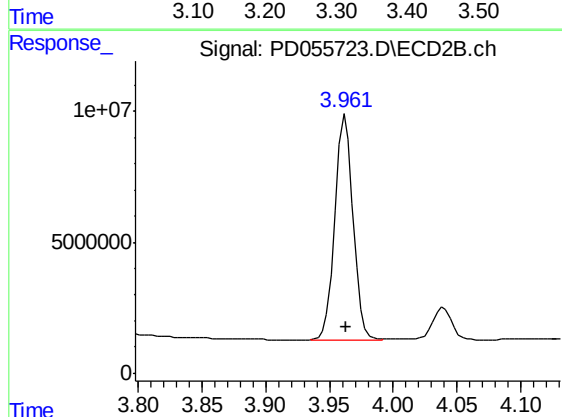


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 84592290
Conc: 73.20 ng/ml

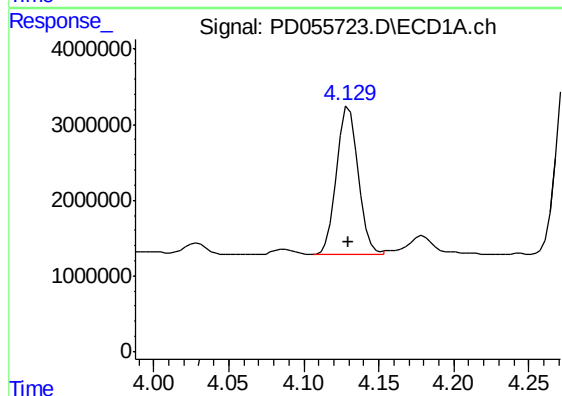


#23 Chlordane-1

R.T.: 4.130 min
Delta R.T.: 0.000 min
Response: 19344743
Conc: 731.23 ng/ml

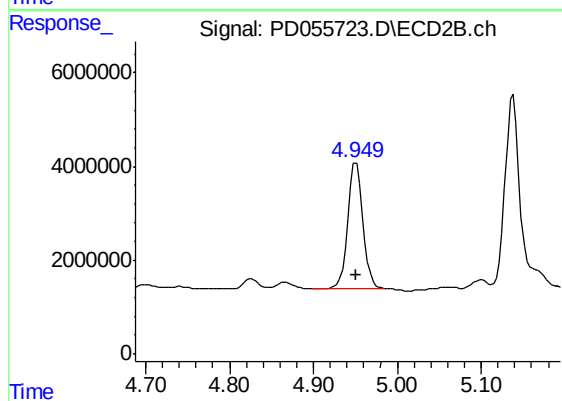

#23 Chlordane-1


R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 33063747
Conc: 730.86 ng/ml

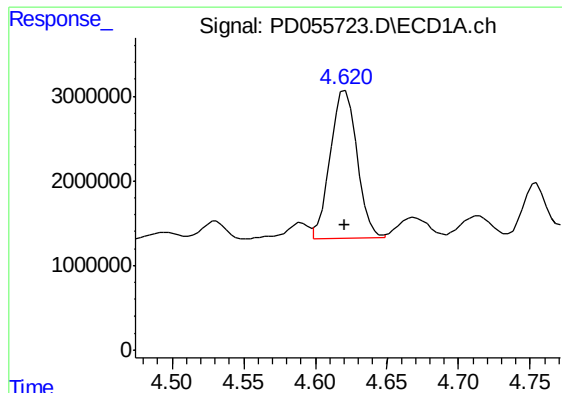

#24 Chlordane-2


R.T.: 4.621 min
Delta R.T.: 0.000 min
Response: 22851551
Conc: 747.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

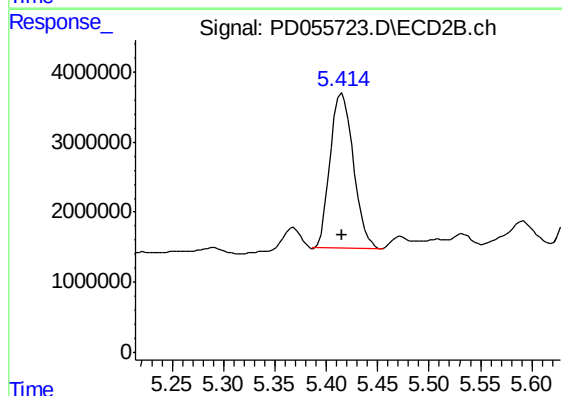


#24 Chlordane-2

R.T.: 5.416 min
Delta R.T.: 0.000 min
Response: 35102366
Conc: 703.77 ng/ml

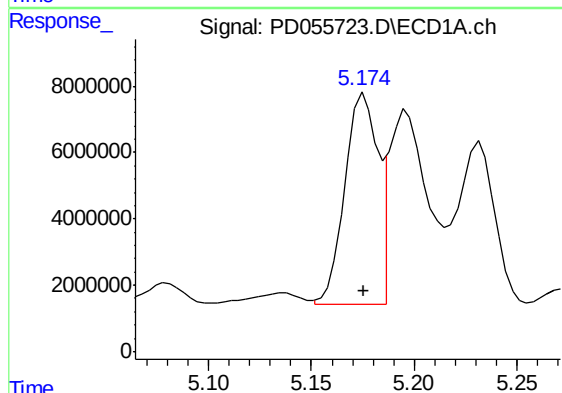


#25 Chlordane-3

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 69981341
Conc: 737.55 ng/ml

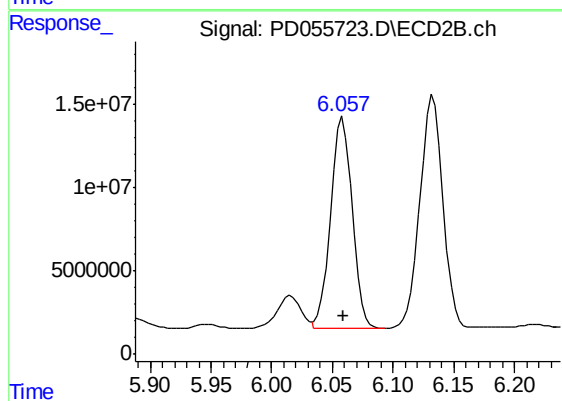

#25 Chlordane-3


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 156954999
Conc: 734.10 ng/ml

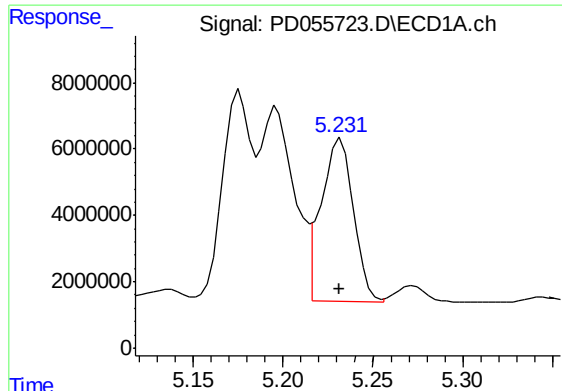

#26 Chlordane-4


R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 61815956
Conc: 743.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

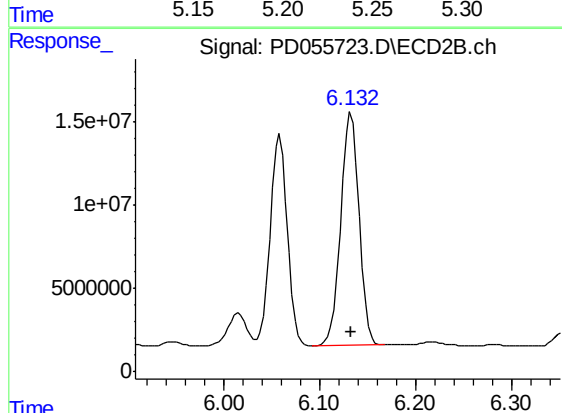


#26 Chlordane-4

R.T.: 6.133 min
Delta R.T.: 0.000 min
Response: 185341584
Conc: 728.31 ng/ml

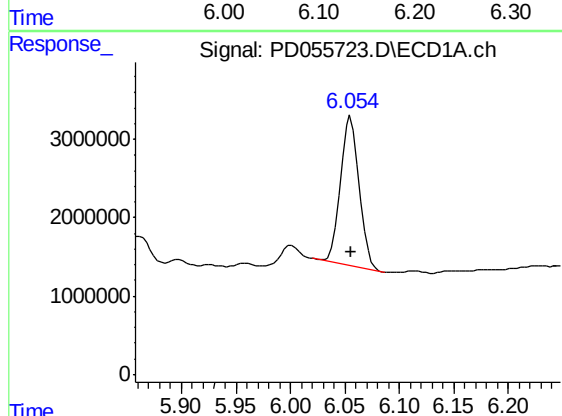


#27 Chlordane-5

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 22558463
Conc: 732.98 ng/ml

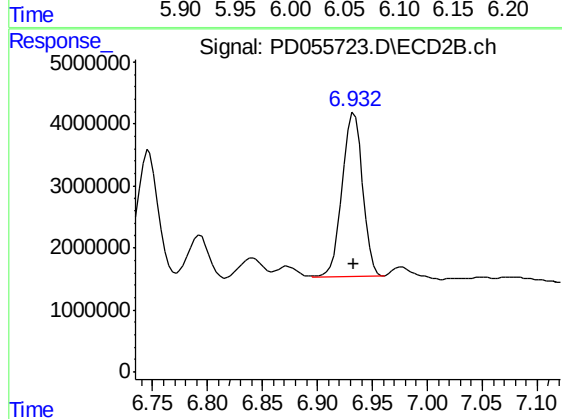

#27 Chlordane-5


R.T.: 6.933 min
Delta R.T.: 0.000 min
Response: 34113382
Conc: 742.24 ng/ml

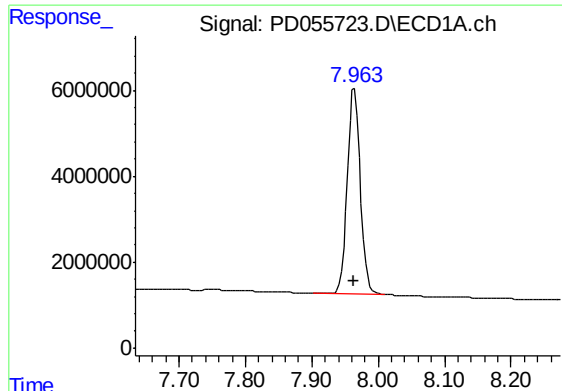

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 64852894
Conc: 71.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

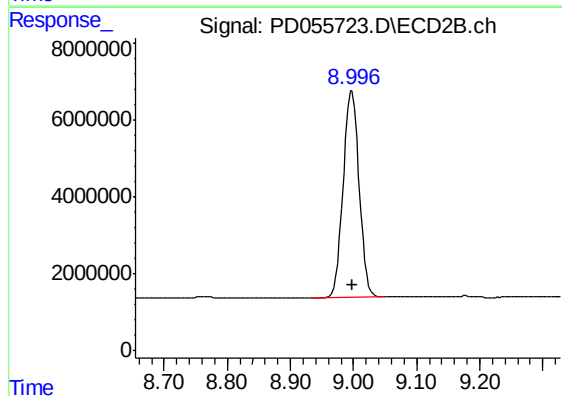

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.000 min
Response: 93539965
Conc: 71.07 ng/ml