

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
 Data File : PD055733.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 01:43
 Operator : SG\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD110119CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 07:42:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:48:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.963	43709749	56470236	51.272	46.889
28)	SA Decachlor...	7.965	8.999	43540717	63295116	46.023	45.484
Target Compounds							
23)	Chlordane-1	4.131	4.951	12672700	22815094	488.659	491.640
24)	Chlordane-2	4.620	5.416	15618069	24390834	491.100m	464.324
25)	Chlordane-3	5.176	6.059	45478142	106.1E6	472.912	484.530
26)	Chlordane-4	5.232	6.133	39710757	126.3E6	472.199	480.299
27)	Chlordane-5	6.056	6.934	15170235	22923549	499.619	491.717



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
Data File : PD055733.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 01:43
Operator : SG\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD110119CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 07:42:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:48:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

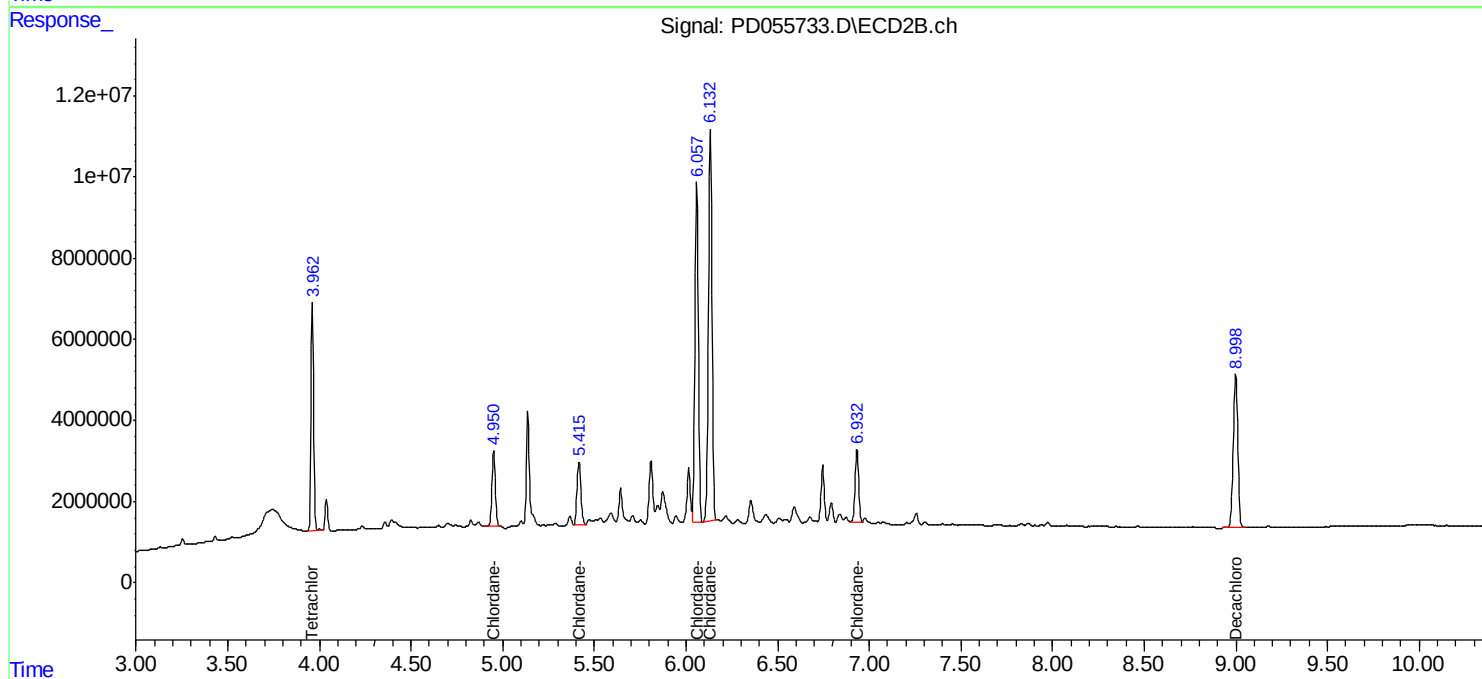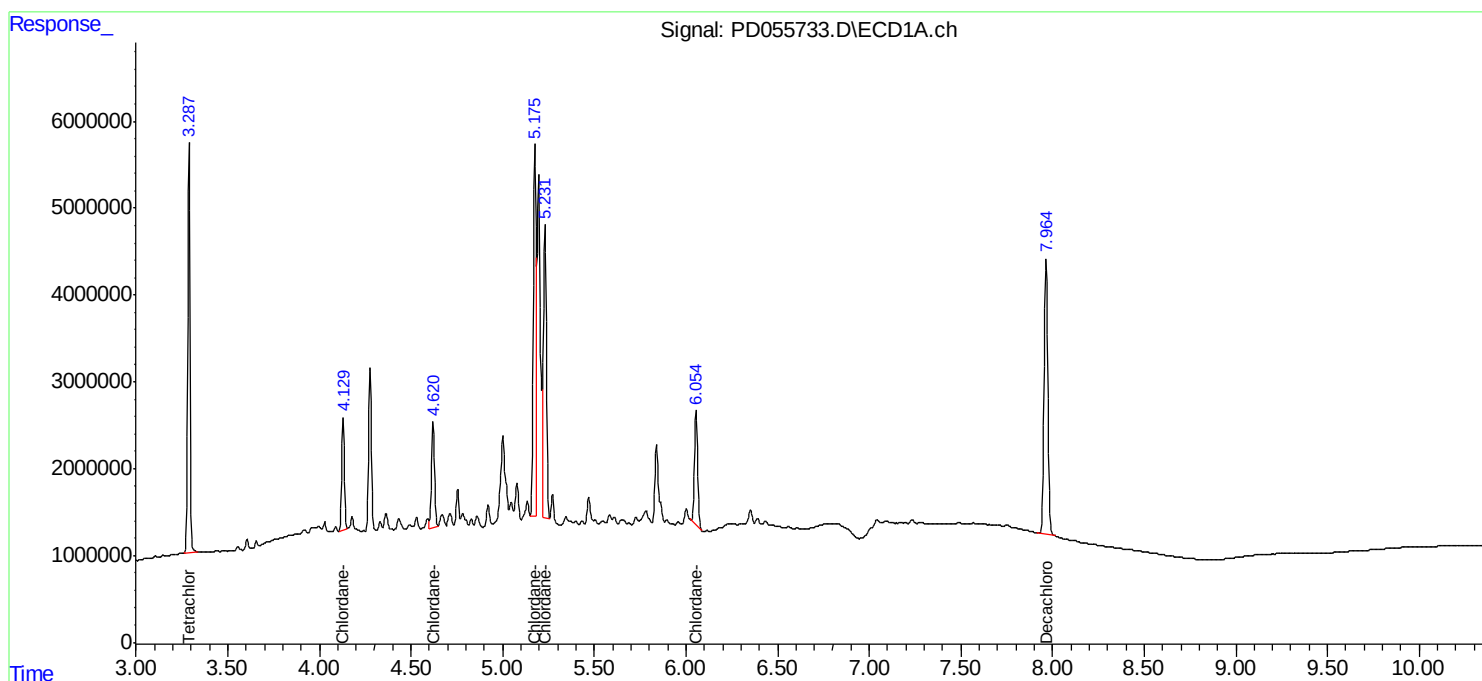


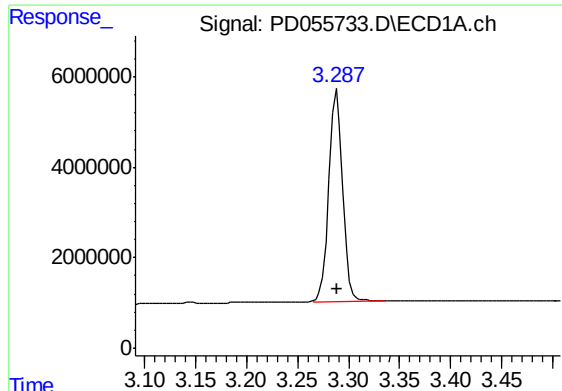

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 43709749
Conc: 51.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD110119CHLOR

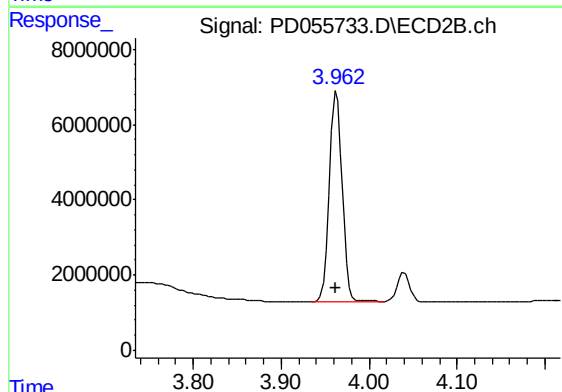


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 56470236
Conc: 46.89 ng/ml

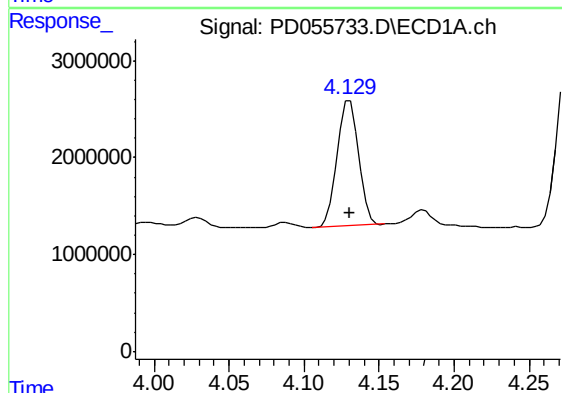


#23 Chlordane-1

R.T.: 4.131 min
Delta R.T.: 0.000 min
Response: 12672700
Conc: 488.66 ng/ml

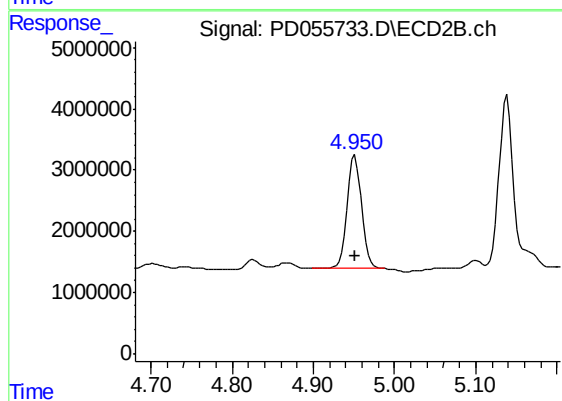

#23 Chlordane-1


R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 22815094
Conc: 491.64 ng/ml

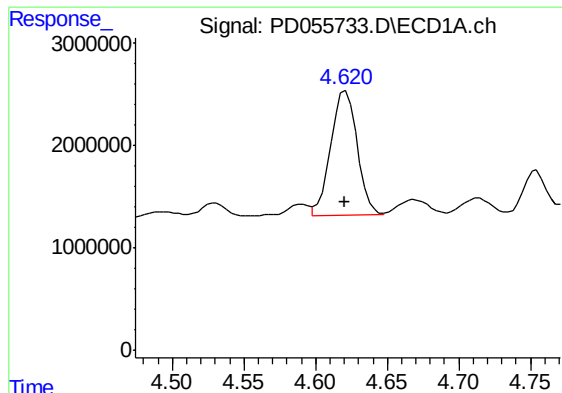

#24 Chlordane-2


R.T.: 4.620 min
Delta R.T.: 0.000 min
Response: 15618069
Conc: 491.10 ng/ml m

Instrument :
ECD_D
ClientSampleId :
ICVPD110119CHLOR

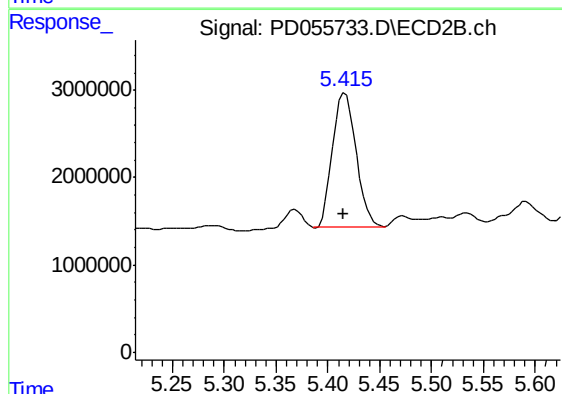


#24 Chlordane-2

R.T.: 5.416 min
Delta R.T.: 0.000 min
Response: 24390834
Conc: 464.32 ng/ml

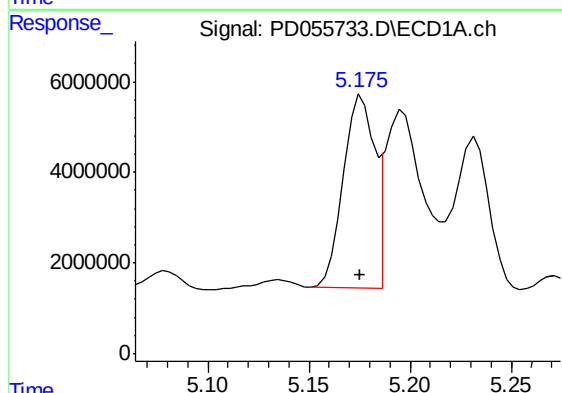


#25 Chlordane-3

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 45478142
Conc: 472.91 ng/ml

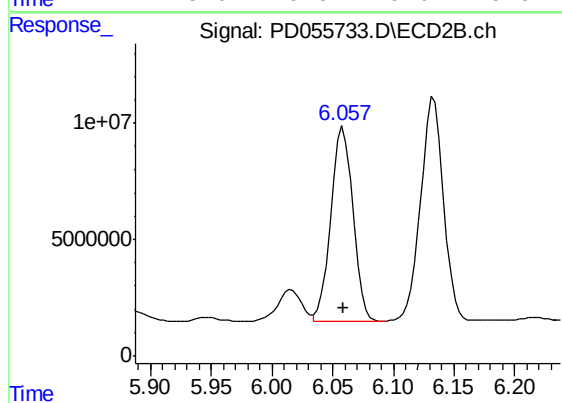

#25 Chlordane-3


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 106102272
Conc: 484.53 ng/ml

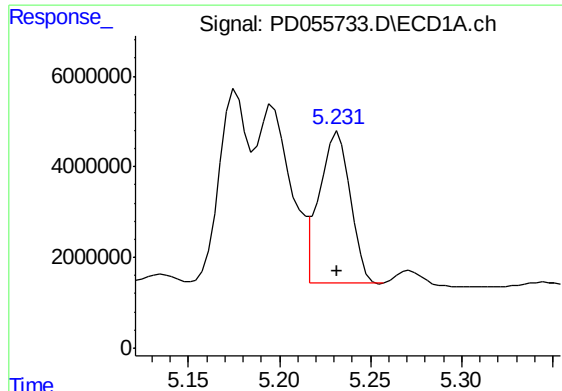

#26 Chlordane-4


R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 39710757
Conc: 472.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD110119CHLOR

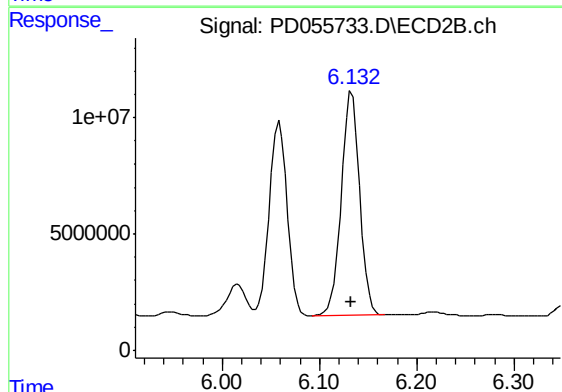


#26 Chlordane-4

R.T.: 6.133 min
Delta R.T.: 0.000 min
Response: 126342209
Conc: 480.30 ng/ml

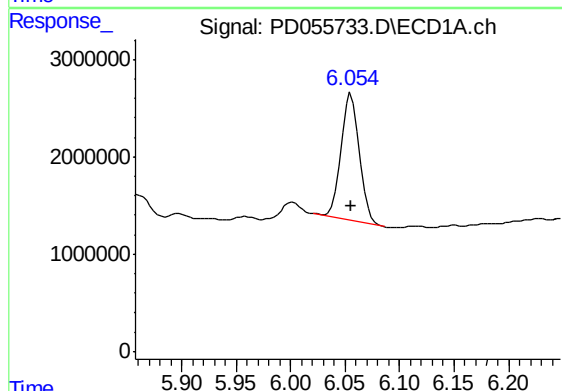


#27 Chlordane-5

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 15170235
Conc: 499.62 ng/ml

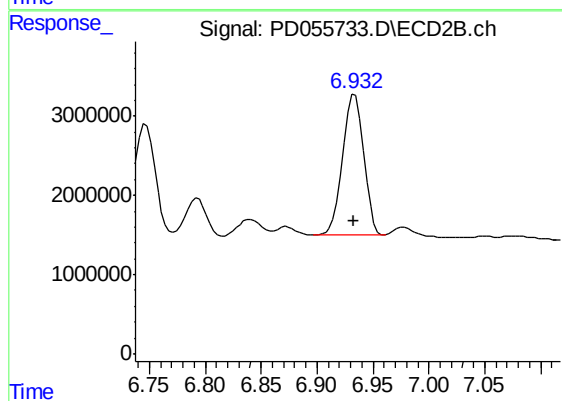

#27 Chlordane-5


R.T.: 6.934 min
Delta R.T.: 0.000 min
Response: 22923549
Conc: 491.72 ng/ml

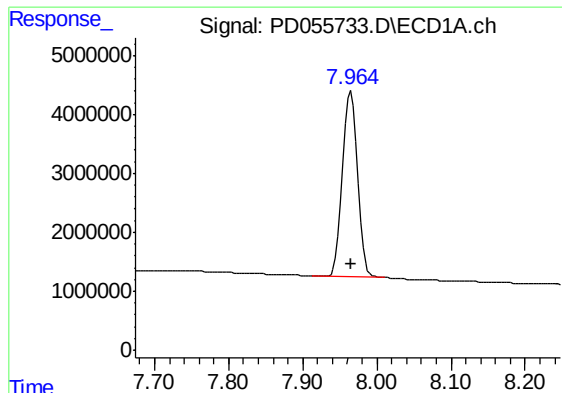

#28 Decachlorobiphenyl

R.T.: 7.965 min
Delta R.T.: 0.000 min
Response: 43540717
Conc: 46.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD110119CHLOR

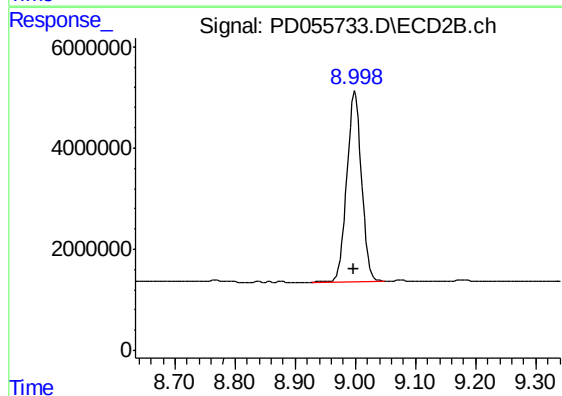

#28 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: 0.002 min
Response: 63295116
Conc: 45.48 ng/ml