

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
 Data File : PD055738.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 08:31
 Operator : SG\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 04:12:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:48:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.962	46422879	60093966	54.455	49.898
28)	SA Decachlor...	7.966	8.998	46372833	67593161	49.017	48.573
Target Compounds							
23)	Chlordane-1	4.131	4.951	13644749	23889960	526.141	514.802
24)	Chlordane-2	4.622	5.415	16404582	26447556	515.831	503.477
25)	Chlordane-3	5.177	6.059	49719371	114.1E6	517.015	521.214
26)	Chlordane-4	5.234	6.133	44534888	137.2E6	529.563	521.556
27)	Chlordane-5	6.057	6.934	15851414	27935071	522.053	599.216



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
Data File : PD055738.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 08:31
Operator : SG\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 04:12:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:48:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

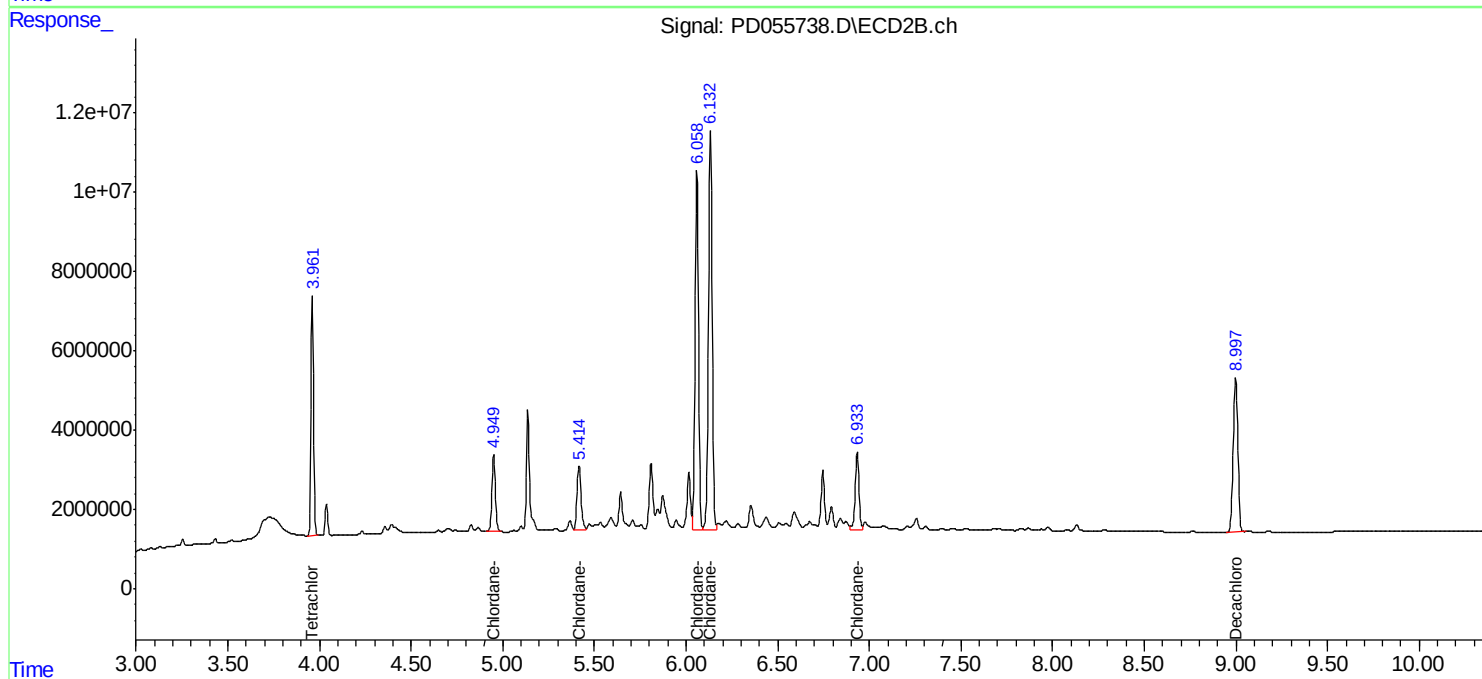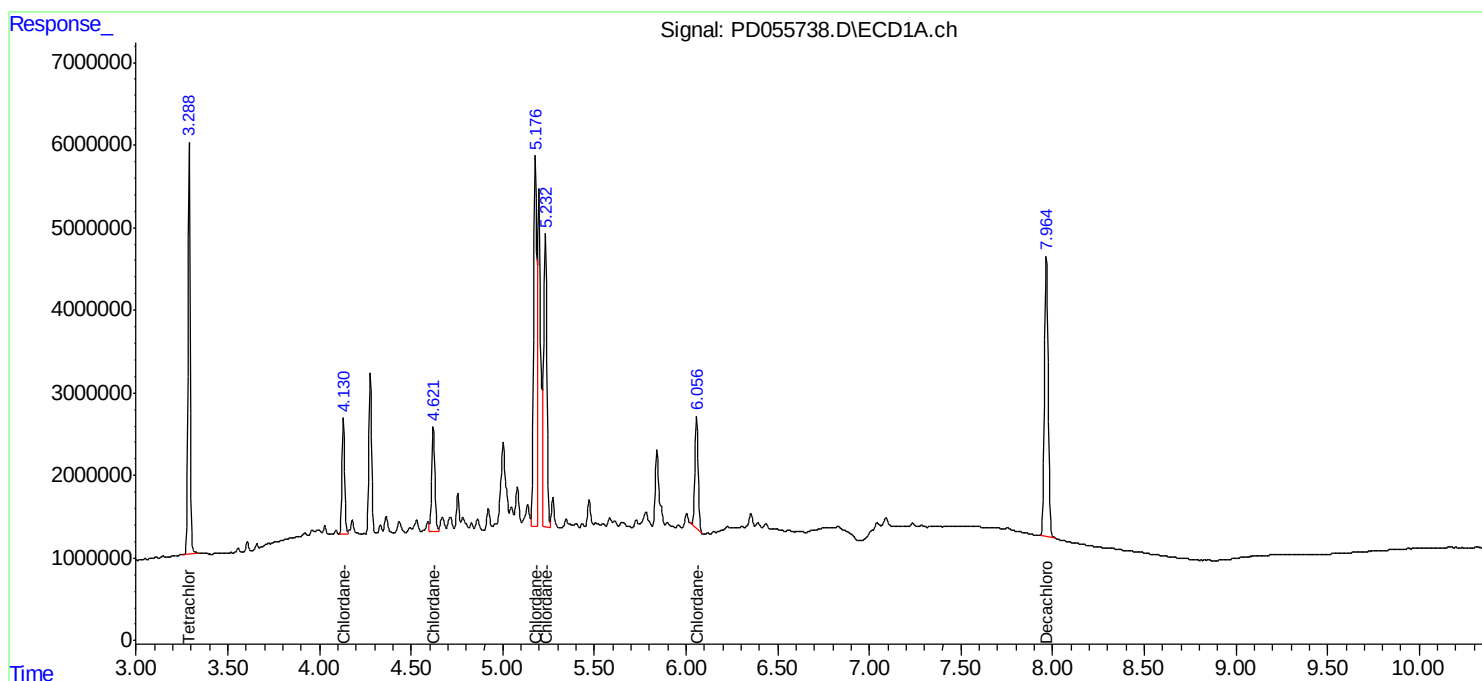


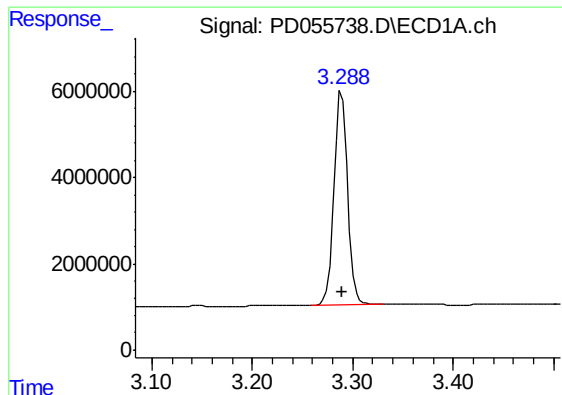

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 46422879
Conc: 54.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

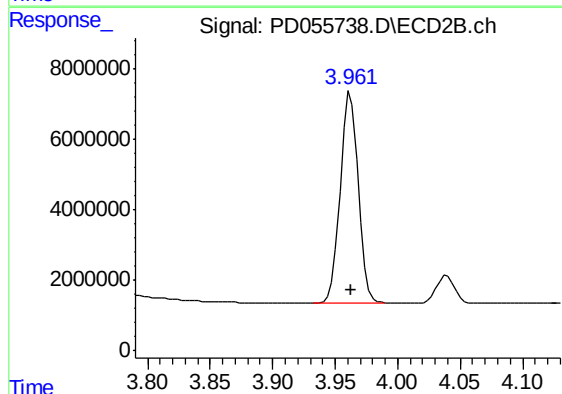


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 60093966
Conc: 49.90 ng/ml

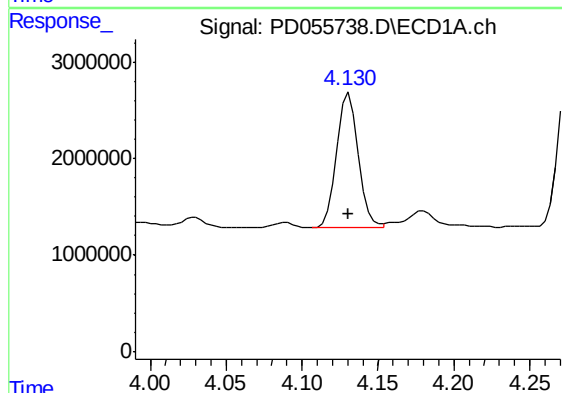


#23 Chlordane-1

R.T.: 4.131 min
Delta R.T.: 0.000 min
Response: 13644749
Conc: 526.14 ng/ml

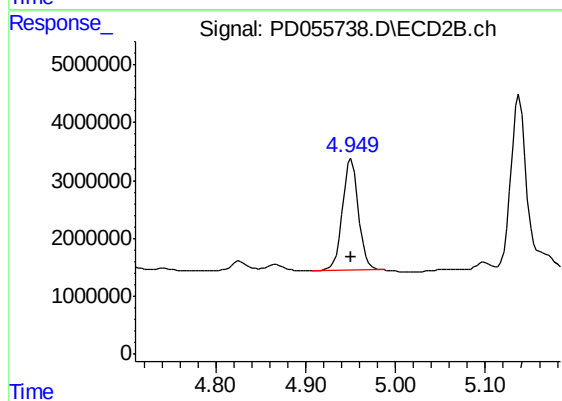

#23 Chlordane-1


R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 23889960
Conc: 514.80 ng/ml

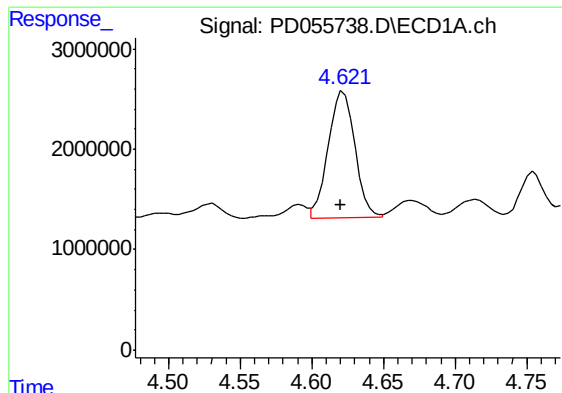

#24 Chlordane-2


R.T.: 4.622 min
Delta R.T.: 0.002 min
Response: 16404582
Conc: 515.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

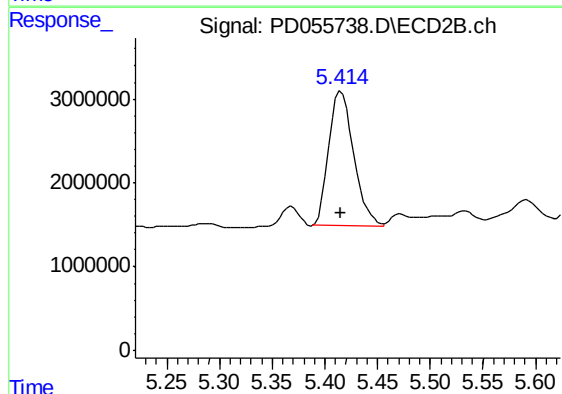


#24 Chlordane-2

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 26447556
Conc: 503.48 ng/ml

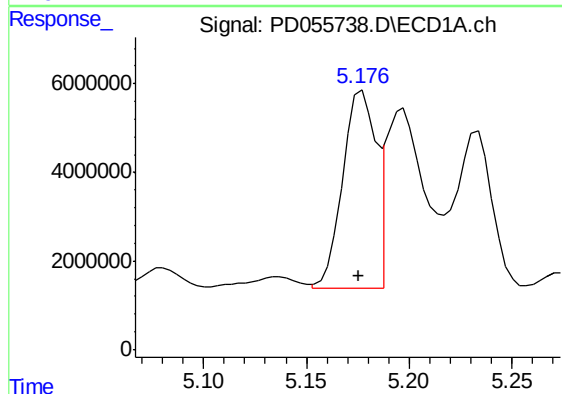


#25 Chlordane-3

R.T.: 5.177 min
Delta R.T.: 0.002 min
Response: 49719371
Conc: 517.01 ng/ml

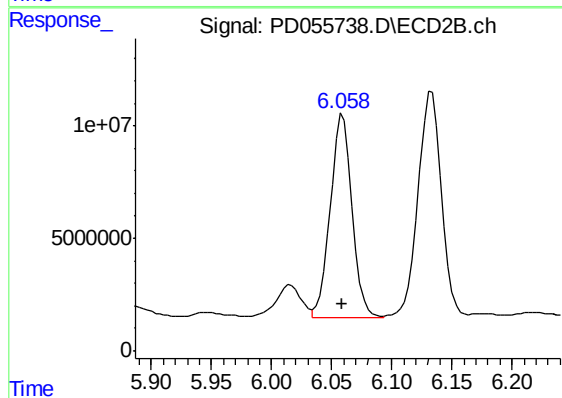

#25 Chlordane-3


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 114135297
Conc: 521.21 ng/ml

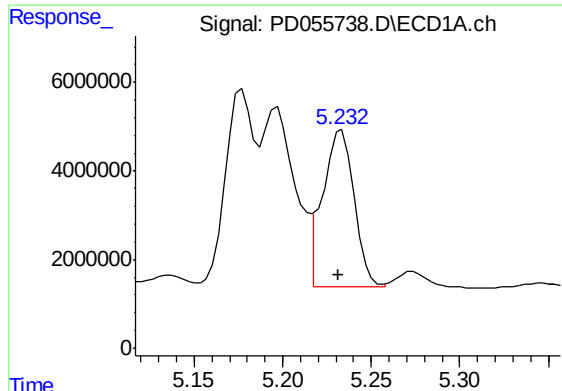

#26 Chlordane-4


R.T.: 5.234 min
Delta R.T.: 0.002 min
Response: 44534888
Conc: 529.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

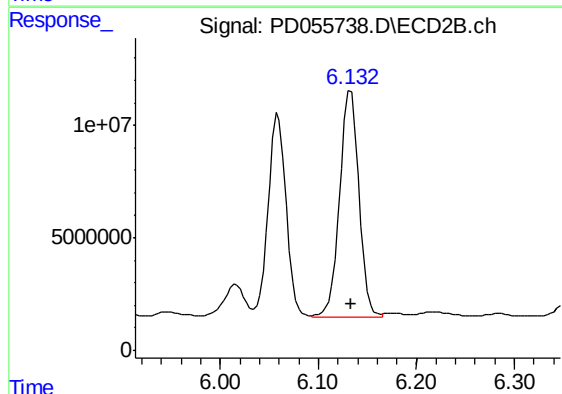


#26 Chlordane-4

R.T.: 6.133 min
Delta R.T.: 0.000 min
Response: 137194833
Conc: 521.56 ng/ml

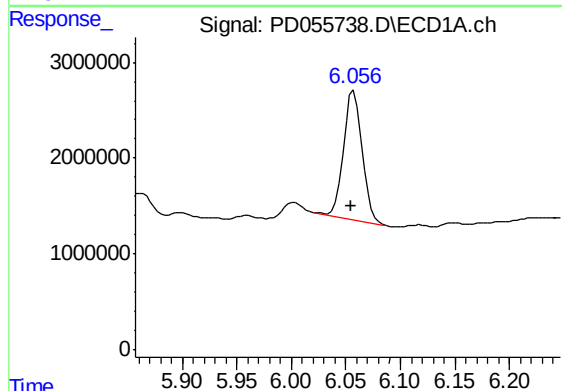


#27 Chlordane-5

R.T.: 6.057 min
Delta R.T.: 0.002 min
Response: 15851414
Conc: 522.05 ng/ml

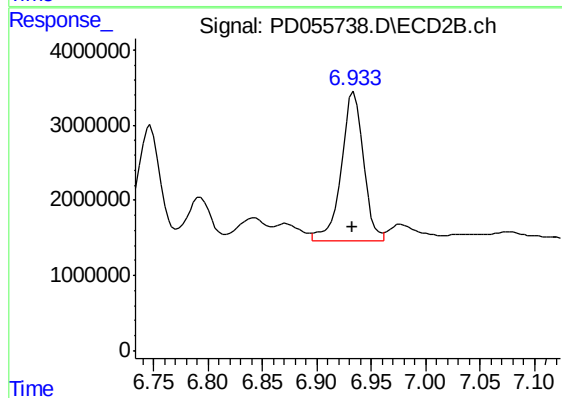

#27 Chlordane-5


R.T.: 6.934 min
Delta R.T.: 0.002 min
Response: 27935071
Conc: 599.22 ng/ml

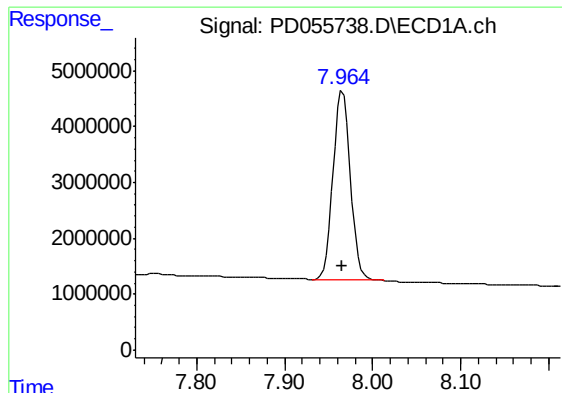

#28 Decachlorobiphenyl

R.T.: 7.966 min
Delta R.T.: 0.000 min
Response: 46372833
Conc: 49.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

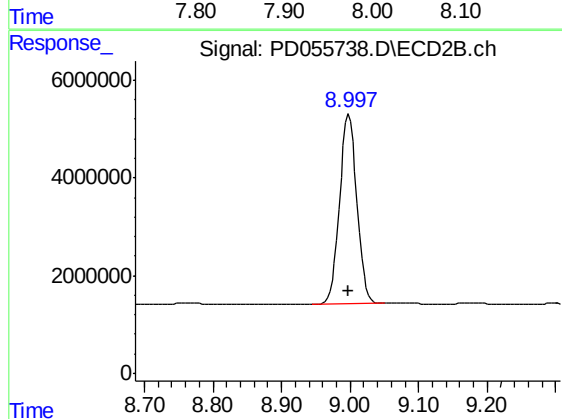

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.001 min
Response: 67593161
Conc: 48.57 ng/ml