

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
 Data File : PD055751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 11:41
 Operator : SG\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 04:03:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:48:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.963	44927272	58900005	52.700	48.907
28)	SA Decachlor...	7.965	8.997	45352592	64994996	47.939	46.706m
Target Compounds							
23)	Chlordane-1	4.131	4.951	13350928	23046080	514.811	496.617
24)	Chlordane-2	4.622	5.416	15965540	25698184	502.026	489.212
25)	Chlordane-3	5.177	6.059	47419783	111.0E6	493.102	506.696
26)	Chlordane-4	5.233	6.134	41924505	133.1E6	498.523	506.129
27)	Chlordane-5	6.056	6.934	15402723	27514328	507.276	590.191



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
Data File : PD055751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 11:41
Operator : SG\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 04:03:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:48:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

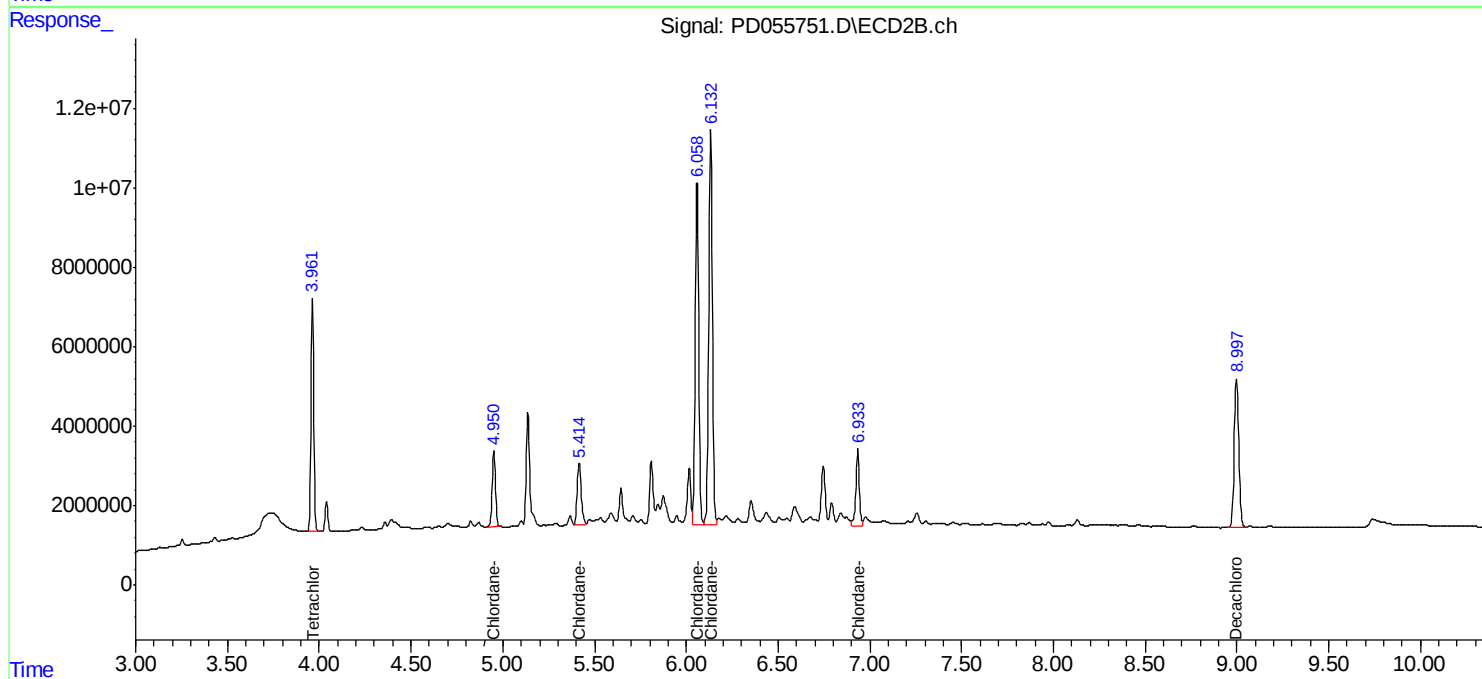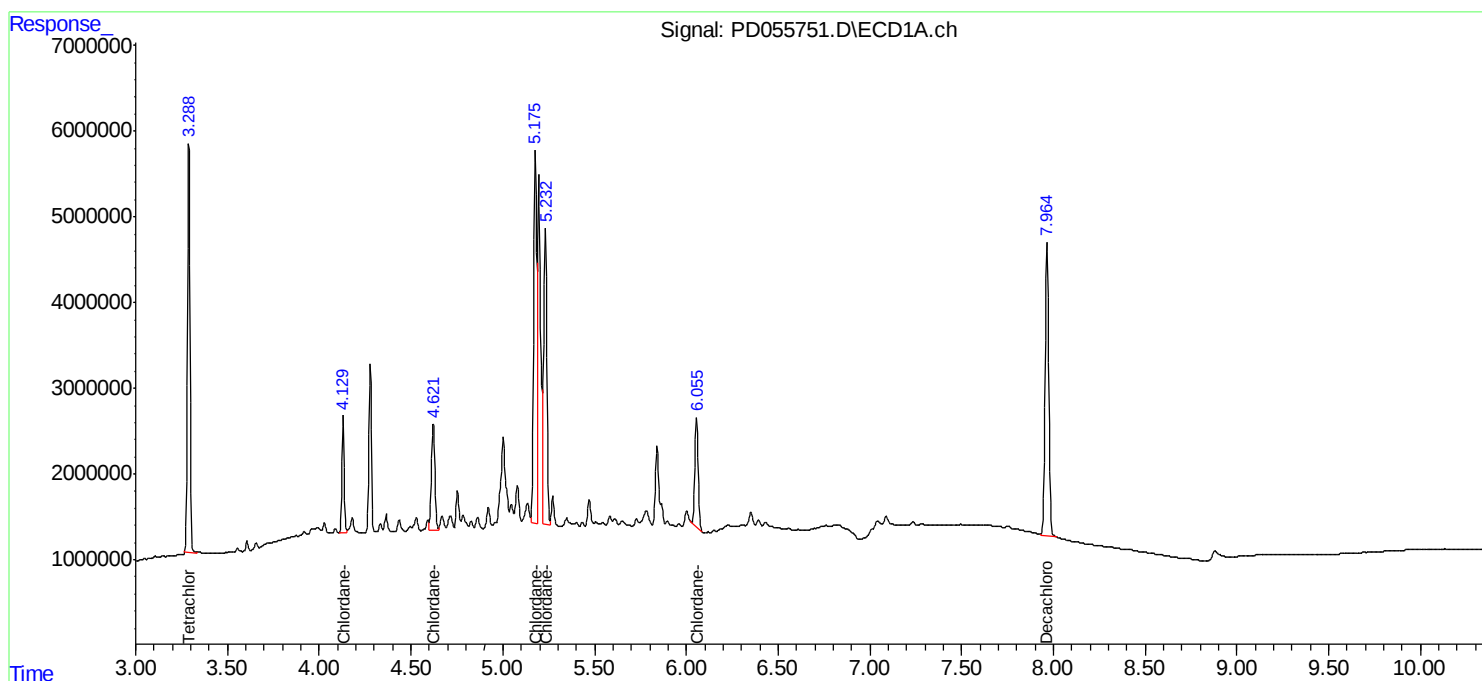


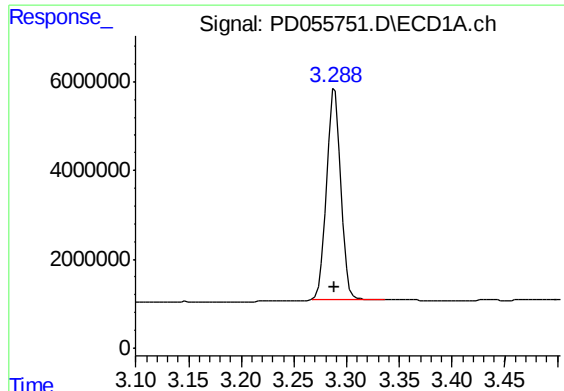

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 44927272
Conc: 52.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

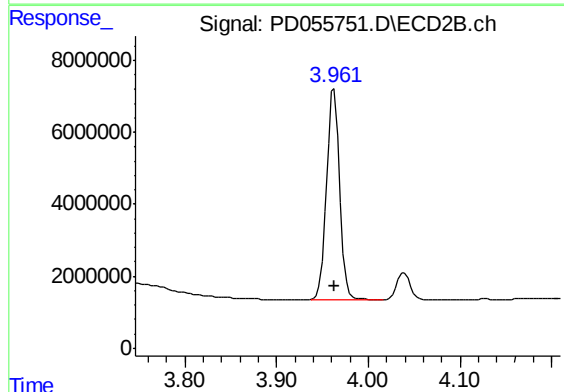


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 58900005
Conc: 48.91 ng/ml

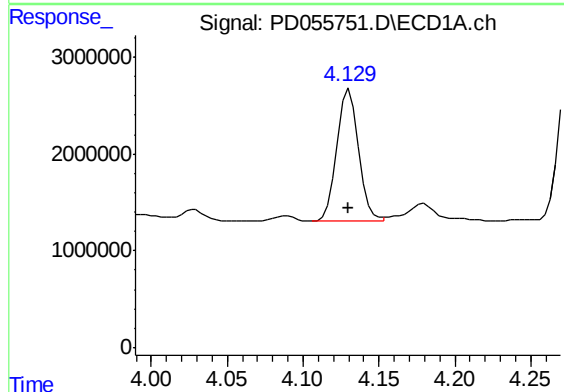


#23 Chlordane-1

R.T.: 4.131 min
Delta R.T.: 0.000 min
Response: 13350928
Conc: 514.81 ng/ml

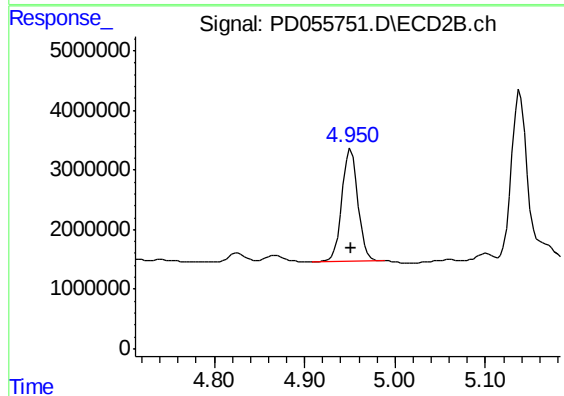

#23 Chlordane-1


R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 23046080
Conc: 496.62 ng/ml

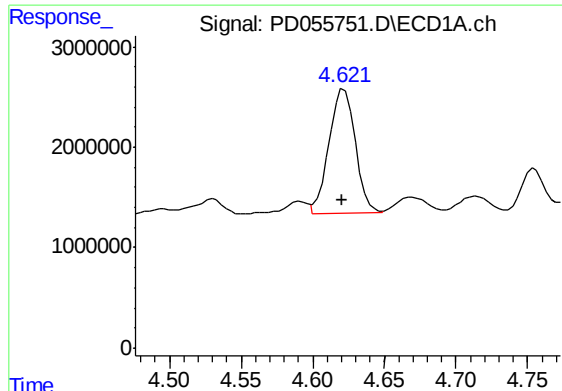

#24 Chlordane-2


R.T.: 4.622 min
Delta R.T.: 0.001 min
Response: 15965540
Conc: 502.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

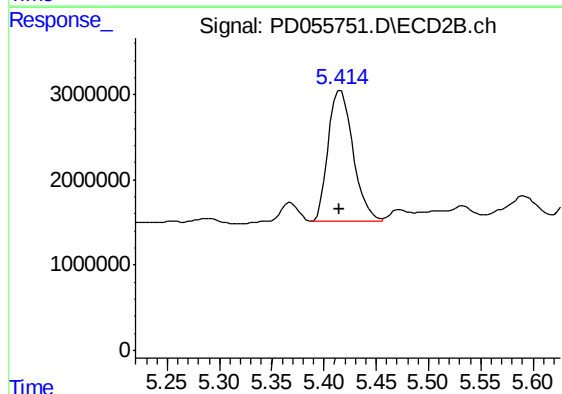


#24 Chlordane-2

R.T.: 5.416 min
Delta R.T.: 0.000 min
Response: 25698184
Conc: 489.21 ng/ml

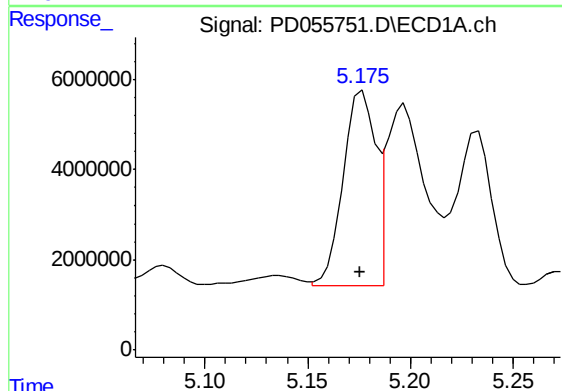


#25 Chlordane-3

R.T.: 5.177 min
Delta R.T.: 0.001 min
Response: 47419783
Conc: 493.10 ng/ml

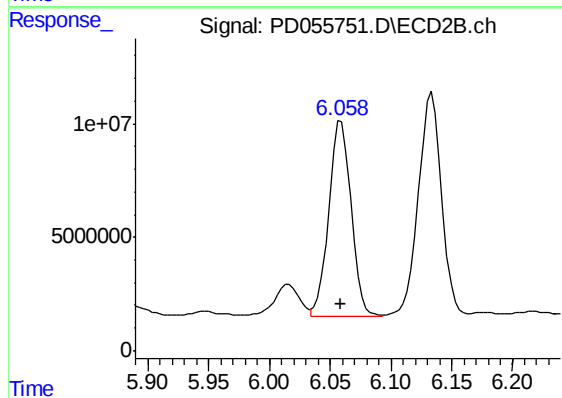

#25 Chlordane-3


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 110956126
Conc: 506.70 ng/ml

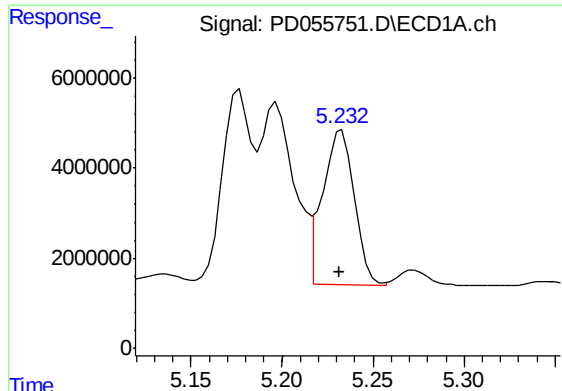

#26 Chlordane-4


R.T.: 5.233 min
Delta R.T.: 0.001 min
Response: 41924505
Conc: 498.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

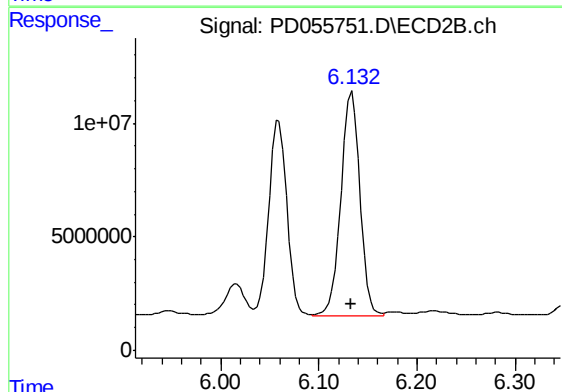


#26 Chlordane-4

R.T.: 6.134 min
Delta R.T.: 0.000 min
Response: 133136617
Conc: 506.13 ng/ml

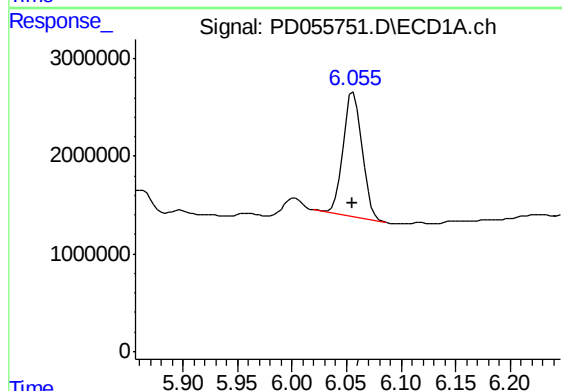


#27 Chlordane-5

R.T.: 6.056 min
Delta R.T.: 0.001 min
Response: 15402723
Conc: 507.28 ng/ml

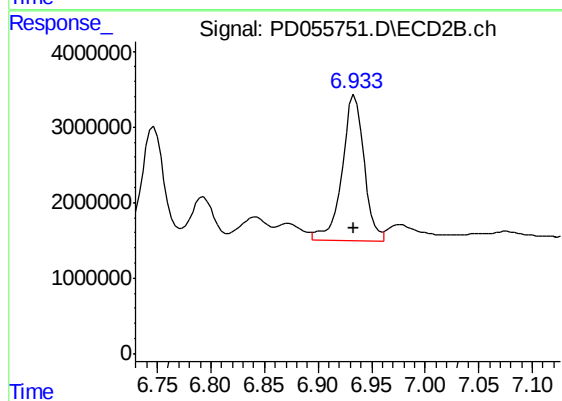

#27 Chlordane-5


R.T.: 6.934 min
Delta R.T.: 0.002 min
Response: 27514328
Conc: 590.19 ng/ml

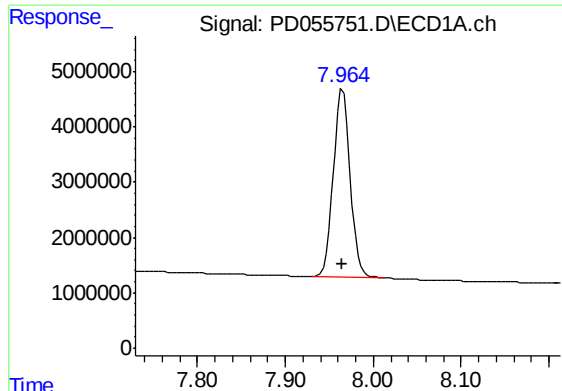

#28 Decachlorobiphenyl

R.T.: 7.965 min
Delta R.T.: 0.000 min
Response: 45352592
Conc: 47.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

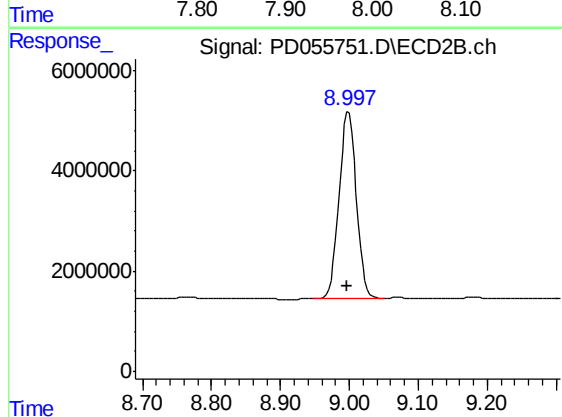

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 64994996
Conc: 46.71 ng/ml m