

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
 Data File : PD055780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 19:50
 Operator : SG\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 04:41:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:48:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.963	45056138	58646012	52.851	48.696
28)	SA Decachlor...	7.968	9.001	44169567	63484180	46.688	45.620
Target Compounds							
23)	Chlordane-1	4.131	4.951	12826733	23059055	494.598	496.897
24)	Chlordane-2	4.622	5.416	15335833	25031863	482.225	476.527
25)	Chlordane-3	5.178	6.060	46297548	108.0E6	481.432	493.424
26)	Chlordane-4	5.233	6.134	40575543	128.0E6	482.482	486.468
27)	Chlordane-5	6.057	6.935	15563940	22765491	512.585	488.327



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110119\
Data File : PD055780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 19:50
Operator : SG\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 04:41:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:48:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

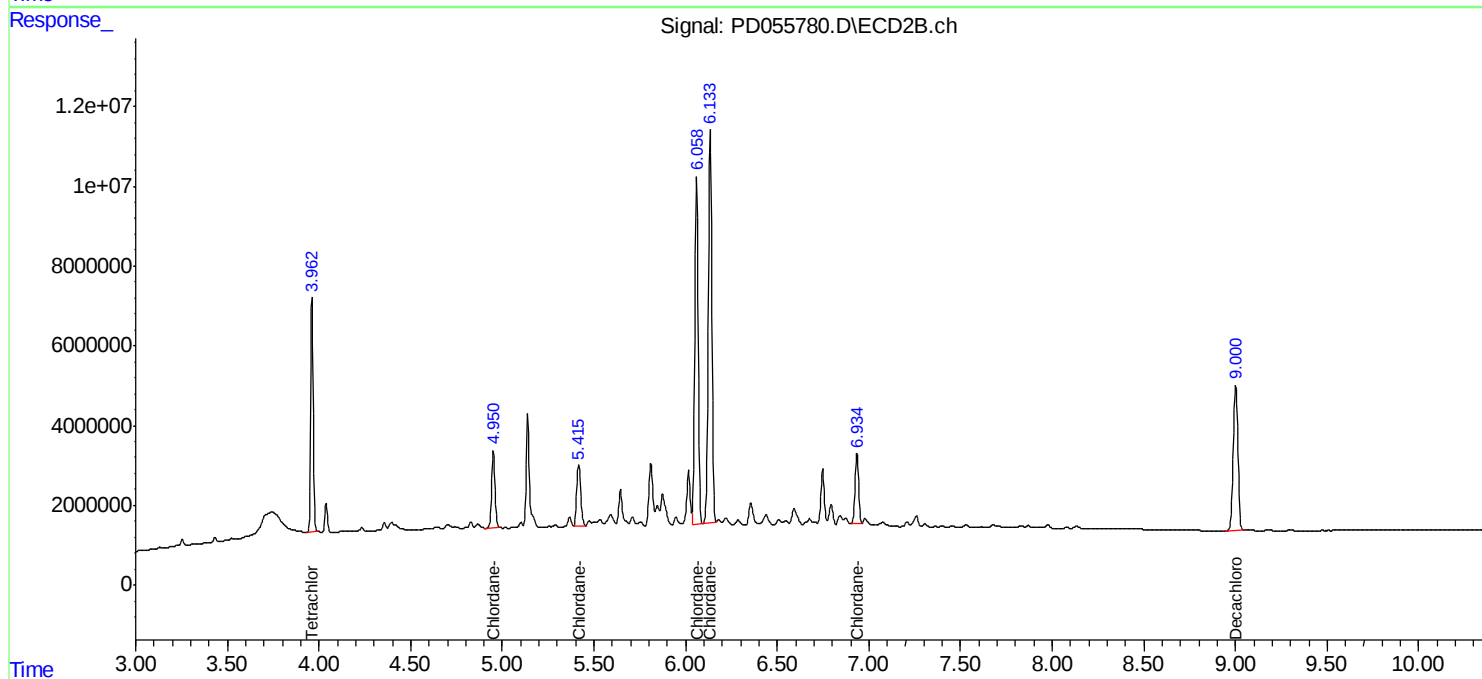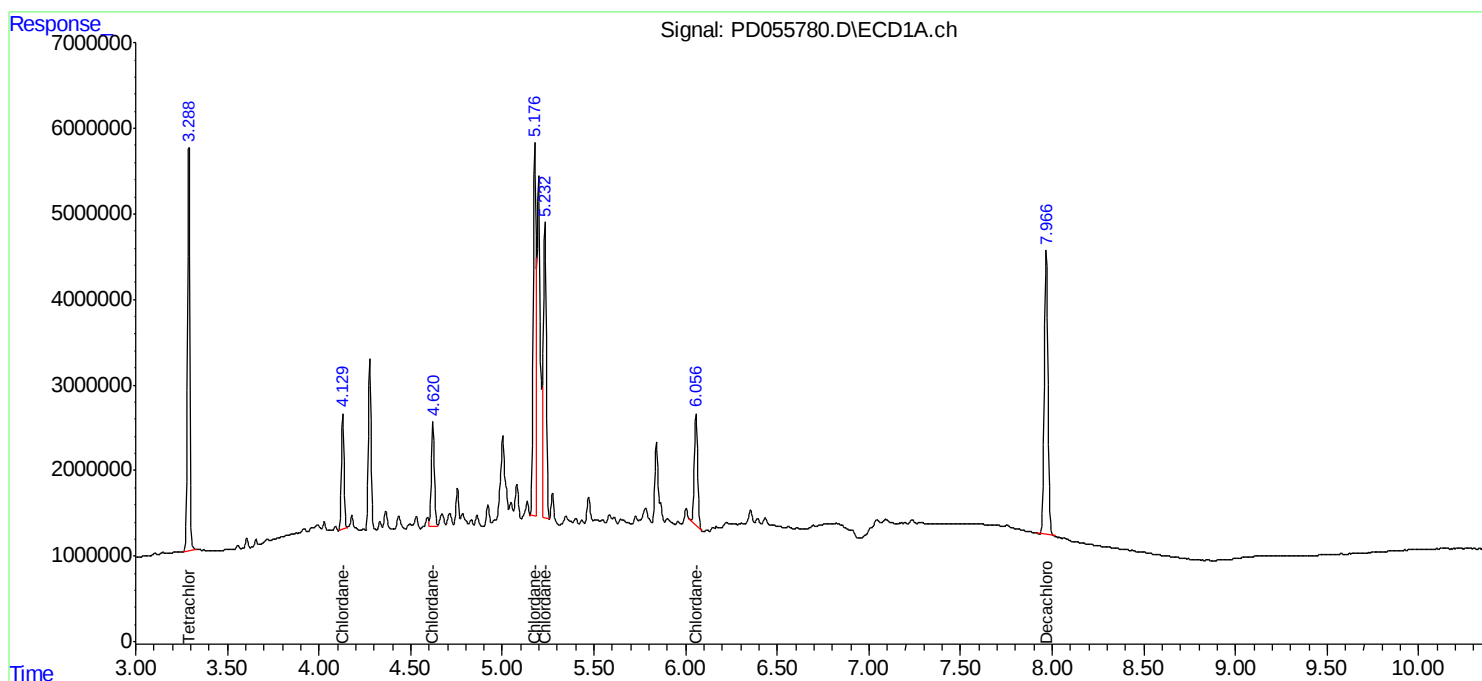


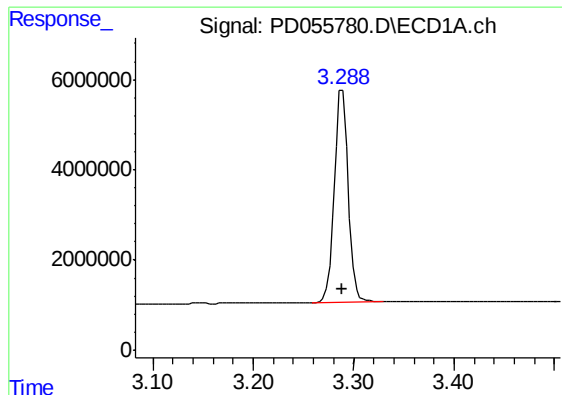

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 45056138
Conc: 52.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

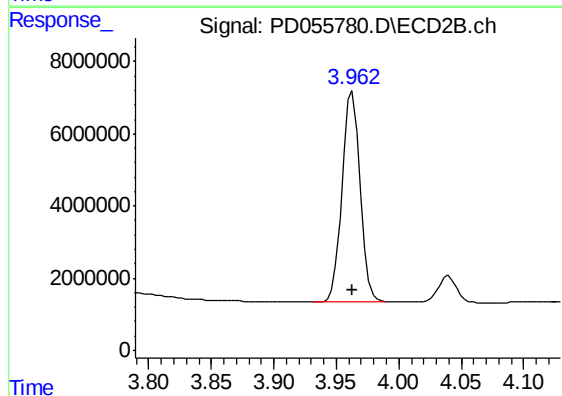


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 58646012
Conc: 48.70 ng/ml

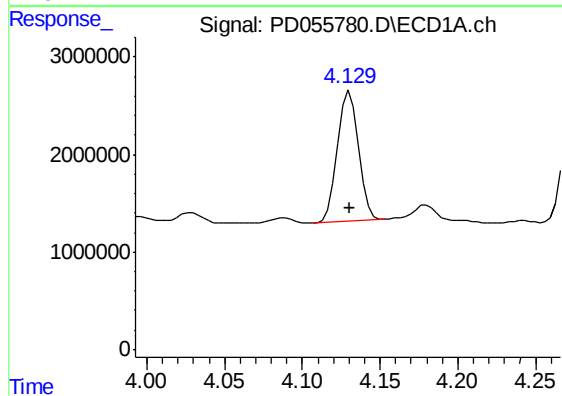


#23 Chlordane-1

R.T.: 4.131 min
Delta R.T.: 0.000 min
Response: 12826733
Conc: 494.60 ng/ml

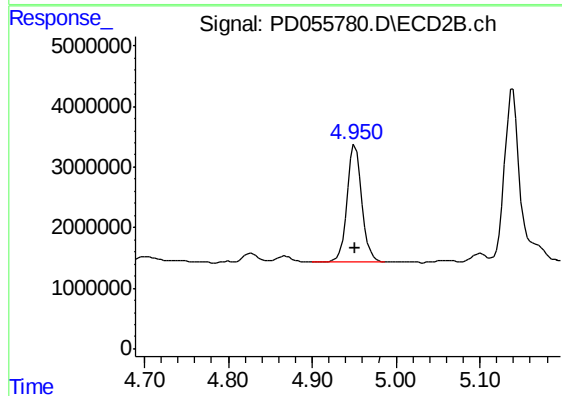

#23 Chlordane-1


R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 23059055
Conc: 496.90 ng/ml

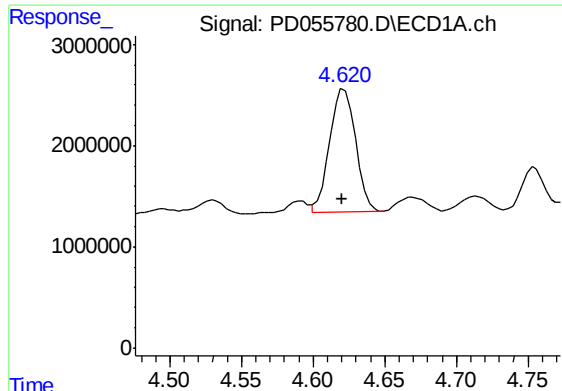

#24 Chlordane-2


R.T.: 4.622 min
Delta R.T.: 0.001 min
Response: 15335833
Conc: 482.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

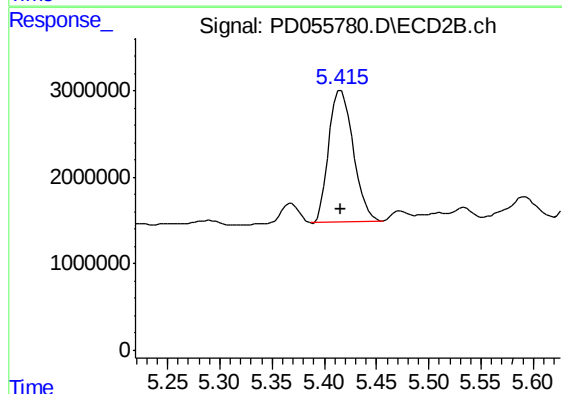


#24 Chlordane-2

R.T.: 5.416 min
Delta R.T.: 0.000 min
Response: 25031863
Conc: 476.53 ng/ml

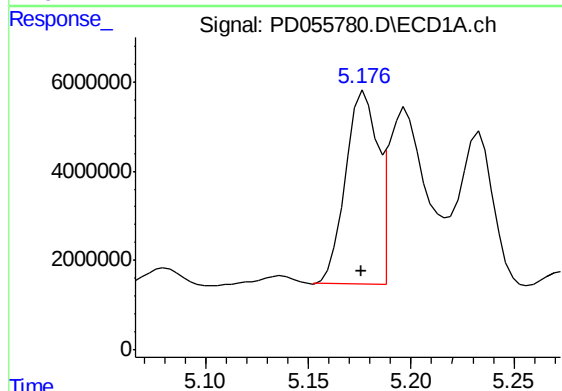


#25 Chlordane-3

R.T.: 5.178 min
Delta R.T.: 0.002 min
Response: 46297548
Conc: 481.43 ng/ml

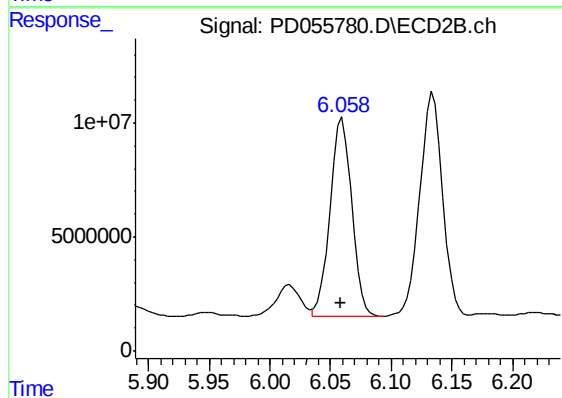

#25 Chlordane-3


R.T.: 6.060 min
Delta R.T.: 0.001 min
Response: 108049852
Conc: 493.42 ng/ml

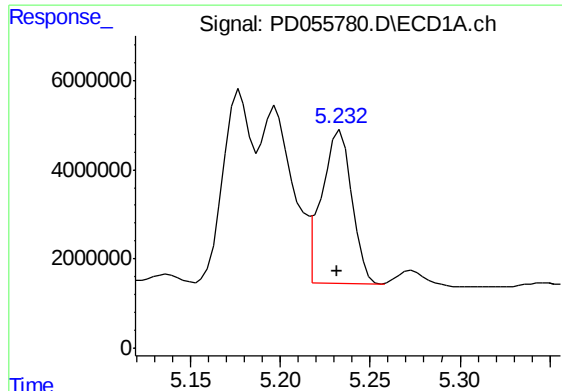

#26 Chlordane-4


R.T.: 5.233 min
Delta R.T.: 0.002 min
Response: 40575543
Conc: 482.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

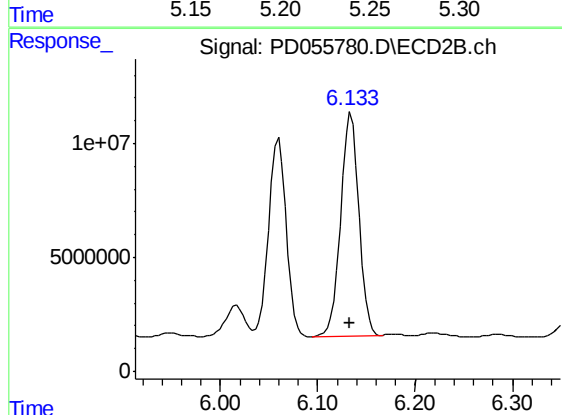


#26 Chlordane-4

R.T.: 6.134 min
Delta R.T.: 0.001 min
Response: 127964803
Conc: 486.47 ng/ml

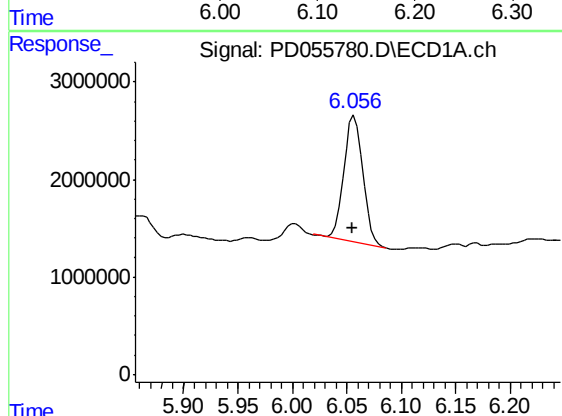


#27 Chlordane-5

R.T.: 6.057 min
Delta R.T.: 0.002 min
Response: 15563940
Conc: 512.59 ng/ml

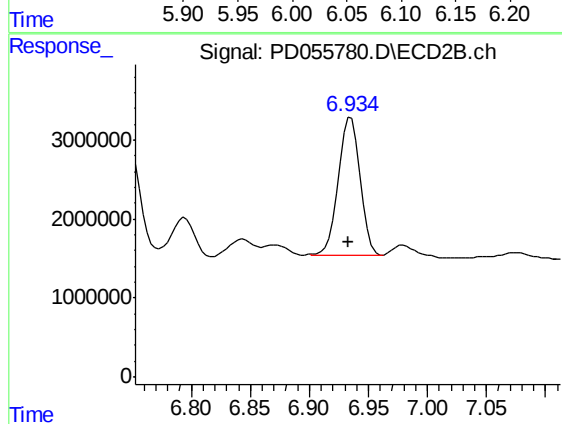

#27 Chlordane-5


R.T.: 6.935 min
Delta R.T.: 0.003 min
Response: 22765491
Conc: 488.33 ng/ml

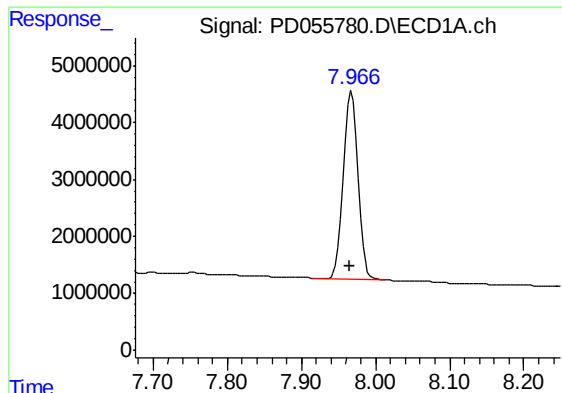

#28 Decachlorobiphenyl

R.T.: 7.968 min
Delta R.T.: 0.003 min
Response: 44169567
Conc: 46.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

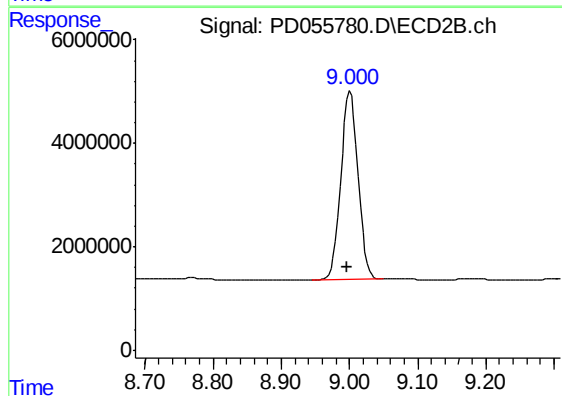

#28 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: 0.004 min
Response: 63484180
Conc: 45.62 ng/ml