

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110122\
 Data File : PD072755.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2022 18:50
 Operator : AR\AJ
 Sample : N5321-21MS
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBWU9MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/02/2022
 Supervised By :Ankita Jodhani 11/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 22:45:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.704	3.466	40165419	894.9E6	17.276	22.331 #
27)	SA Decachlor...	7.835	8.918	67858008	345.8E6	34.570	36.776
Target Compounds							
2)	A alpha-BHC	3.208	3.930	153.1E6	1996.3E6	43.832	37.632
3)	MA gamma-BHC...	3.538	4.263	146.7E6	1704.4E6	46.272	40.107
4)	MA Heptachlor	3.871	4.830	140.1E6	1137.1E6	43.178	38.243
5)	MB Aldrin	4.149	5.168	149.1E6	990.6E6	47.058	39.526
6)	B beta-BHC	3.840	4.478	67486770	712.3E6	44.419	41.986
7)	B delta-BHC	4.069	4.722	18261175	207.6E6	5.448	6.072
8)	B Heptachlo...	4.654	5.601	131.9E6	858.5E6	46.371	41.521
9)	A Endosulfan I	5.024	5.985	123.4E6	782.8E6	48.661	45.181
10)	B trans-Chl...	4.903	5.854	131.5E6	829.0E6	44.790	41.396
11)	B cis-Chlor...	4.966	5.929	127.7E6	818.8E6	44.715	42.009
12)	B 4,4'-DDE	5.155	6.103	266.0E6	1615.7E6	97.716	90.478
13)	MA Dieldrin	5.290	6.262	283.6E6	1735.8E6	102.934	97.415
14)	MA Endrin	5.567	6.493	239.8E6	1364.1E6	98.936	93.247
15)	B Endosulfa...	5.865	6.723	234.4E6	1407.1E6	99.651	98.497
16)	A 4,4'-DDD	5.713	6.627	211.4E6	1272.1E6	99.297	94.257
17)	MA 4,4'-DDT	5.962	6.935	209.8E6	1306.5E6	96.820	96.661
18)	B Endrin al...	6.047	6.854	174.3E6	1039.0E6	88.509	86.704
19)	B Endosulfa...	6.270	7.087	154.5E6	880.1E6	67.480	66.869
20)	A Methoxychlor	6.546	7.414	565.4E6	2888.1E6	487.066	477.475
21)	B Endrin ke...	6.780	7.575	274.0E6	1473.6E6	102.728	102.874m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110122\
Data File : PD072755.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2022 18:50
Operator : AR\AJ
Sample : N5321-21MS
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 22:45:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

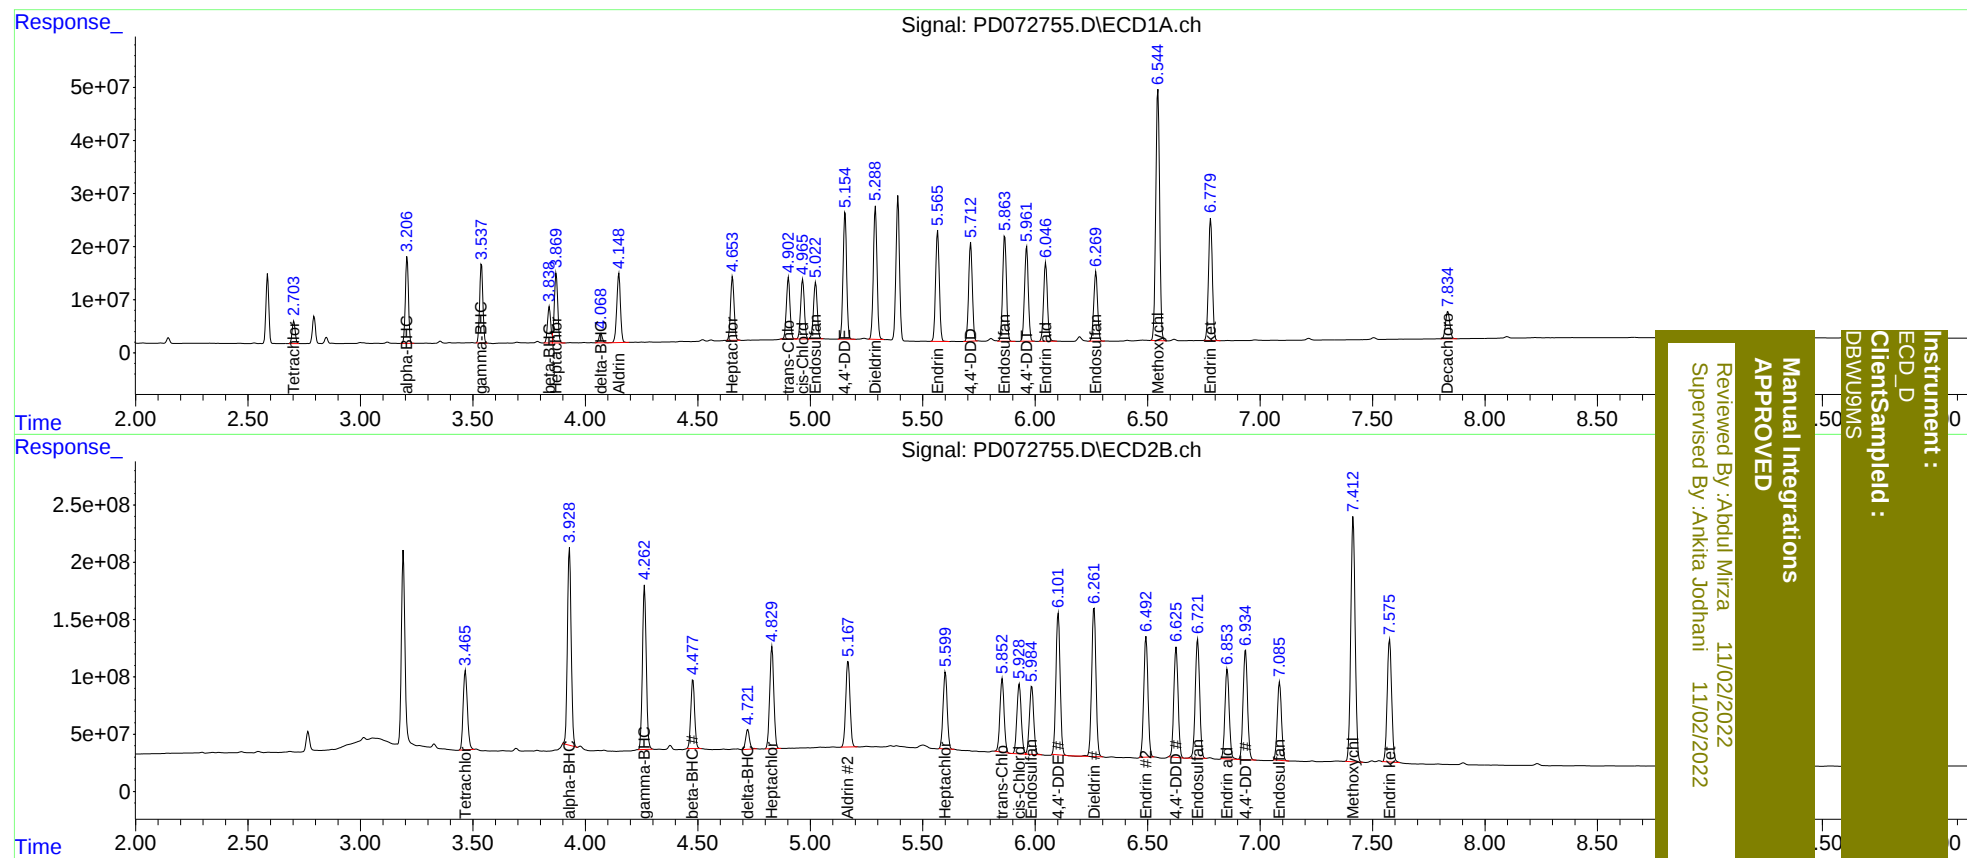

Reviewed By: Abdul Mirza 11/02/2022
Supervised By: Ankita Jodhani 11/02/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DBWU9MS