

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110122\
 Data File : PD072726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2022 11:20
 Operator : AR\AJ
 Sample : N5301-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBWU8

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/02/2022
 Supervised By :Ankita Jodhani 11/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 22:13:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.708	3.463	39309328	677.0E6	16.908	16.895
27)	SA Decachlor...	7.840	8.919	60415276	323.0E6	30.778	34.343
Target Compounds							
2)	A alpha-BHC	3.211	3.927	156.8E6	2169.8E6	44.894m	40.903m
6)	B beta-BHC	3.846	4.477	39771075	442.9E6	26.177	26.106
7)	B delta-BHC	4.074	4.720	10547660	129.3E6	3.147m	3.781
9)	A Endosulfan I	5.016	5.989	9988662	26382566	3.937	1.523 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110122\
Data File : PD072726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2022 11:20
Operator : AR\AJ
Sample : N5301-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 22:13:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

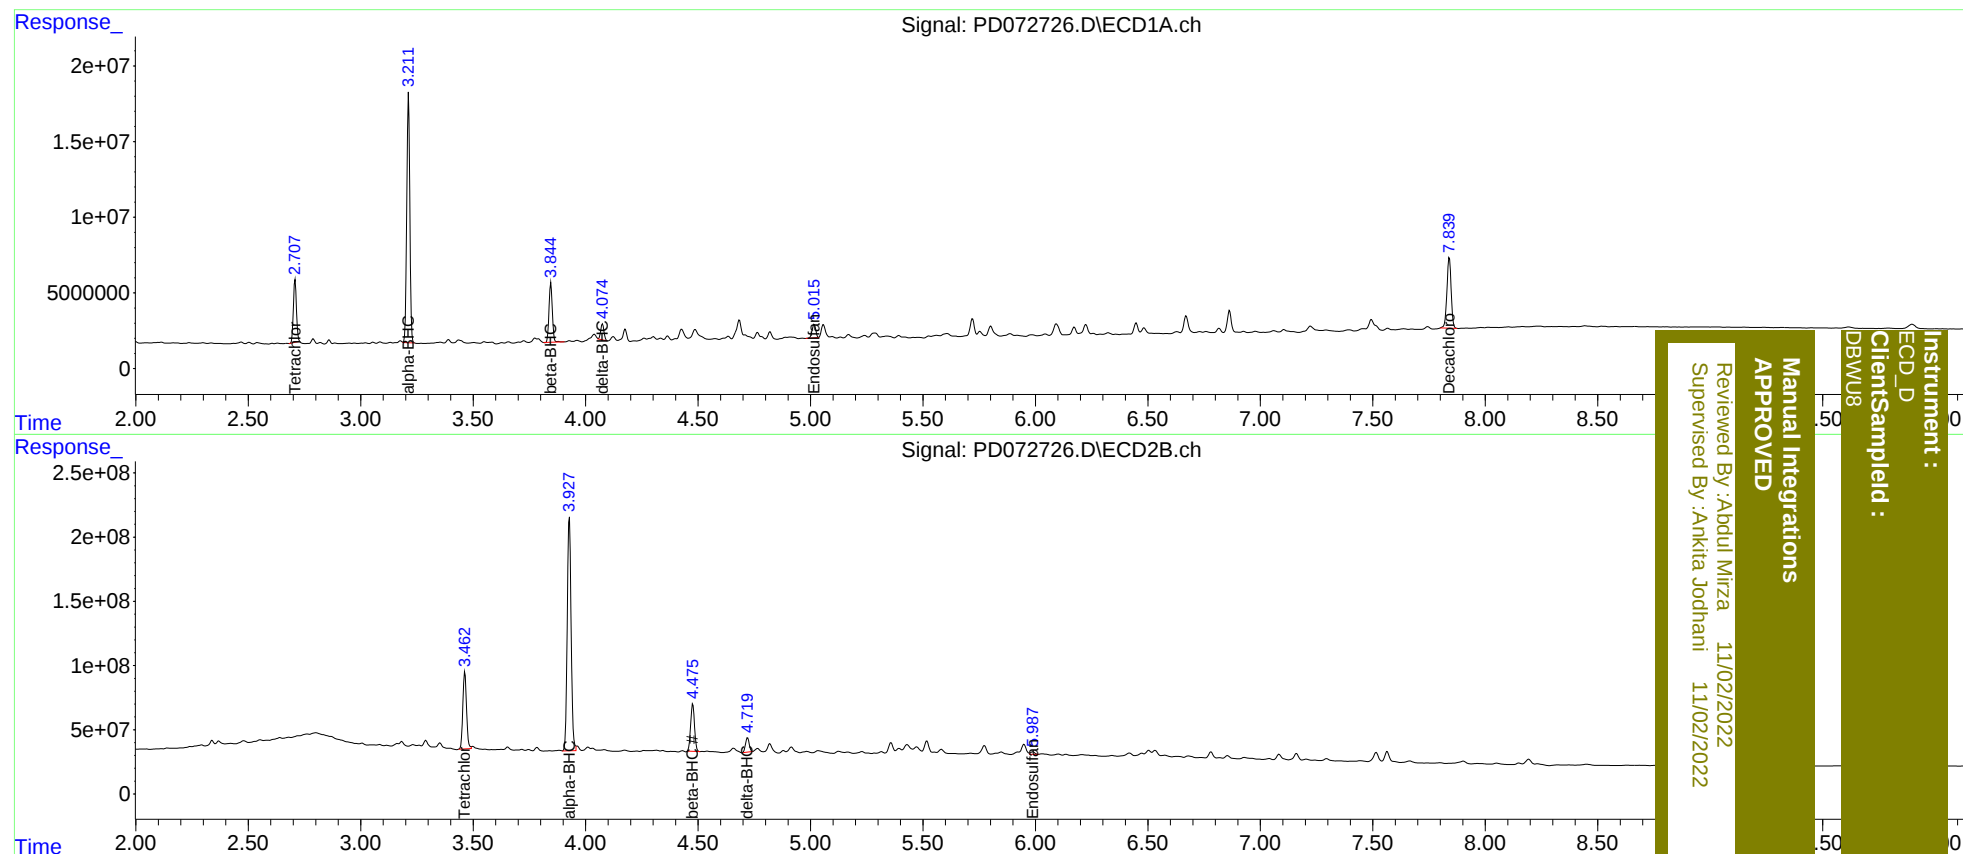

Instrument :
ECD_D
ClientSampled :
DBWU8

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/02/2022
Supervised By :Ankita Jodhani 11/02/2022