

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110123\
 Data File : PD079309.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2023 13:34
 Operator : AR\AJ
 Sample : 05139-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 22:18:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 17 09:38:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	0.000	2.774f	0	82661	N.D.	<MDL
Target Compounds						
3) MA gamma-BHC...	0.000	3.661	0	44420	N.D.	<MDL
14) MA Endrin	0.000	5.691	0	335851	N.D.	0.133
21) B Endrin ke...	0.000	6.839f	0	51917	N.D.	<MDL
23) Toxaphene-2	0.000	5.691f	0	335851	N.D.	20.442


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110123\
Data File : PD079309.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2023 13:34
Operator : AR\AJ
Sample : 05139-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 22:18:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101723CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 17 09:38:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

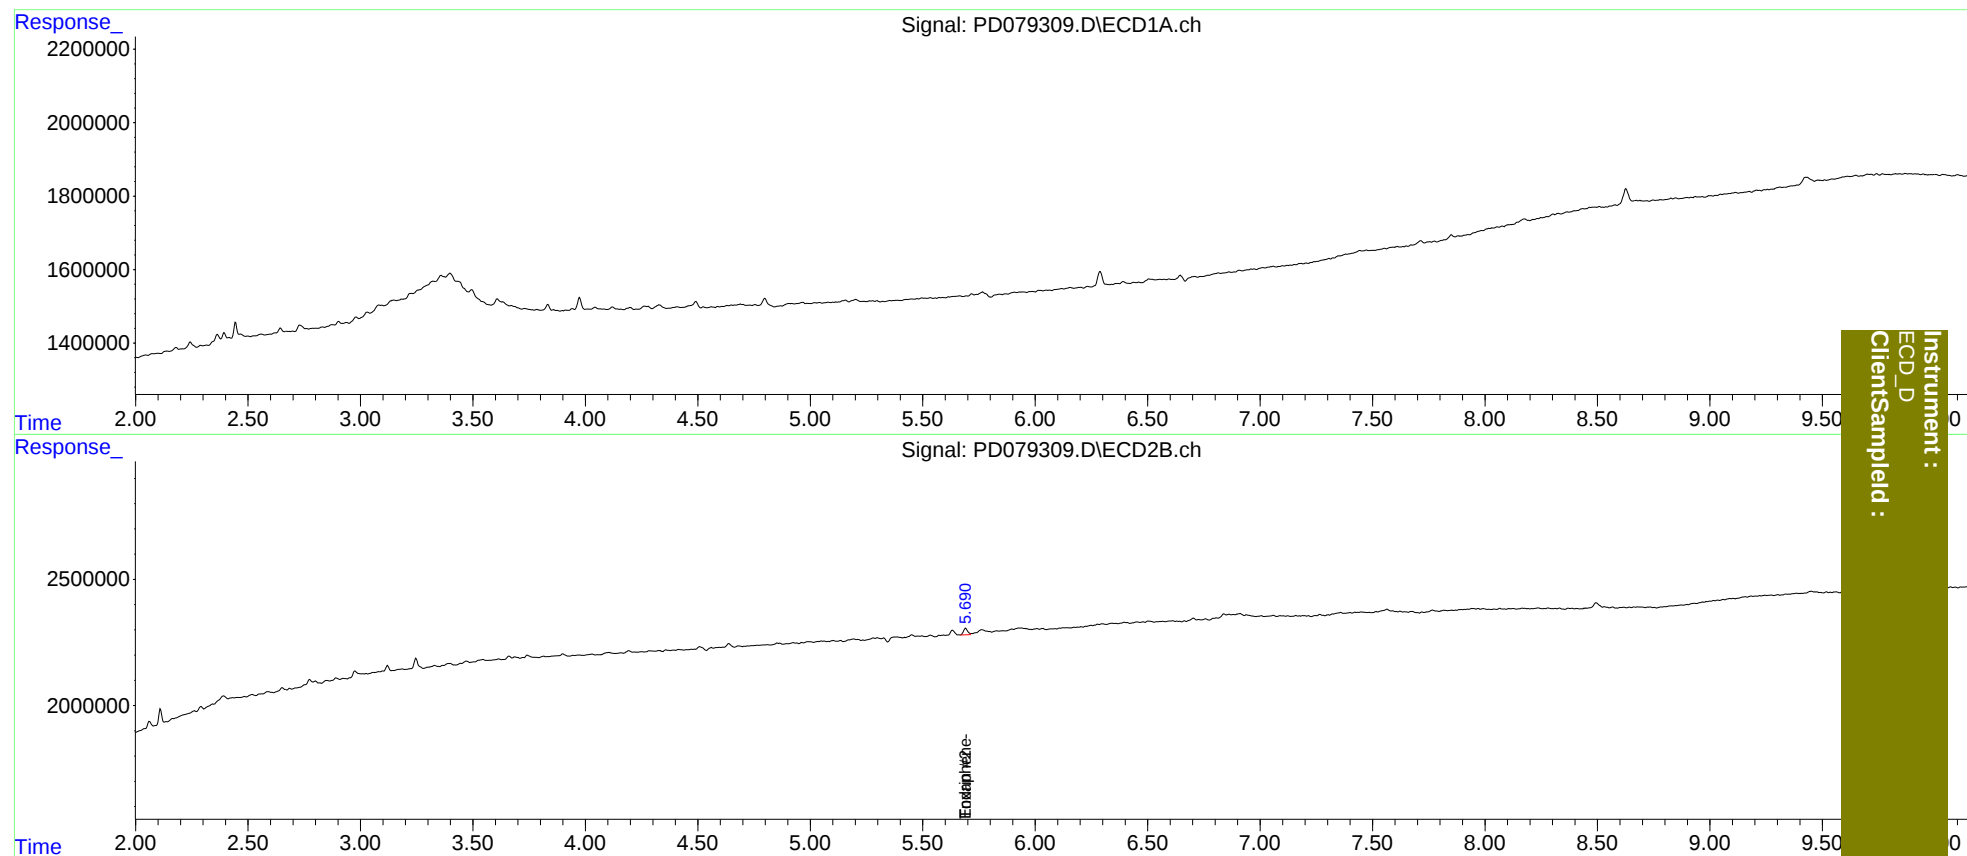


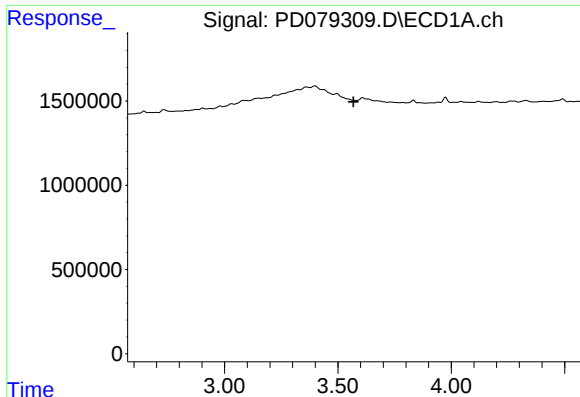

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

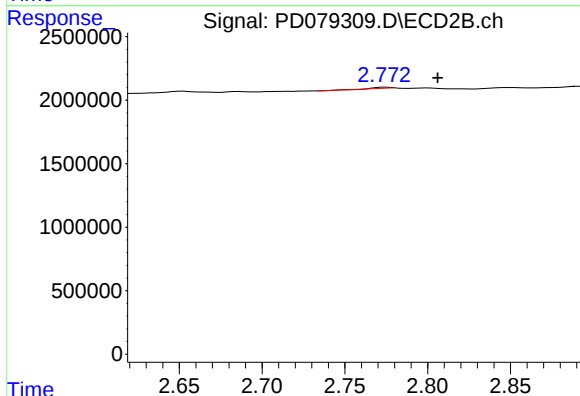


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: -0.032 min
Response: 82661
Conc: N.D.

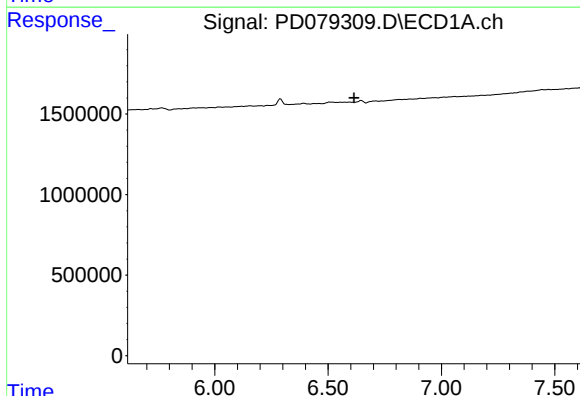


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.615 min
Response: 0
Conc: N.D.

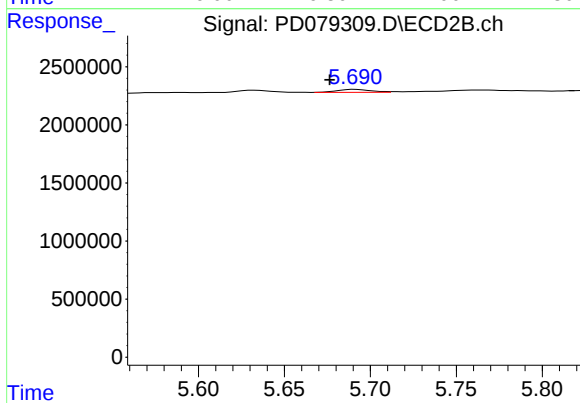

#14 Endrin


R.T.: 5.691 min
Delta R.T.: 0.015 min
Response: 335851
Conc: 0.13 ng/ml

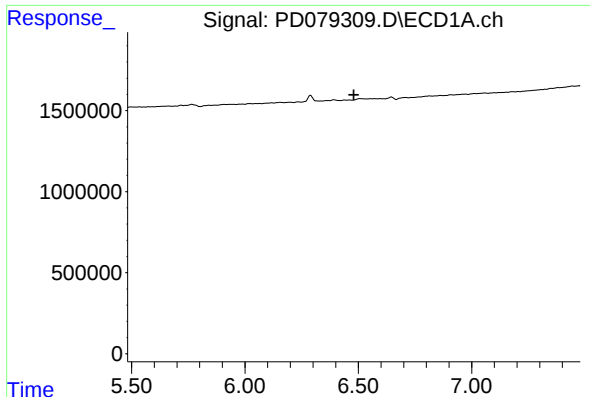

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 6.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

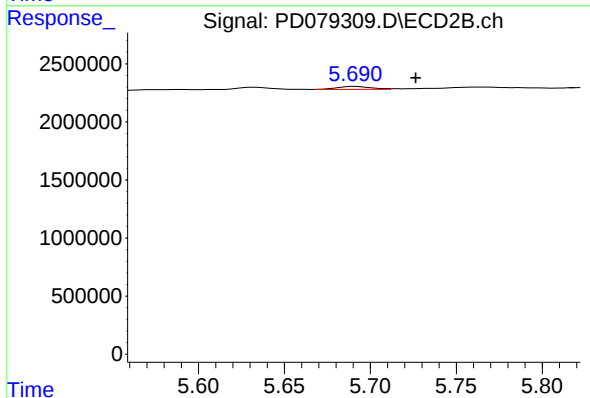


#23 Toxaphene-2

R.T.: 5.691 min
Delta R.T.: -0.035 min
Response: 335851
Conc: 20.44 ng/ml

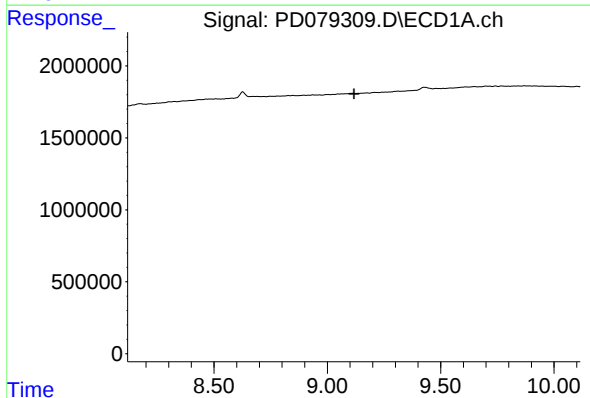

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.118 min
Response: 0
Conc: N.D.

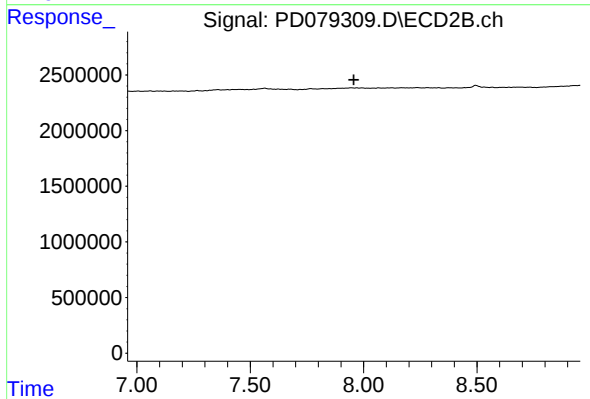

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.957 min
Response: 0
Conc: N.D.