

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110124\
 Data File : PD086279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2024 18:14
 Operator : AR\AJ
 Sample : PB164588BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK588

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:18:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.889	29150950	217.1E6	22.141	23.407
27)	SA Decachlor...	9.097	8.098	41866026	247.3E6	23.353	26.149
Target Compounds							
2)	A alpha-BHC	4.034	3.393	94034	782717	<MDL	<MDL #
3)	MA gamma-BHC...	4.353	3.742	-23514	636850	N.D.	<MDL
4)	MA Heptachlor	4.933	0.000	39468	0	<MDL	N.D. #
6)	B beta-BHC	4.562	0.000	52158	0	<MDL	N.D. #
7)	B delta-BHC	4.794	4.294	701153	169829	0.271	<MDL #
8)	B Heptachlo...	5.731	0.000	276499	0	0.121	N.D. #
9)	A Endosulfan I	6.090	5.263	37360	562132	<MDL	<MDL #
10)	B trans-Chl...	5.956	5.086f	14623	387649	<MDL	<MDL #
11)	B cis-Chlor...	6.040	5.219	92902	2819504	<MDL	0.222 #
13)	MA Dieldrin	6.368	0.000	33676	0	<MDL	N.D. #
14)	MA Endrin	6.538f	5.810	30274	1025259	<MDL	<MDL #
15)	B Endosulfa...	6.799	0.000	220002	0	0.110	N.D. #
16)	A 4,4'-DDD	6.725	6.006f	118097	239438	<MDL	<MDL #
17)	MA 4,4'-DDT	7.056	6.201	-898	809732	N.D.	<MDL
18)	B Endrin al...	0.000	6.307	0	303591	N.D.	<MDL
19)	B Endosulfa...	0.000	6.514	0	281348	N.D.	<MDL
20)	A Methoxychlor	7.453f	6.803	84080	-133263	<MDL	N.D. #
21)	B Endrin ke...	7.680	6.968f	99969	1003229	<MDL	<MDL #
22)	Toxaphene-1	0.000	5.219f	0	2819504	N.D.	42.956
23)	Toxaphene-2	6.464	5.810f	45257	1025259	2.279	14.633 #
25)	Toxaphene-4	0.000	7.231	0	1063882	N.D.	6.555
26)	Toxaphene-5	0.000	7.352	0	684712	N.D.	5.855


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110124\
Data File : PD086279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2024 18:14
Operator : AR\AJ
Sample : PB164588BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:18:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

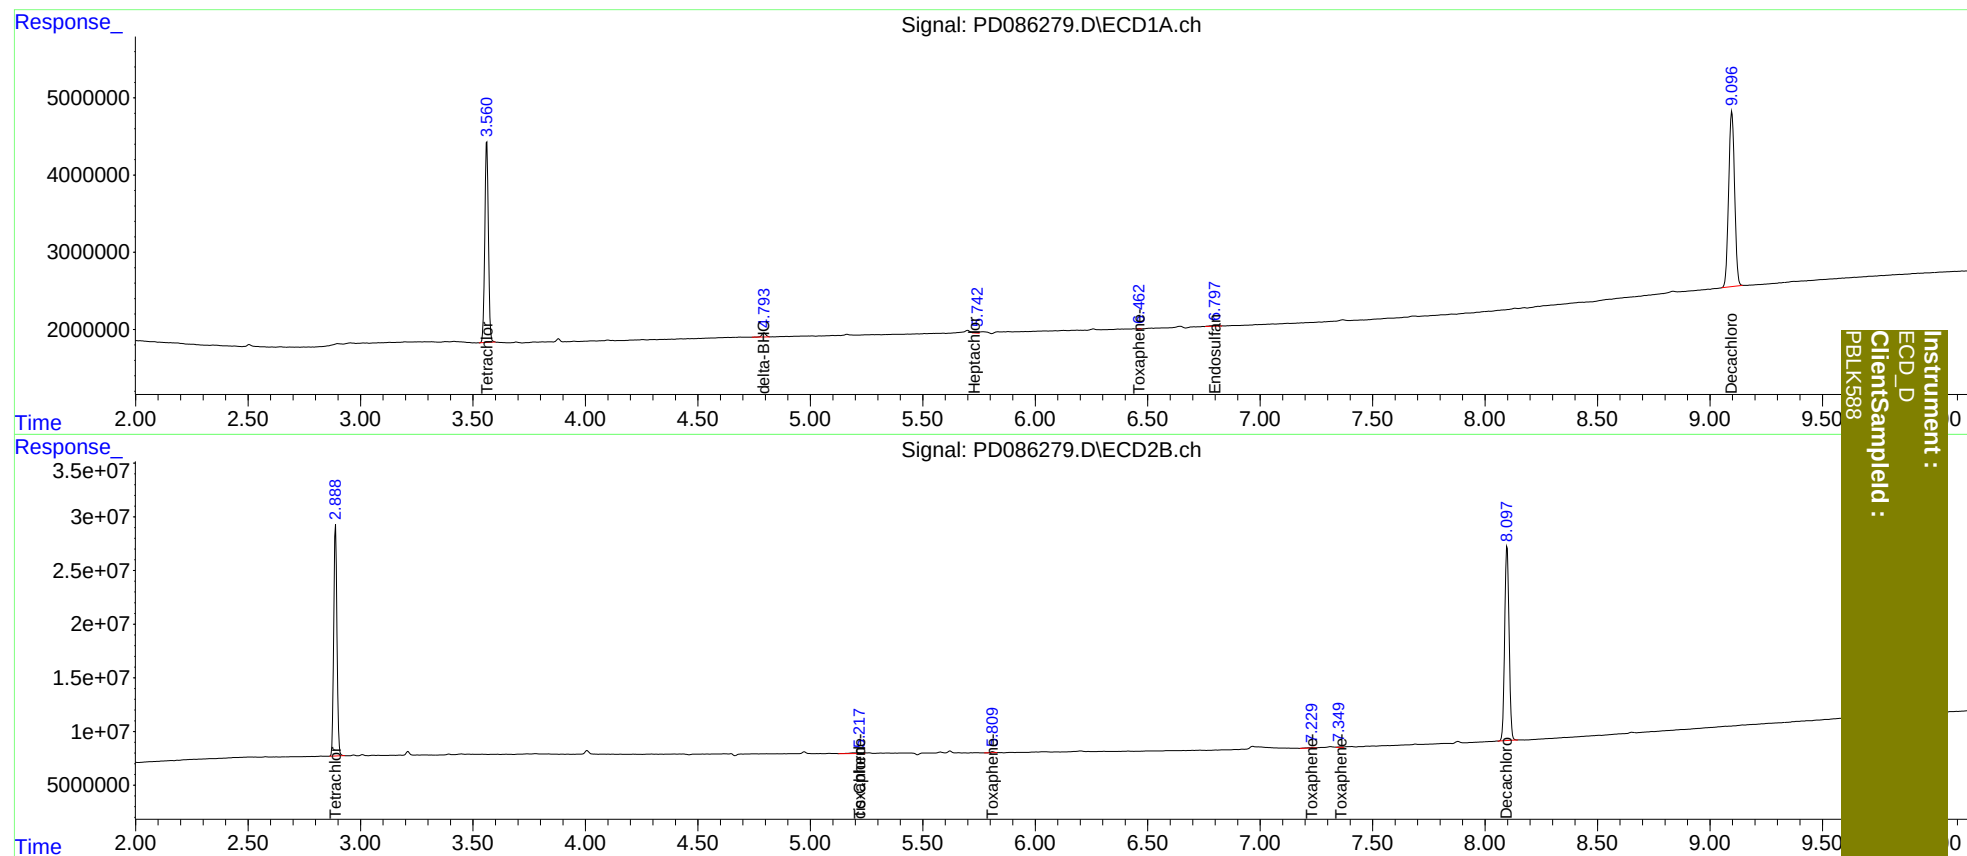


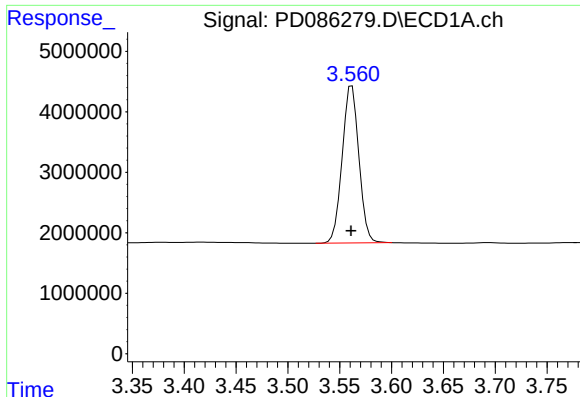

#1 Tetrachloro-m-xylene


R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 29150950
Conc: 22.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK588

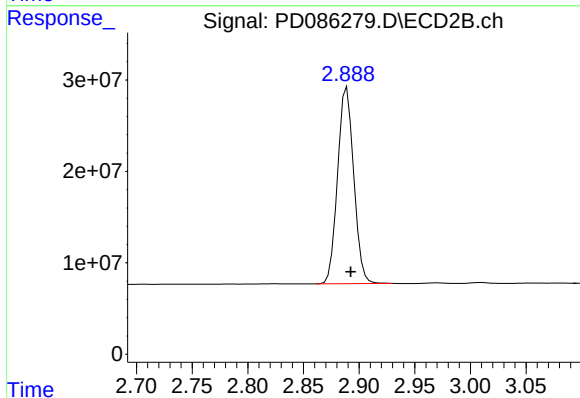


#1 Tetrachloro-m-xylene

R.T.: 2.889 min
Delta R.T.: -0.004 min
Response: 217117567
Conc: 23.41 ng/ml

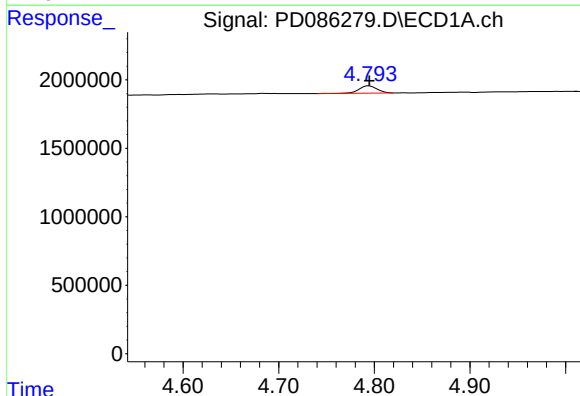


#7 delta-BHC

R.T.: 4.794 min
Delta R.T.: 0.000 min
Response: 701153
Conc: 0.27 ng/ml

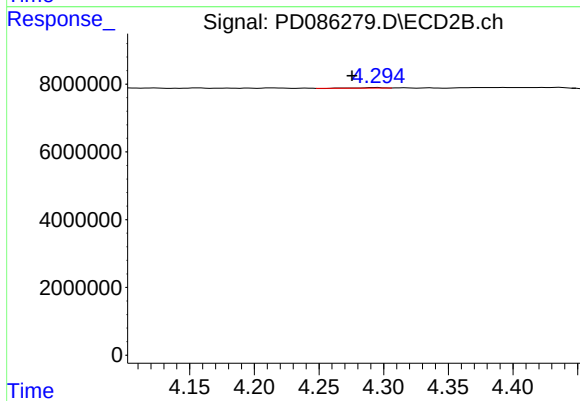

#7 delta-BHC


R.T.: 4.294 min
Delta R.T.: 0.019 min
Response: 169829
Conc: N.D.

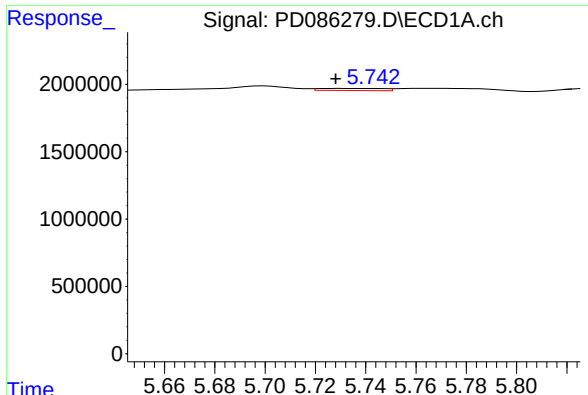

#8 Heptachlor epoxide


R.T.: 5.731 min
Delta R.T.: 0.003 min
Response: 276499
Conc: 0.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK588

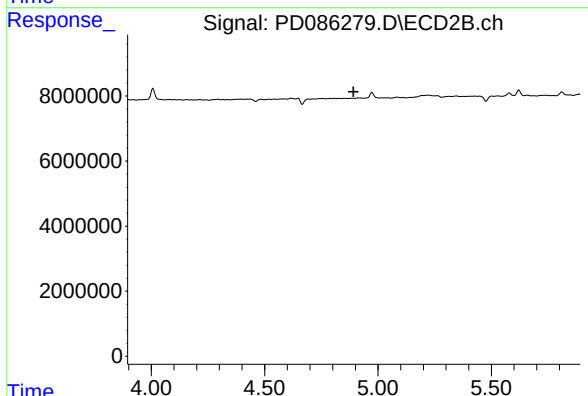


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.892 min
Response: 0
Conc: N.D.

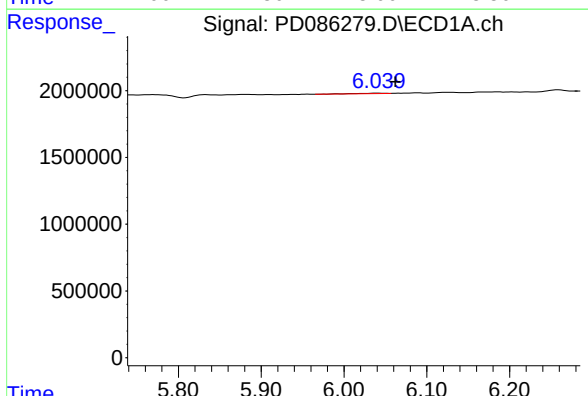


#11 cis-Chlordane

R.T.: 6.040 min
Delta R.T.: -0.022 min
Response: 92902
Conc: N.D.

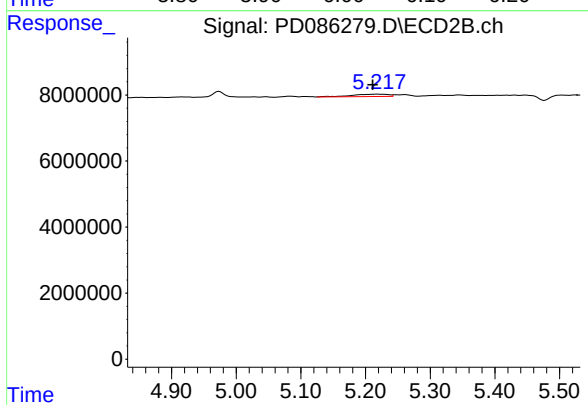

#11 cis-Chlordane


R.T.: 5.219 min
Delta R.T.: 0.008 min
Response: 2819504
Conc: 0.22 ng/ml

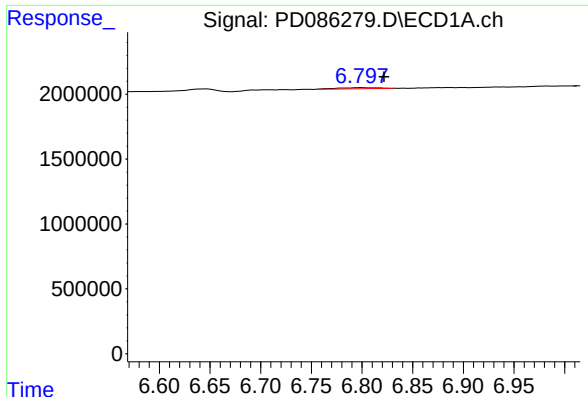

#15 Endosulfan II


R.T.: 6.799 min
Delta R.T.: -0.023 min
Response: 220002
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK588

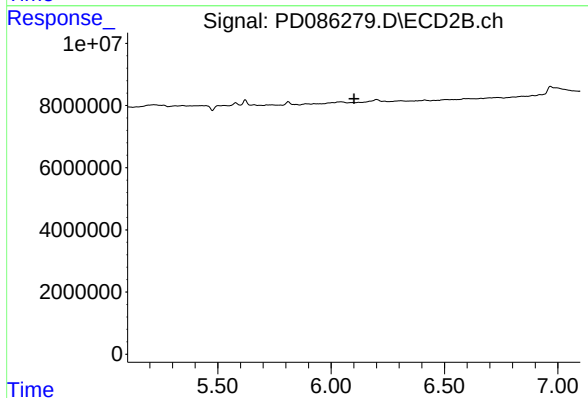


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.101 min
Response: 0
Conc: N.D.

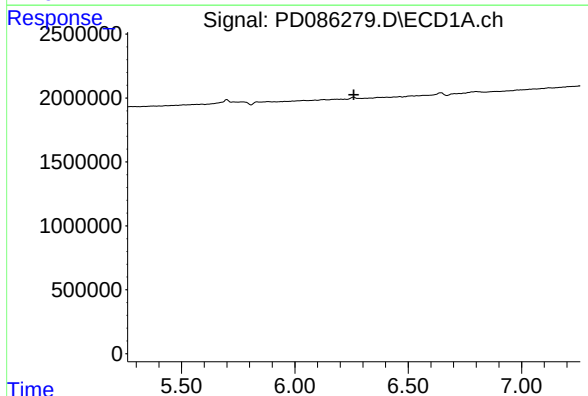


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 6.259 min
Response: 0
Conc: N.D.

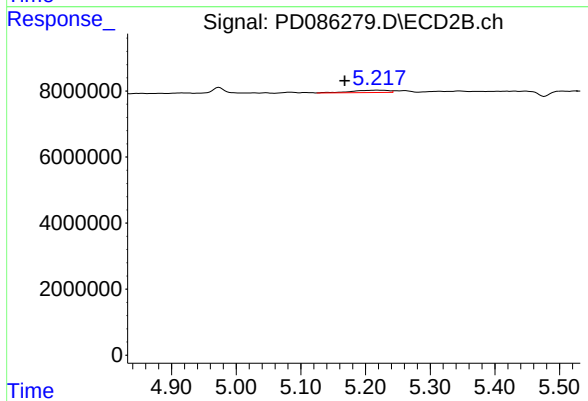

#22 Toxaphene-1


R.T.: 5.219 min
Delta R.T.: 0.051 min
Response: 2819504
Conc: 42.96 ng/ml

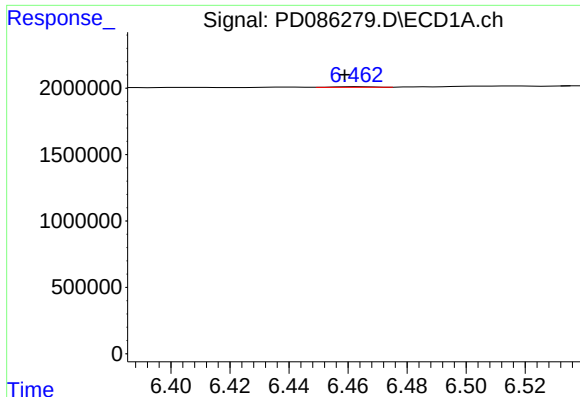

#23 Toxaphene-2


R.T.: 6.464 min
Delta R.T.: 0.005 min
Response: 45257
Conc: 2.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK588

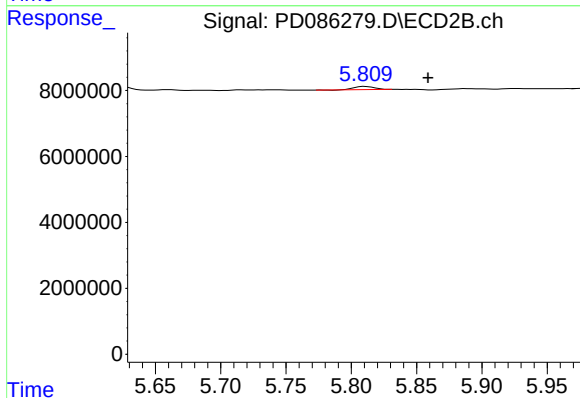


#23 Toxaphene-2

R.T.: 5.810 min
Delta R.T.: -0.048 min
Response: 1025259
Conc: 14.63 ng/ml

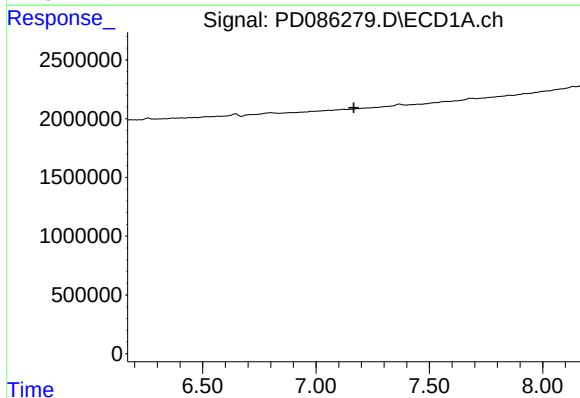


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

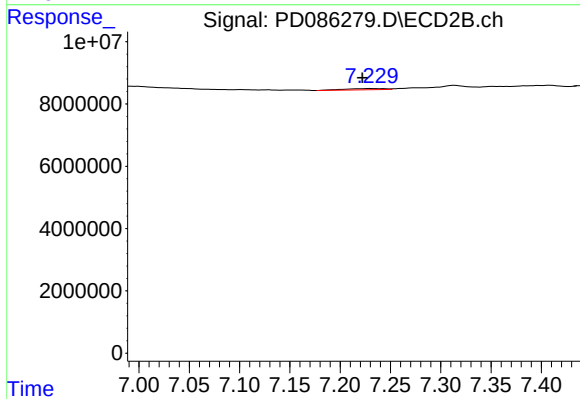

#25 Toxaphene-4


R.T.: 7.231 min
Delta R.T.: 0.009 min
Response: 1063882
Conc: 6.56 ng/ml

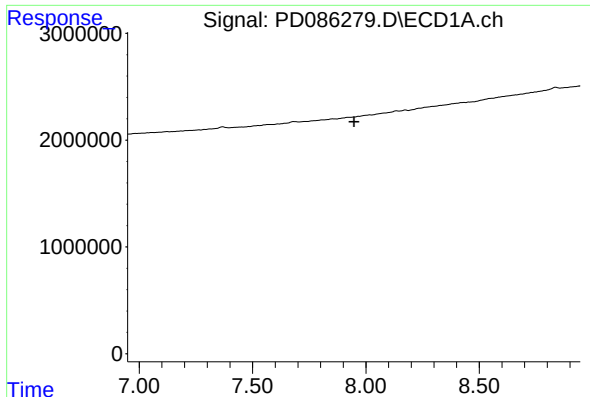

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 7.947 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK588

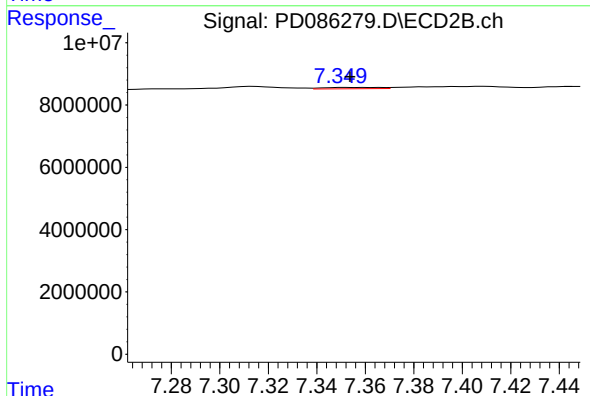


#26 Toxaphene-5

R.T.: 7.352 min
Delta R.T.: -0.002 min
Response: 684712
Conc: 5.85 ng/ml

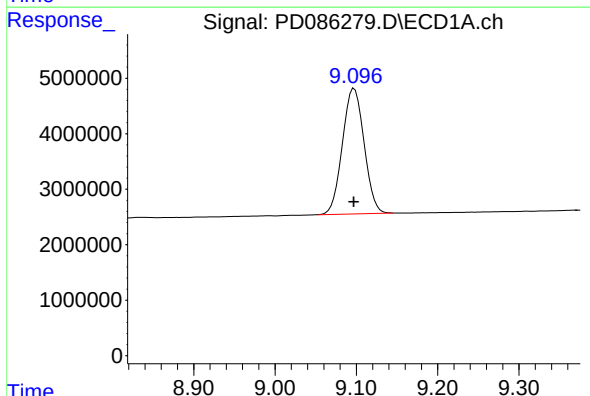

#27 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.000 min
Response: 41866026
Conc: 23.35 ng/ml

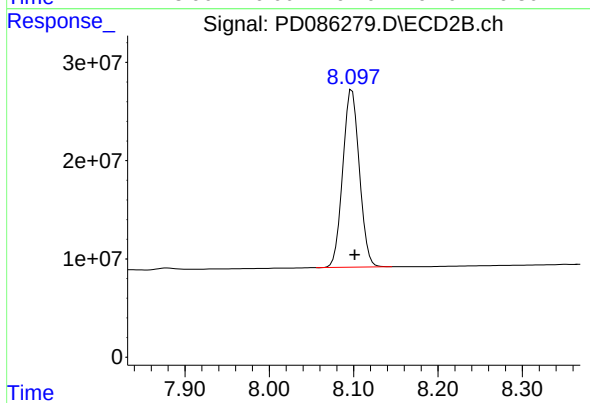

#27 Decachlorobiphenyl

R.T.: 8.098 min
Delta R.T.: -0.003 min
Response: 247260096
Conc: 26.15 ng/ml