

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110124\
 Data File : PD086280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2024 18:28
 Operator : AR\AJ
 Sample : PB164588BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS588

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/04/2024
 Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:18:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.889	24756805	187.0E6	18.804	20.155
2)	SA Decachlor...	9.099	8.099	36095133	215.2E6	20.134	22.762
Target Compounds							
2)	A alpha-BHC	4.013	3.404	11701754	84863412	4.701	5.907 #
3)	MA gamma-BHC...	4.345	3.741	11991268	82422708	4.820	6.111 #
4)	MA Heptachlor	4.946	4.098	12526524	84218713	5.067	6.165
5)	MB Aldrin	5.289	4.384	12087851	82055726	4.987	6.048
6)	B beta-BHC	4.529	4.035	5677546	37549936	5.112	5.989m
7)	B delta-BHC	4.777	4.273	12417302	80485715	4.797	5.736
8)	B Heptachlo...	5.709	4.889	11703968	76266484	5.121	6.082
9)	A Endosulfan I	6.092	5.265	11013686	73123370	5.437	6.369
10)	B trans-Chl...	5.963	5.144	11222427	79141084	5.086	6.016
11)	B cis-Chlor...	6.045	5.208	11613102	79779873	5.252	6.281
12)	B 4,4'-DDE	6.213	5.394	20314449	142.9E6	9.511	11.658
13)	MA Dieldrin	6.365	5.531	23013194	149.5E6	10.089	12.115
14)	MA Endrin	6.592	5.808	19052210	135.8E6	10.136	12.086
15)	B Endosulfa...	6.803	6.099	20741425	132.5E6	10.346	12.013
16)	A 4,4'-DDD	6.722	5.949	16530807	122.2E6	10.202	12.447
17)	MA 4,4'-DDT	7.037	6.204	17540050	126.5E6	10.520m	12.329
18)	B Endrin al...	6.932	6.278	16308987	105.5E6	10.933	12.710
19)	B Endosulfa...	7.167	6.502	19768478	131.8E6	10.724	12.501
20)	A Methoxychlor	7.511	6.777	52043471	304.9E6	55.300	64.152
21)	B Endrin ke...	7.648	7.011	21999872	141.5E6	10.676	12.370

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110124\
Data File : PD086280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2024 18:28
Operator : AR\AJ
Sample : PB164588BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:18:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

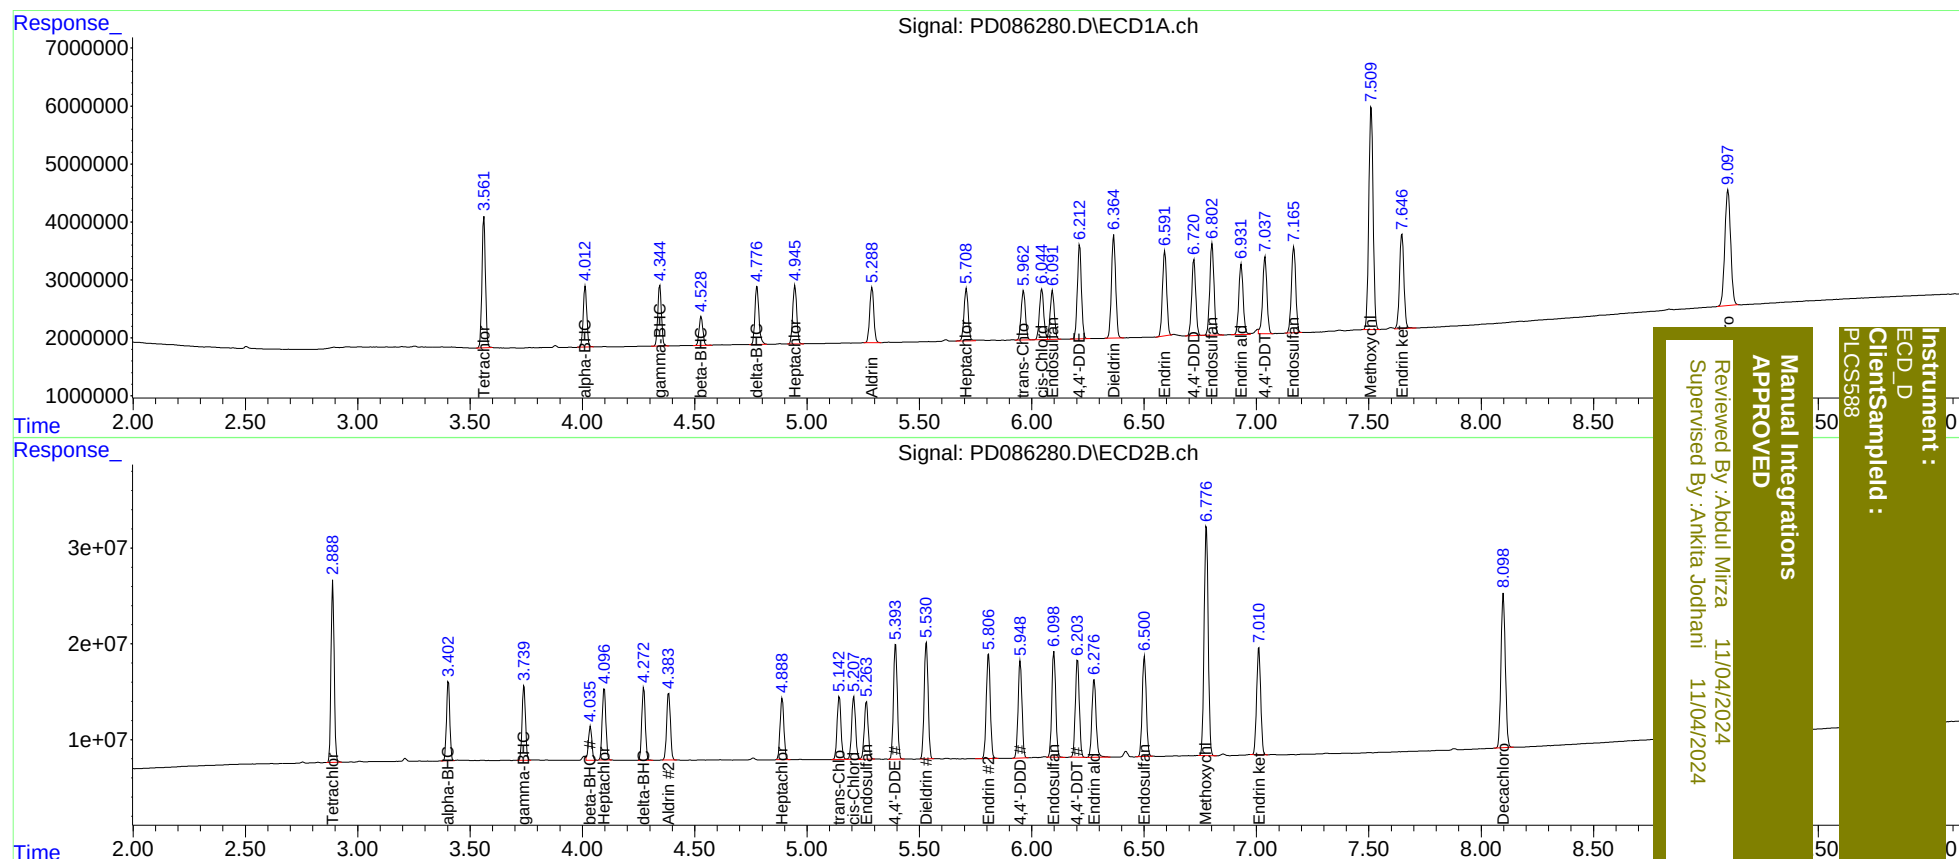

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/04/2024
Supervised By: Ankita Jodhani 11/04/2024

Instrument :
ECD_D
Client Sampled :
PLCS588