

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110124\
 Data File : PD086294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2024 21:45
 Operator : AR\AJ
 Sample : P4627-15MS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0CD2MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/04/2024
 Supervised By : Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:22:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.889	31239674	227.7E6	23.728	24.542
27)	SA Decachlor...	9.095	8.098	27523459	164.5E6	15.353	17.393
Target Compounds							
2)	A alpha-BHC	4.012	3.403	164.7E6	850.8E6	66.170	59.219
3)	MA gamma-BHC...	4.344	3.740	161.5E6	796.3E6	64.927	59.037
4)	MA Heptachlor	4.946	4.097	141.8E6	718.1E6	57.361	52.563
5)	MB Aldrin	5.288	4.384	134.3E6	692.7E6	55.403	51.062
6)	B beta-BHC	4.528	4.034	60241445	332.7E6	54.244	53.067m
7)	B delta-BHC	4.777	4.273	163.3E6	796.0E6	63.072	56.728
8)	B Heptachlo...	5.708	4.889	132.3E6	676.8E6	57.879	53.968
9)	A Endosulfan I	6.091	5.264	123.3E6	640.2E6	60.872	55.763
10)	B trans-Chl...	5.962	5.143	125.9E6	703.7E6	57.069	53.493
11)	B cis-Chlor...	6.044	5.208	128.4E6	685.4E6	58.093	53.964
12)	B 4,4'-DDE	6.212	5.394	252.2E6	1288.8E6	118.084	105.111
13)	MA Dieldrin	6.364	5.529	285.9E6	1361.7E6	125.361	110.371m
14)	MA Endrin	6.590	5.805	245.9E6	1232.0E6	130.828m	109.625m
15)	B Endosulfa...	6.802	6.098	236.2E6	1170.7E6	117.800	106.115
16)	A 4,4'-DDD	6.721	5.949	202.7E6	1082.5E6	125.067	110.279
17)	MA 4,4'-DDT	7.036	6.203	207.0E6	1119.9E6	124.128m	109.129
18)	B Endrin al...	6.930	6.277	176.0E6	884.3E6	117.953	106.524
19)	B Endosulfa...	7.165	6.501	225.0E6	1138.2E6	122.043	107.969
20)	A Methoxychlor	7.509	6.776	552.2E6	2346.1E6	586.700	493.567
21)	B Endrin ke...	7.646	7.010	248.7E6	1226.7E6	120.692	107.204

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110124\
Data File : PD086294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2024 21:45
Operator : AR\AJ
Sample : P4627-15MS
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:22:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

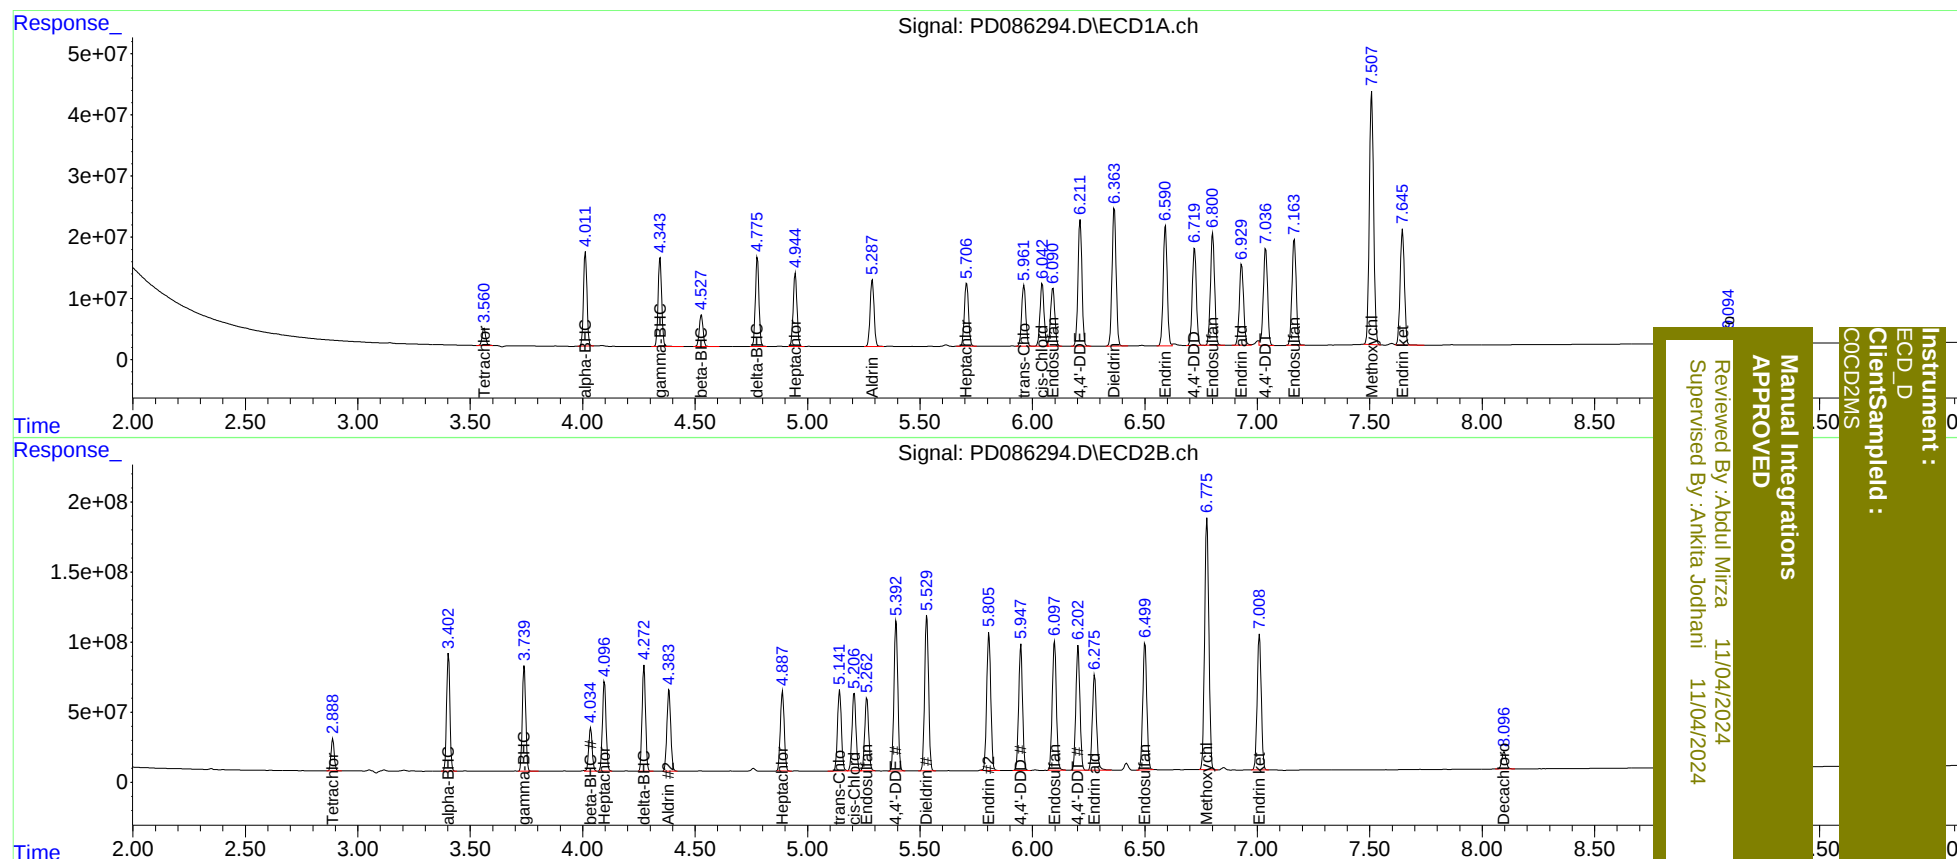

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 11/04/2024
Supervised By: Ankita Jodhani 11/04/2024

Instrument :
ECD_D
Client Sampled :
C00CD2MS