

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
 Data File : PD050150.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2018 18:52
 Operator : AJ\SJ
 Sample : PSTDICC050
 Misc : (FOR MIREX)
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 05:26:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:25:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.061	32675709	1364.2E6	50.000	50.000
28)	SA Decachlor...	9.019	9.173	29904941	835.9E6	50.000	50.000
Target Compounds							
22)	Mirex	8.162	8.273	27941554	714.9E6	50.000	50.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
Data File : PD050150.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 18:52
Operator : AJ\SJ
Sample : PSTDICC050
Misc : (FOR MIREX)
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 05:26:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:25:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

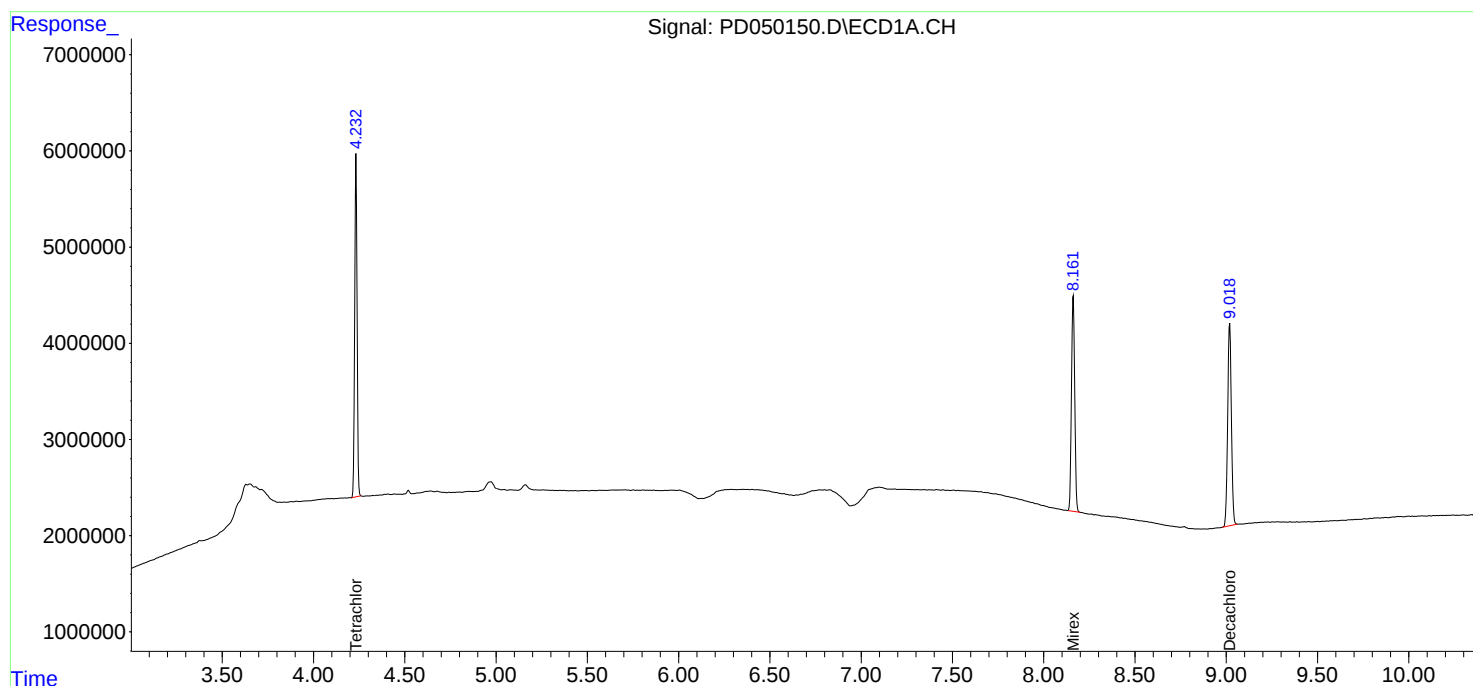


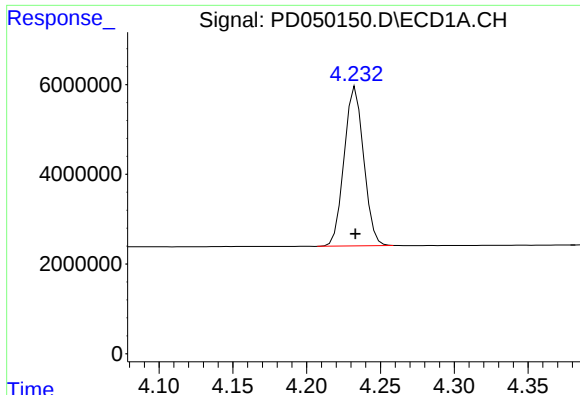

#1 Tetrachloro-m-xylene


R.T.: 4.233 min
Delta R.T.: 0.000 min
Response: 32675709
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

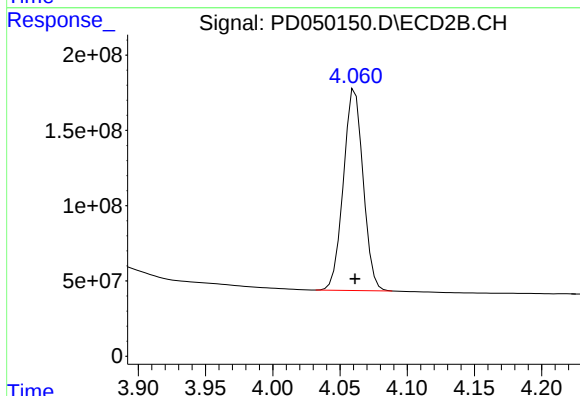


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 1364190774
Conc: 50.00 ng/ml

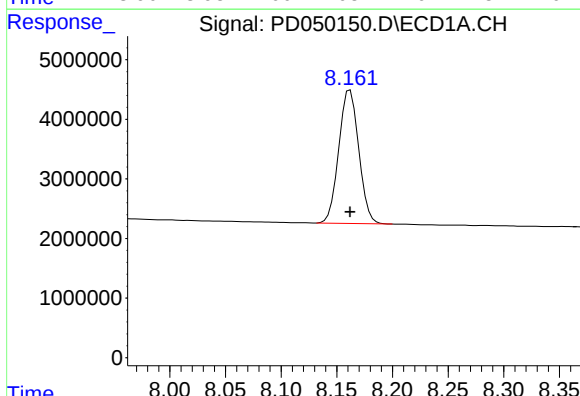


#22 Mirex

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 27941554
Conc: 50.00 ng/ml

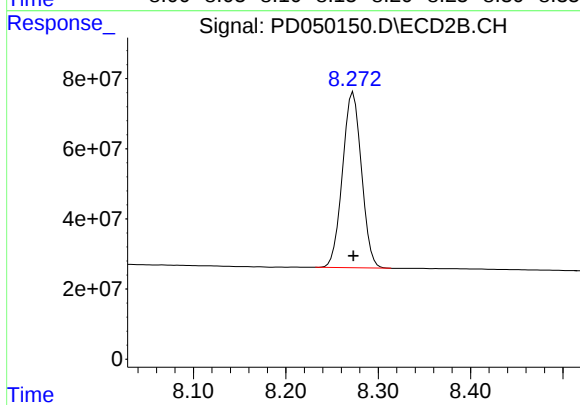

#22 Mirex


R.T.: 8.273 min
Delta R.T.: 0.000 min
Response: 714855800
Conc: 50.00 ng/ml

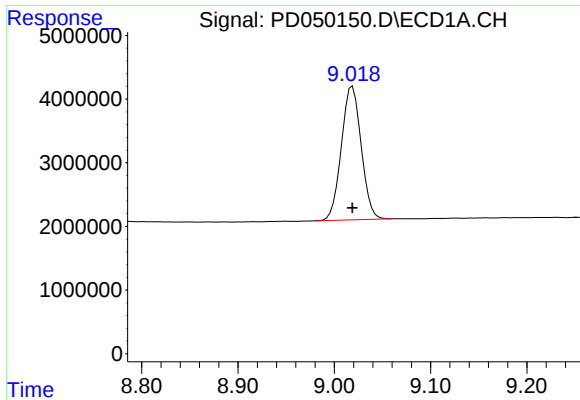

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 29904941
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

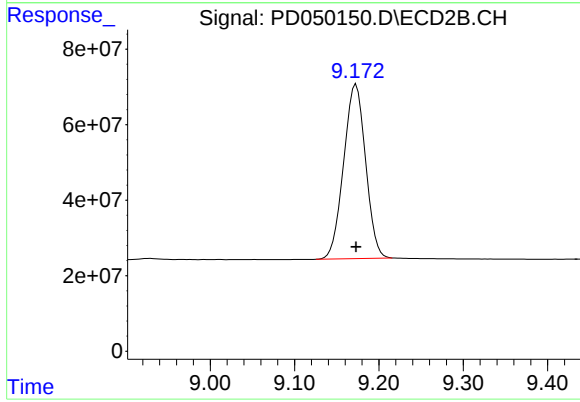

#28 Decachlorobiphenyl

R.T.: 9.173 min
Delta R.T.: 0.000 min
Response: 835901064
Conc: 50.00 ng/ml