

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
 Data File : PD050158.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2018 20:44
 Operator : AJ\SJ
 Sample : MIREX-MDL-S-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 05:38:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.061	11214722	484.2E6	17.304	17.421
28)	SA Decachlor...	9.018	9.172	10978079	327.9E6	18.152	18.948
Target Compounds							
22)	Mirex	8.161	8.271	421009	18748901	0.758	1.277 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
Data File : PD050158.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 20:44
Operator : AJ\SJ
Sample : MIREX-MDL-S-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 05:38:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

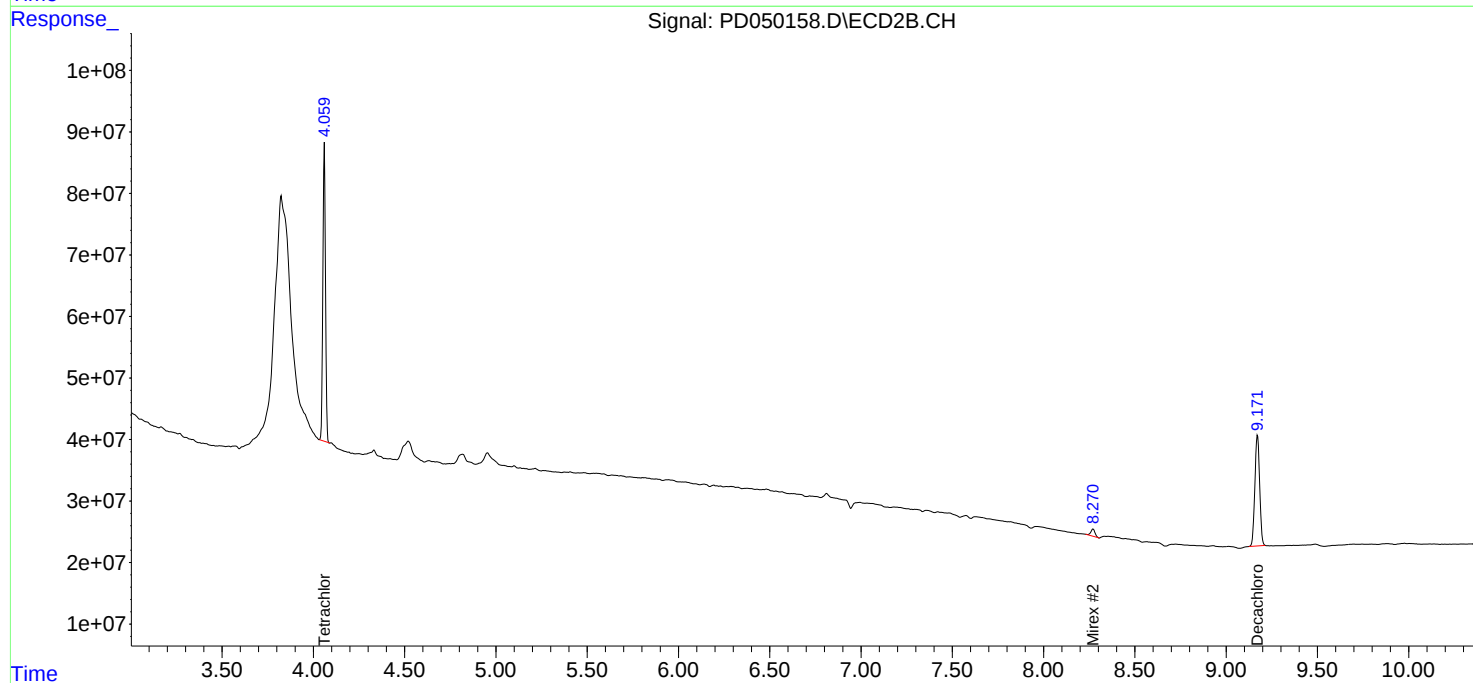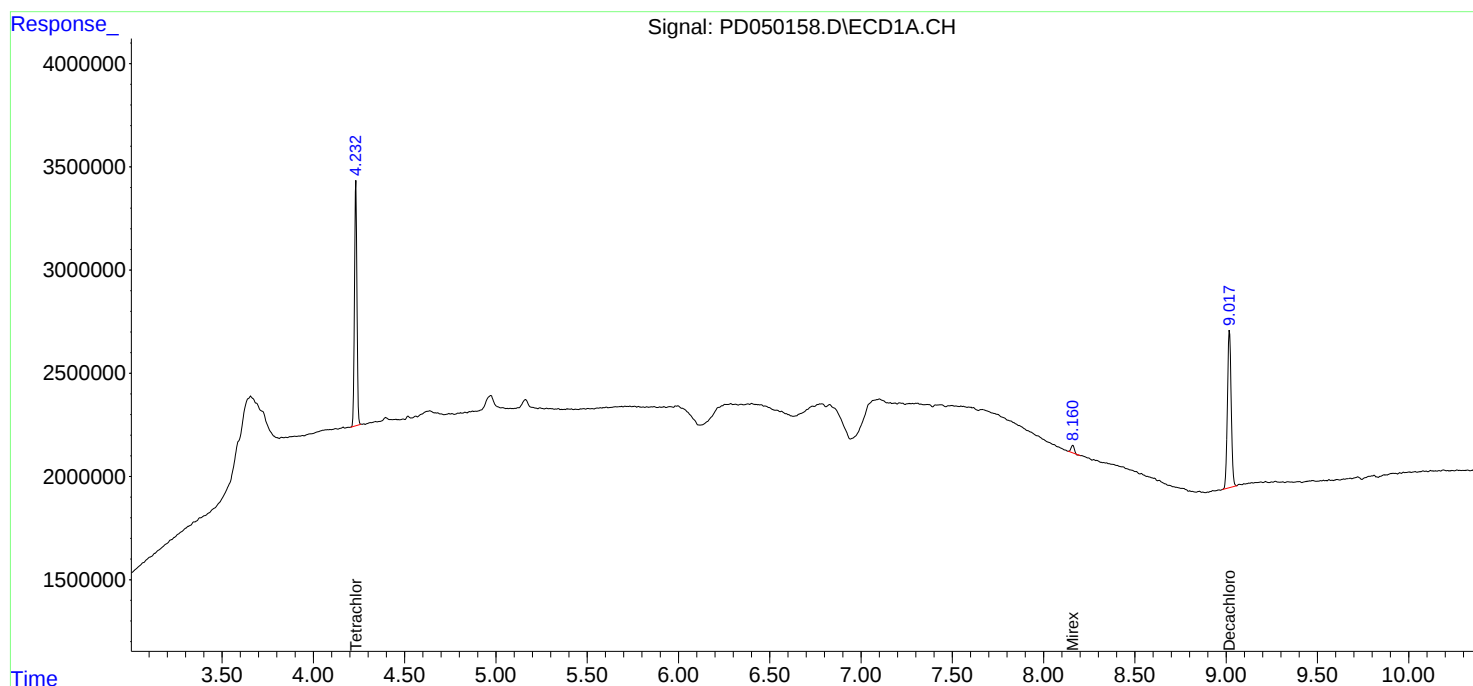


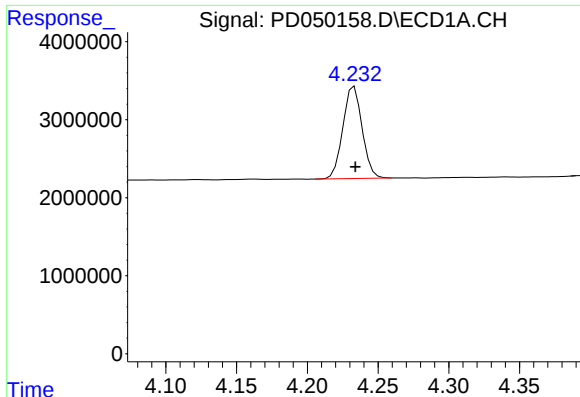

#1 Tetrachloro-m-xylene


R.T.: 4.233 min
Delta R.T.: 0.000 min
Response: 11214722
Conc: 17.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

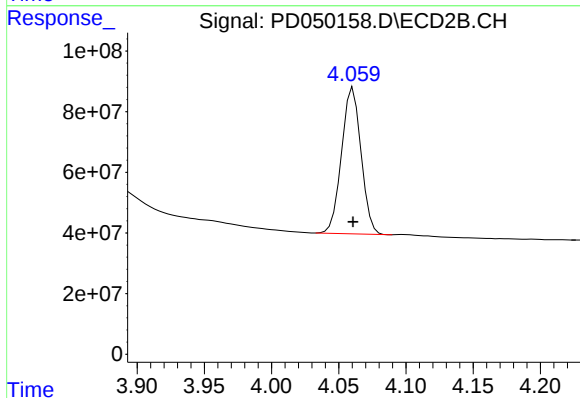


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 484167866
Conc: 17.42 ng/ml

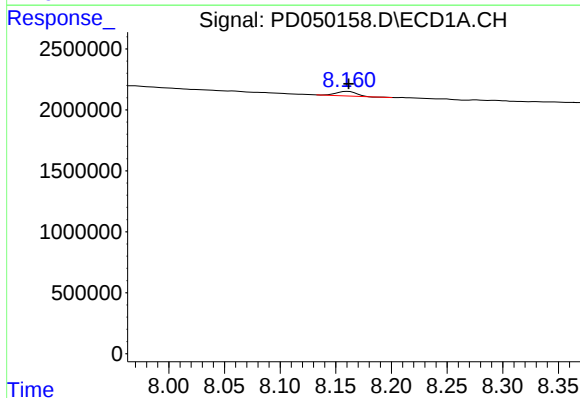


#22 Mirex

R.T.: 8.161 min
Delta R.T.: 0.000 min
Response: 421009
Conc: 0.76 ng/ml

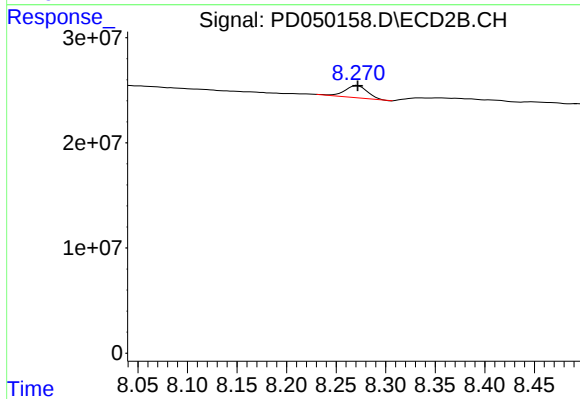

#22 Mirex


R.T.: 8.271 min
Delta R.T.: 0.000 min
Response: 18748901
Conc: 1.28 ng/ml

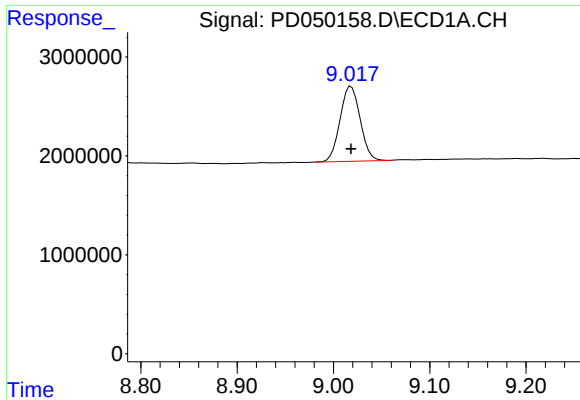

#28 Decachlorobiphenyl

R.T.: 9.018 min
Delta R.T.: 0.000 min
Response: 10978079
Conc: 18.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

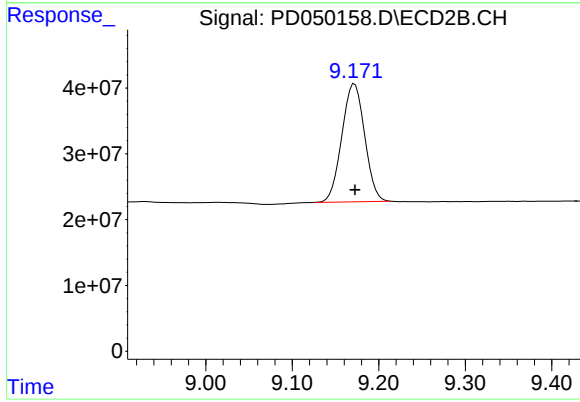

#28 Decachlorobiphenyl

R.T.: 9.172 min
Delta R.T.: 0.000 min
Response: 327896072
Conc: 18.95 ng/ml