

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
 Data File : PD050160.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2018 21:12
 Operator : AJ\SJ
 Sample : MIREX-MDL-S-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 05:38:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.234	4.061	10735105	472.0E6	16.564	16.983
28)	SA Decachlor...	9.019	9.173	10400989	316.1E6	17.198	18.265
Target Compounds							
22)	Mirex	0.000	8.273	0	13399292	N.D.	0.913 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
Data File : PD050160.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 21:12
Operator : AJ\SJ
Sample : MIREX-MDL-S-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 05:38:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

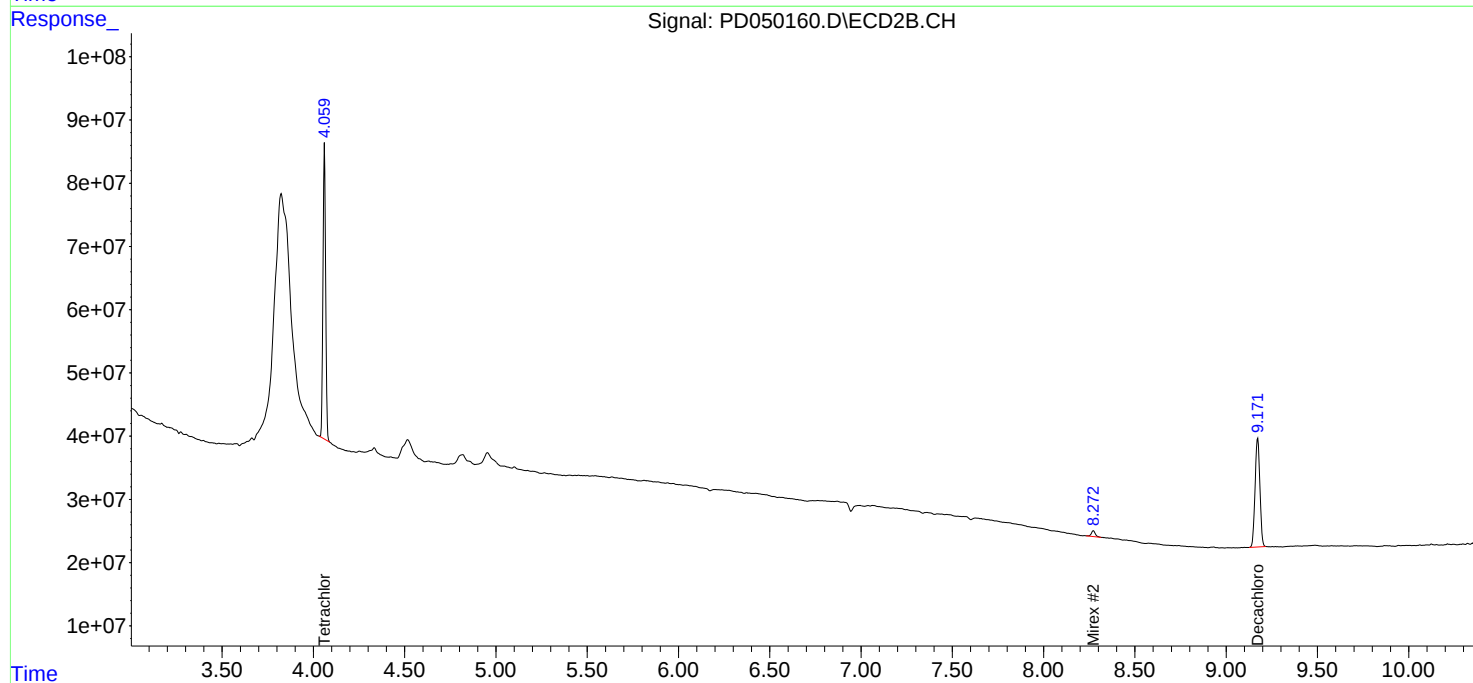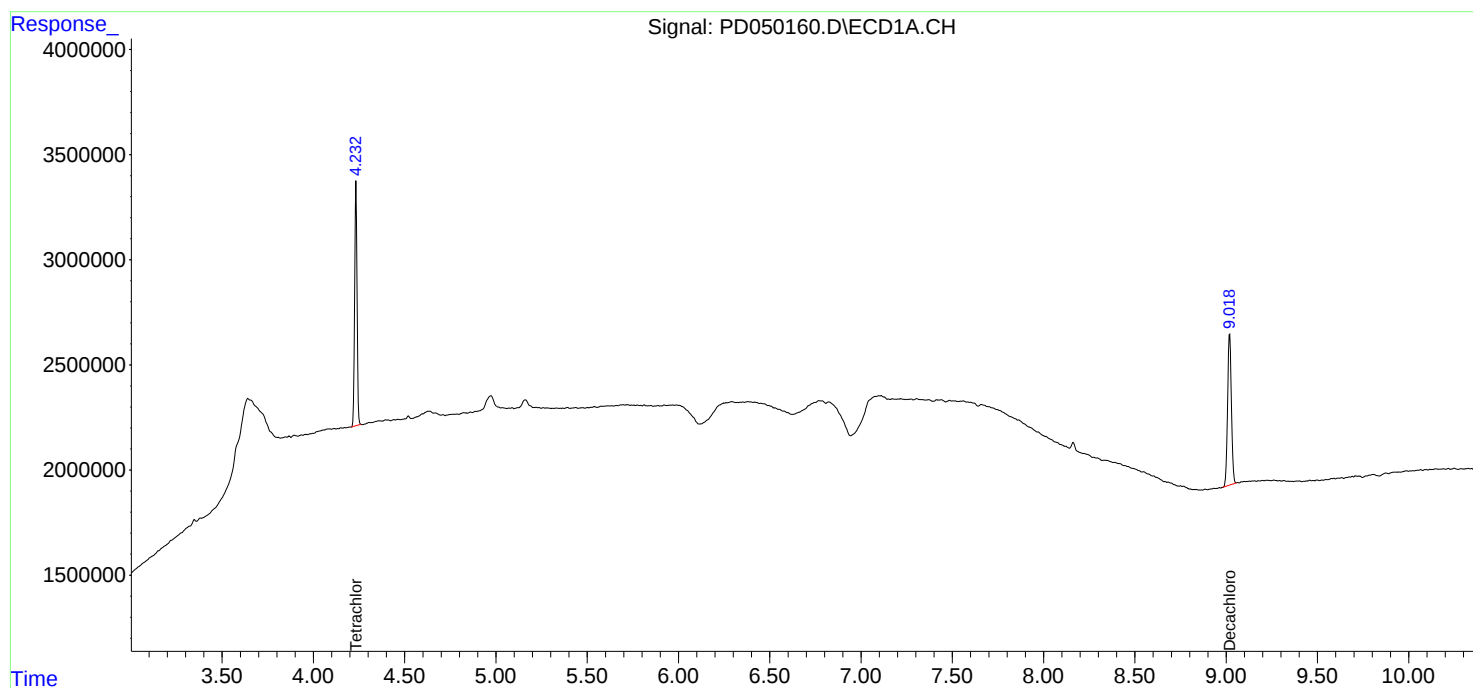


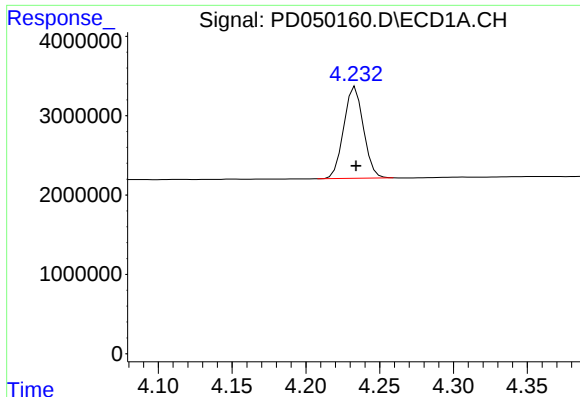

#1 Tetrachloro-m-xylene


R.T.: 4.234 min
Delta R.T.: 0.000 min
Response: 10735105
Conc: 16.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

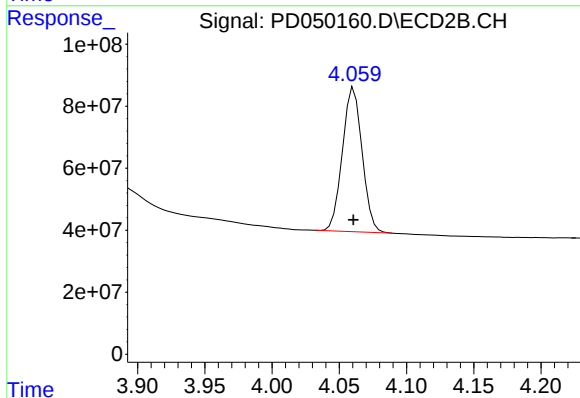


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 471990059
Conc: 16.98 ng/ml

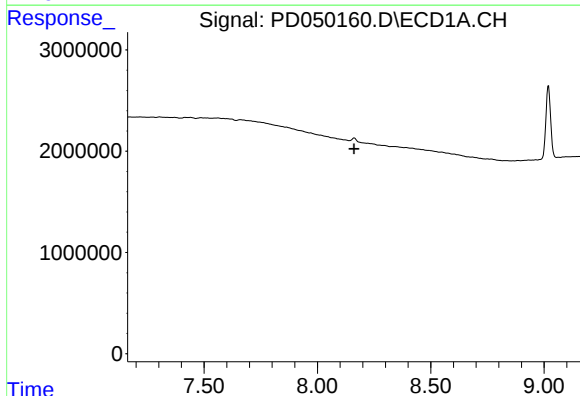


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.162 min
Response: 0
Conc: N.D.

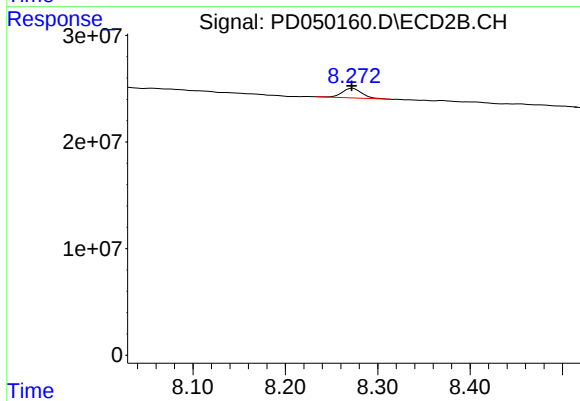

#22 Mirex


R.T.: 8.273 min
Delta R.T.: 0.001 min
Response: 13399292
Conc: 0.91 ng/ml

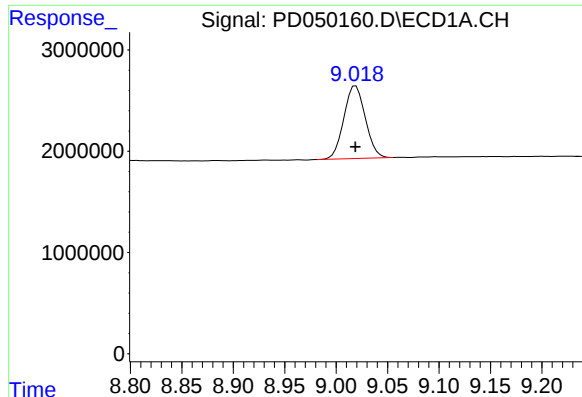

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 10400989
Conc: 17.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

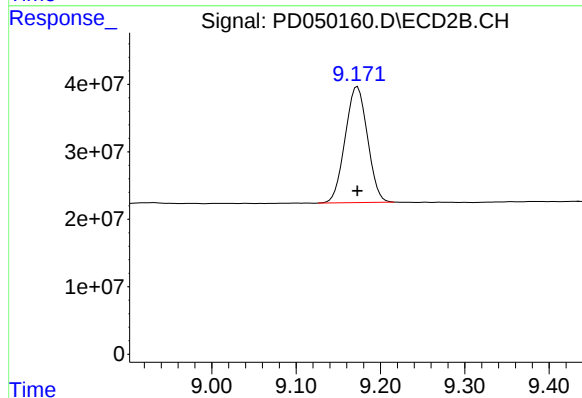

#28 Decachlorobiphenyl

R.T.: 9.173 min
Delta R.T.: 0.000 min
Response: 316086167
Conc: 18.27 ng/ml