

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
 Data File : PD050159.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2018 20:58
 Operator : AJ\SJ
 Sample : MIREX-MDL-S-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MIREX-MDL-S-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 05:38:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.061	10892436	482.2E6	16.807	17.349
28)	SA Decachlor...	9.018	9.172	10828128	324.4E6	17.904	18.748
Target Compounds							
22)	Mirex	8.162	8.272	425231	13812815	0.765	0.941



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
Data File : PD050159.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 20:58
Operator : AJ\SJ
Sample : MIREX-MDL-S-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-S-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 05:38:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

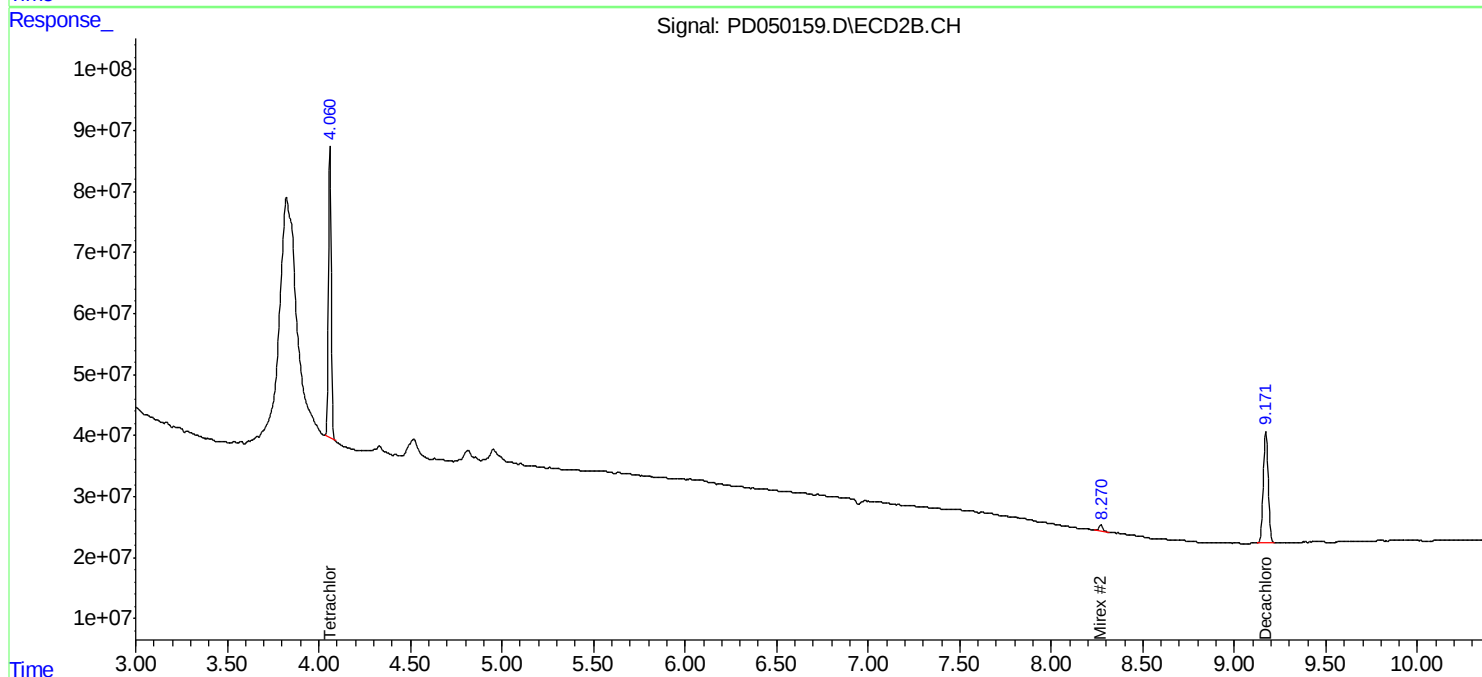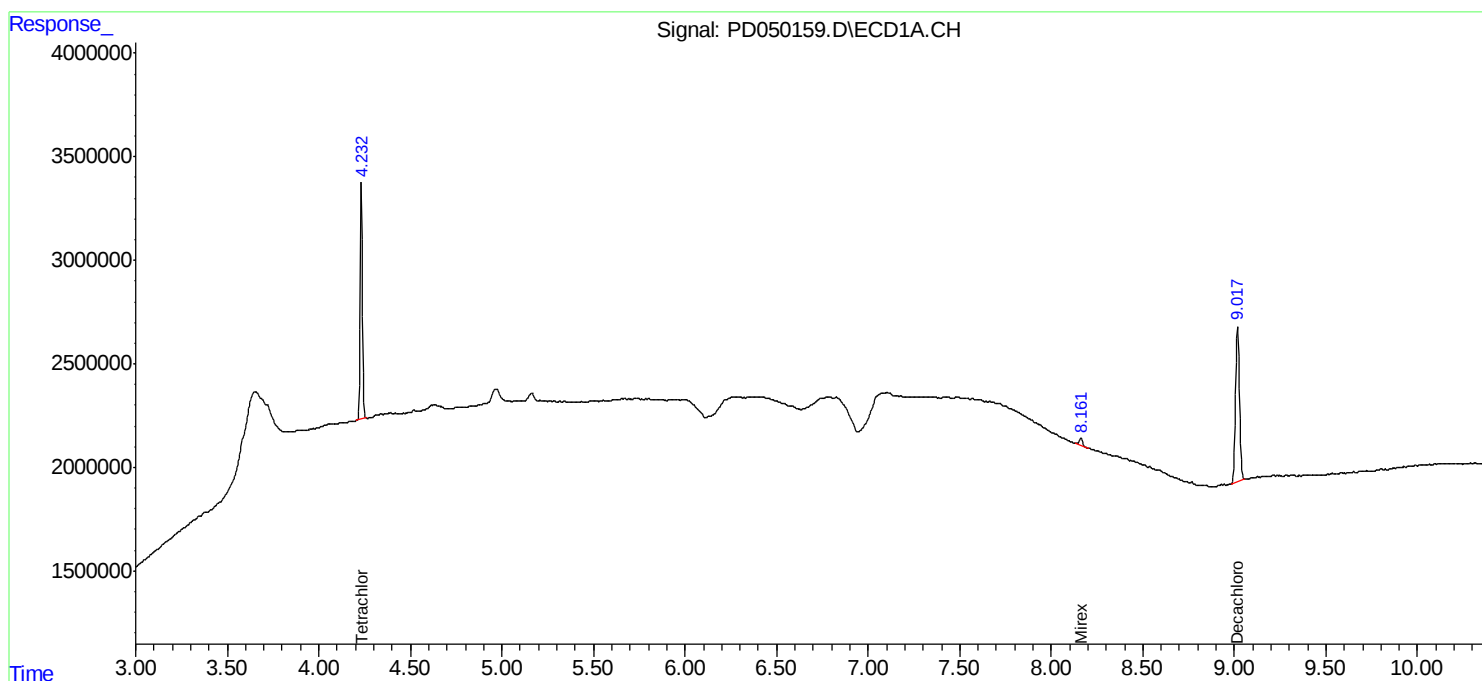


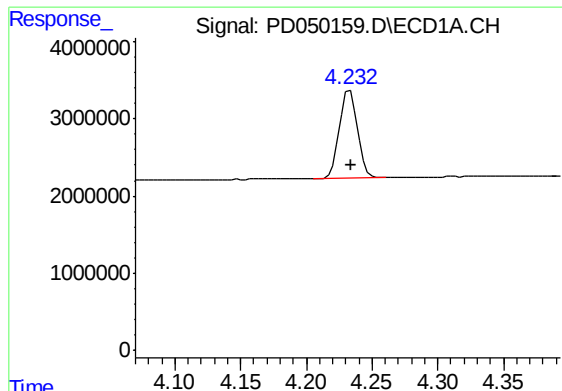

#1 Tetrachloro-m-xylene


R.T.: 4.233 min
Delta R.T.: 0.000 min
Response: 10892436
Conc: 16.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-S-02

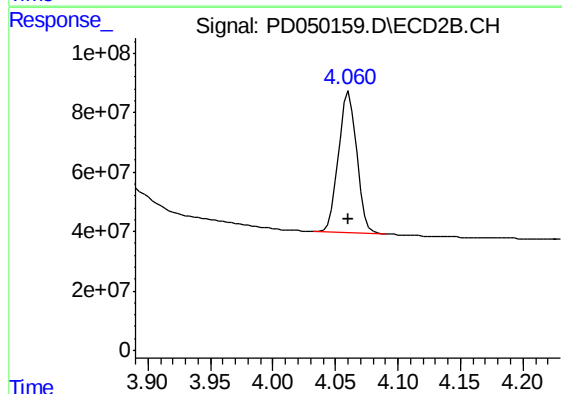


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 482157029
Conc: 17.35 ng/ml

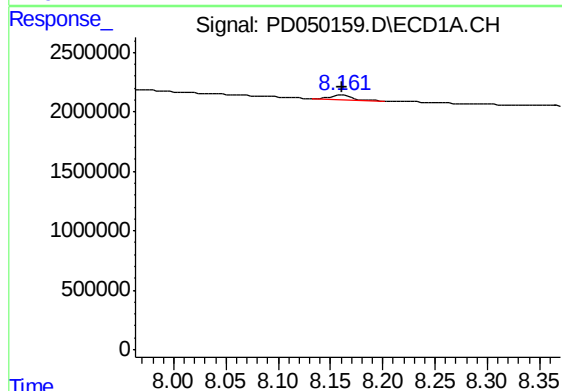


#22 Mirex

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 425231
Conc: 0.77 ng/ml

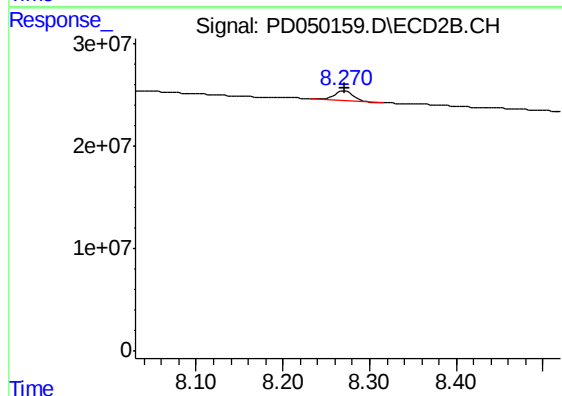

#22 Mirex


R.T.: 8.272 min
Delta R.T.: 0.000 min
Response: 13812815
Conc: 0.94 ng/ml

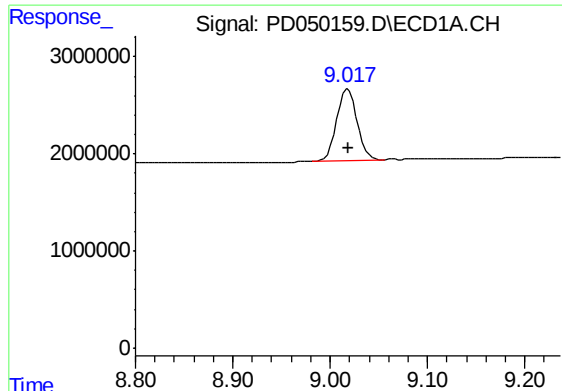

#28 Decachlorobiphenyl

R.T.: 9.018 min
Delta R.T.: 0.000 min
Response: 10828128
Conc: 17.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-S-02

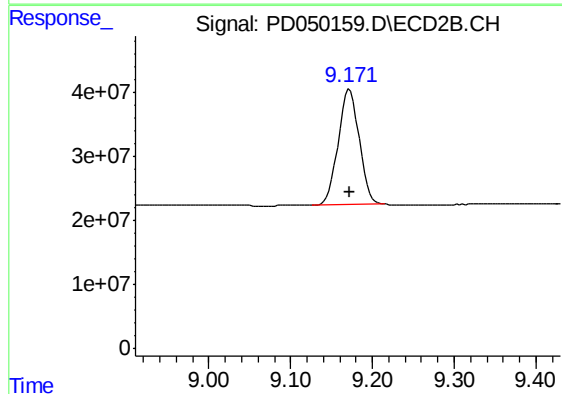

#28 Decachlorobiphenyl

R.T.: 9.172 min
Delta R.T.: 0.000 min
Response: 324430651
Conc: 18.75 ng/ml