

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
 Data File : PD050160.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2018 21:12
 Operator : AJ\SJ
 Sample : MIREX-MDL-S-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MIREX-MDL-S-03

Manual Integrations
 APPROVED

Sohil
 11/2/2018 6:25:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 05:38:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.234	4.061	10735105	472.0E6	16.564	16.983
28)	SA Decachlor...	9.019	9.173	10400989	316.1E6	17.198	18.265
Target Compounds							
22)	Mirex	8.160	8.273	414672	13399292	0.746m	0.913

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
Data File : PD050160.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 21:12
Operator : AJ\SJ
Sample : MIREX-MDL-S-03
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-S-03


Manual Integrations
APPROVED

Sohil
11/2/2018 6:25:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 05:38:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

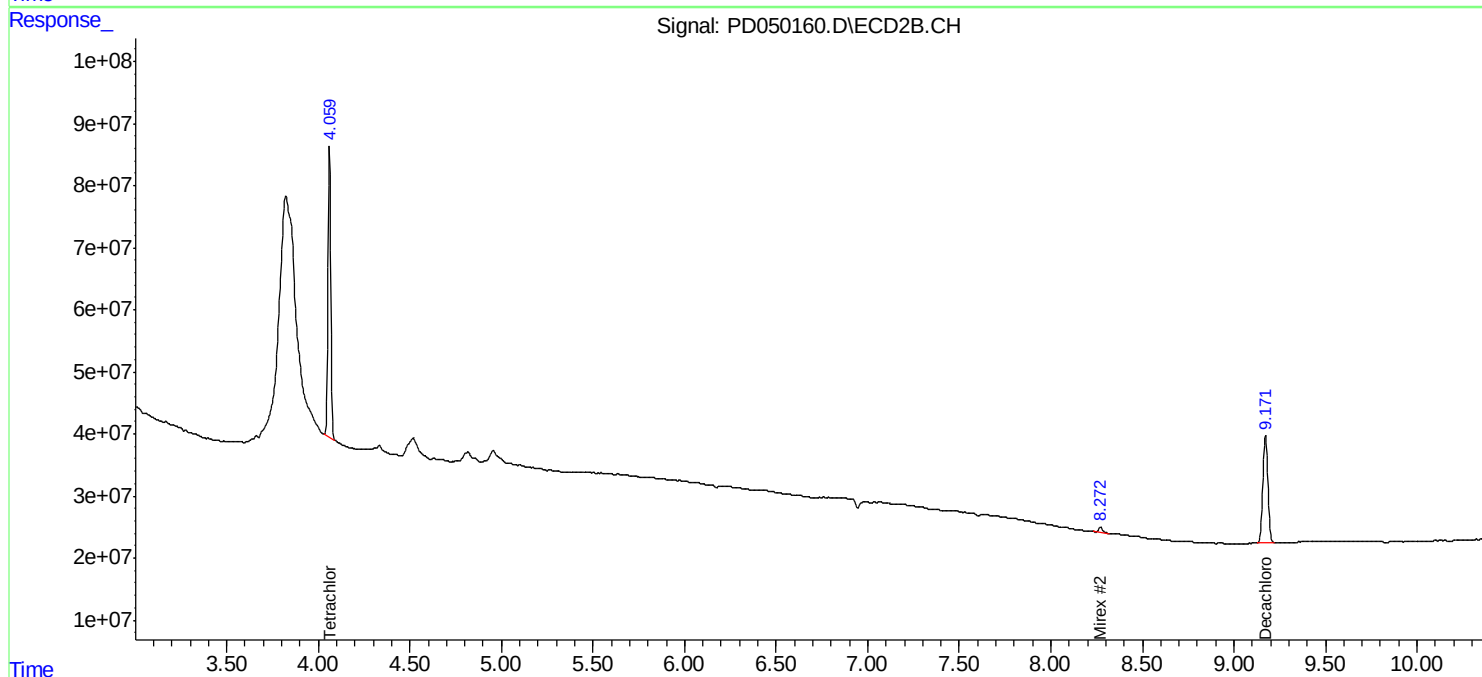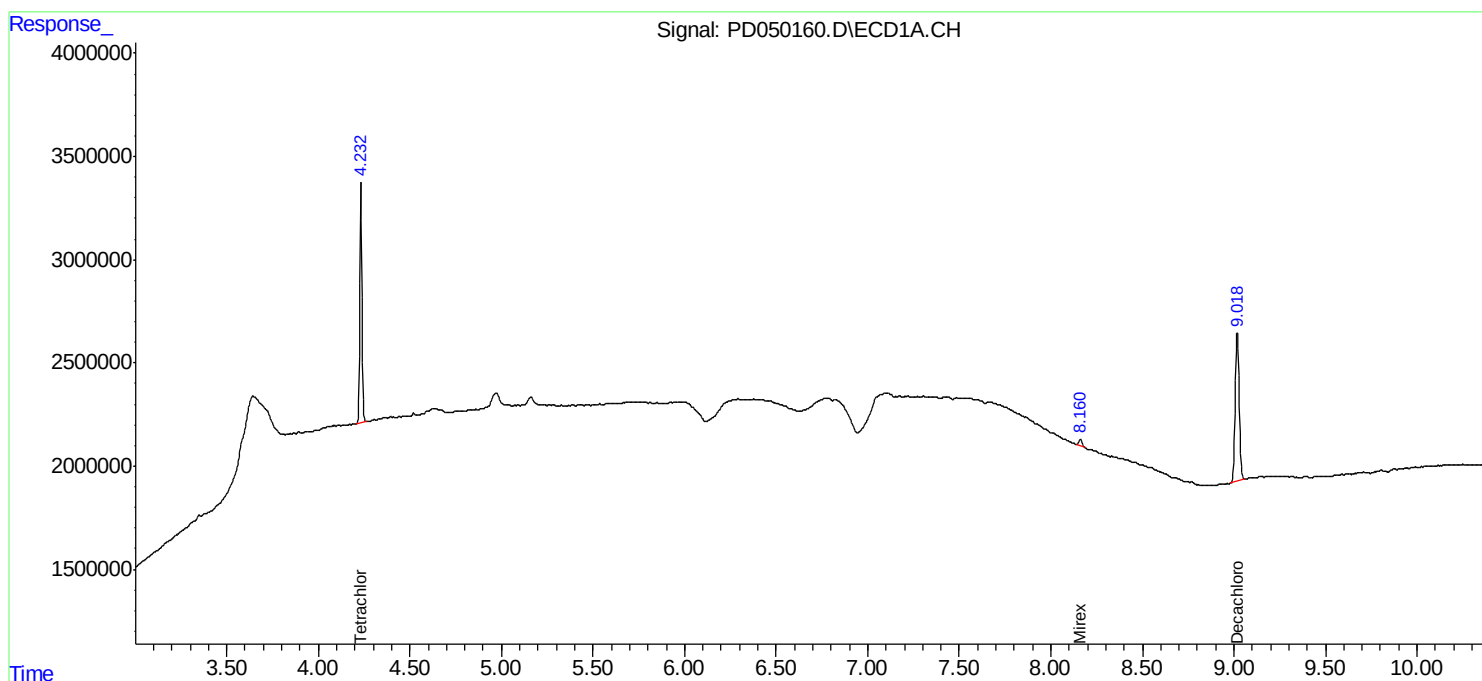

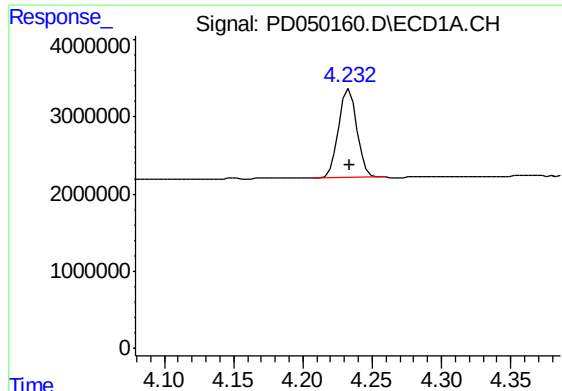


#1 Tetrachloro-m-xylene

R.T.: 4.234 min
Delta R.T.: 0.000 min
Response: 10735105
Conc: 16.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-S-03


Manual Integrations
APPROVED

Sohil
11/2/2018 6:25:22 PM

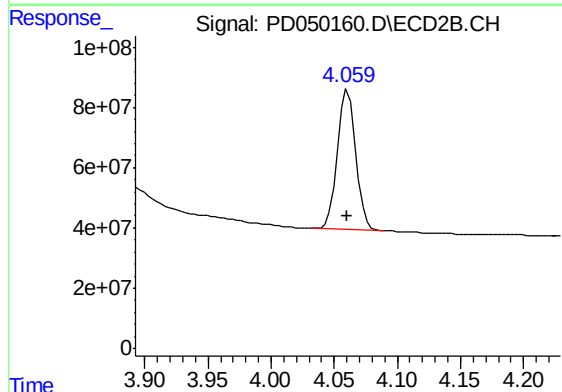


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 471990059
Conc: 16.98 ng/ml

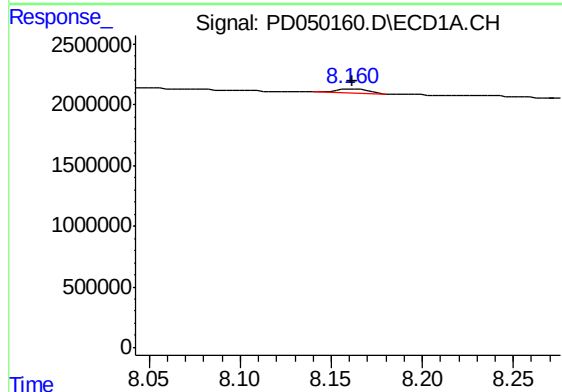


#22 Mirex

R.T.: 8.160 min
Delta R.T.: -0.001 min
Response: 414672
Conc: 0.75 ng/ml m

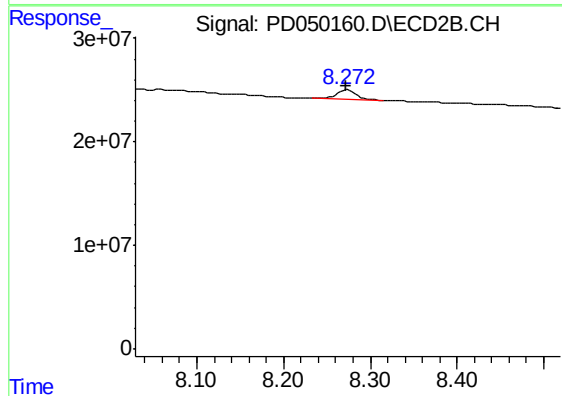

#22 Mirex

R.T.: 8.273 min
Delta R.T.: 0.001 min
Response: 13399292
Conc: 0.91 ng/ml

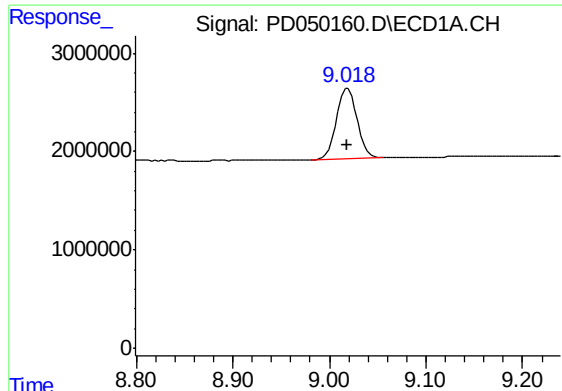


#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 10400989
Conc: 17.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-S-03

Manual Integrations
APPROVED

Sohil
11/2/2018 6:25:22 PM

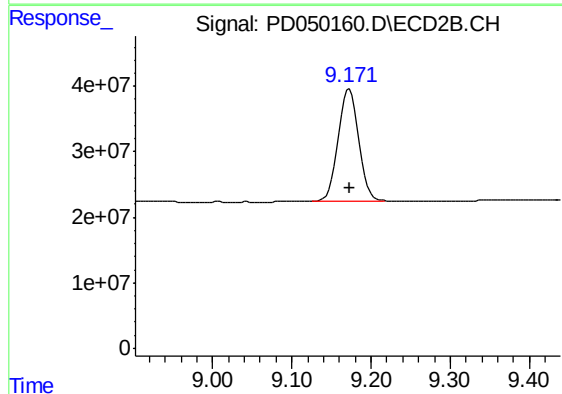

#28 Decachlorobiphenyl

R.T.: 9.173 min
Delta R.T.: 0.000 min
Response: 316086167
Conc: 18.27 ng/ml