

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
 Data File : PD050163.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2018 21:53
 Operator : AJ\SJ
 Sample : MIREX-MDL-W-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MIREX-MDL-W-02

Manual Integrations
 APPROVED

Sohil
 11/2/2018 6:25:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 05:38:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.061	11077700	487.4E6	17.093	17.536
28)	SA Decachlor...	9.019	9.172	11225069	332.1E6	18.560	19.189
Target Compounds							
22)	Mirex	8.160	8.270	424490	15027254	0.764m	1.024m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
Data File : PD050163.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 21:53
Operator : AJ\SJ
Sample : MIREX-MDL-W-02
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-W-02


Manual Integrations
APPROVED

Sohil
11/2/2018 6:25:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 05:38:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

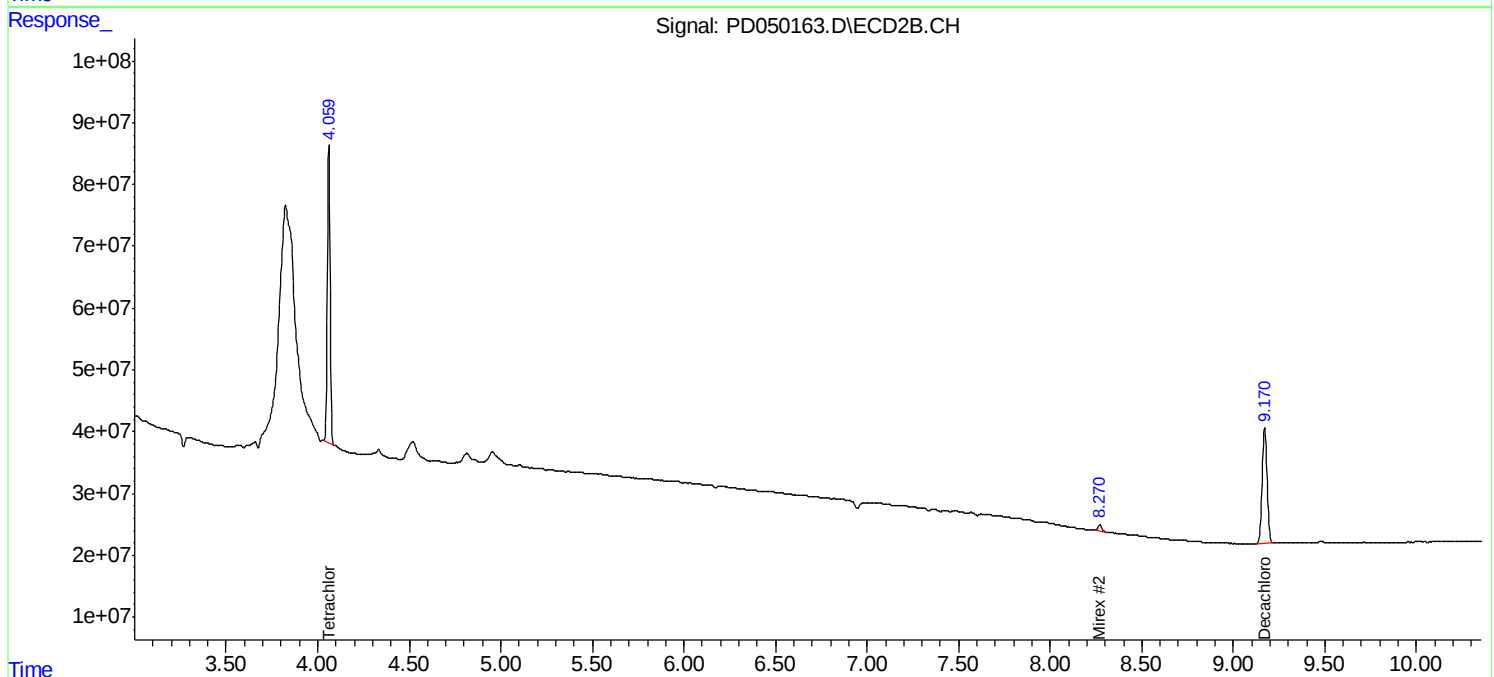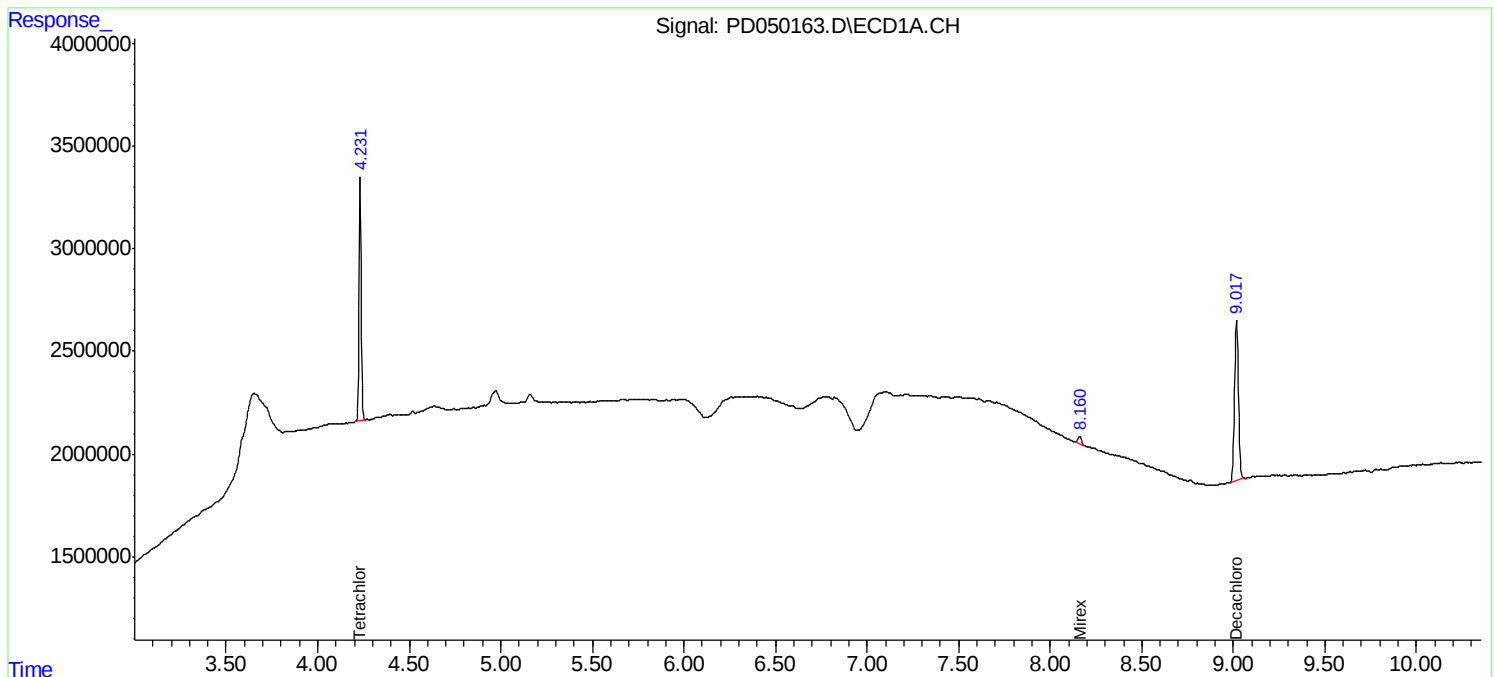

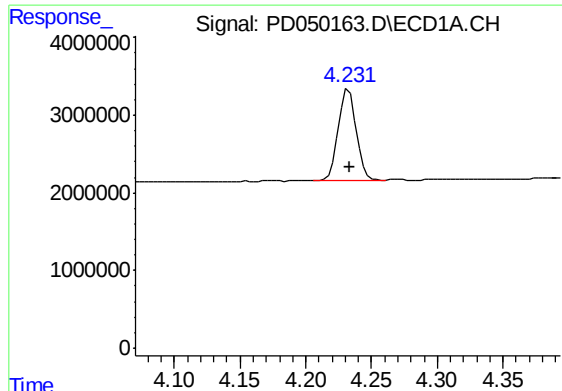


#1 Tetrachloro-m-xylene

R.T.: 4.233 min
Delta R.T.: -0.001 min
Response: 11077700
Conc: 17.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-W-02


Manual Integrations
APPROVED

Sohil
11/2/2018 6:25:24 PM

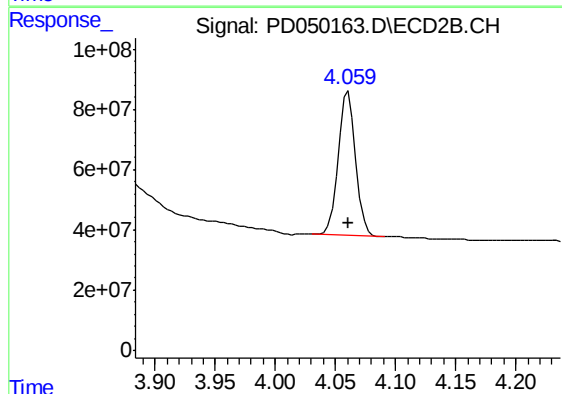


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 487360774
Conc: 17.54 ng/ml

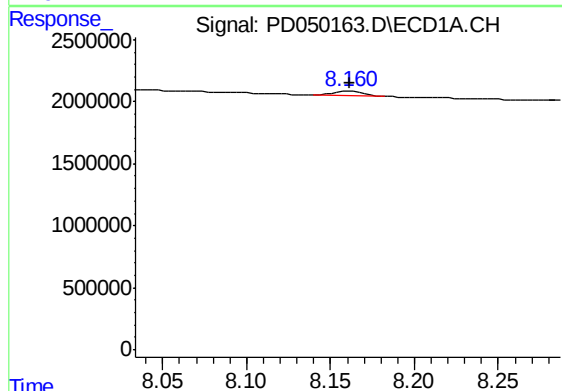


#22 Mirex

R.T.: 8.160 min
Delta R.T.: -0.001 min
Response: 424490
Conc: 0.76 ng/ml m

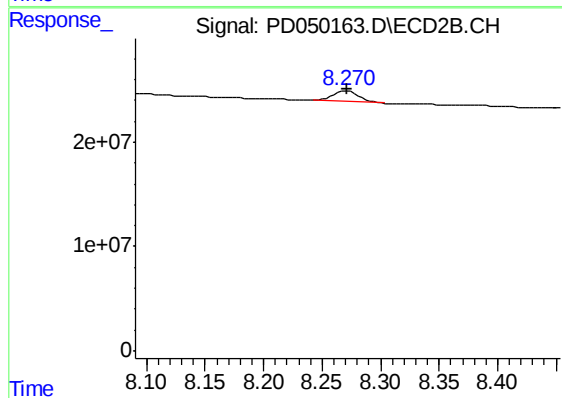

#22 Mirex

R.T.: 8.270 min
Delta R.T.: -0.001 min
Response: 15027254
Conc: 1.02 ng/ml m

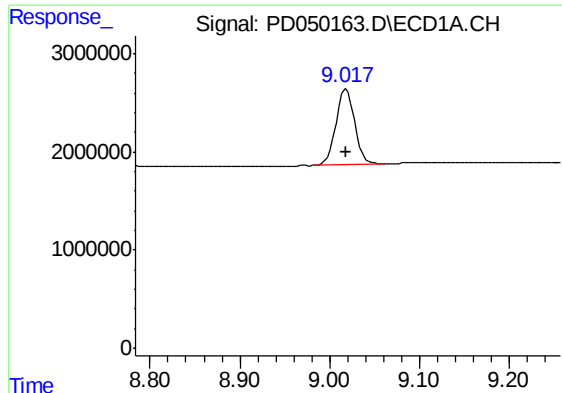


#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 11225069
Conc: 18.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-W-02

Manual Integrations
APPROVED

Sohil
11/2/2018 6:25:24 PM

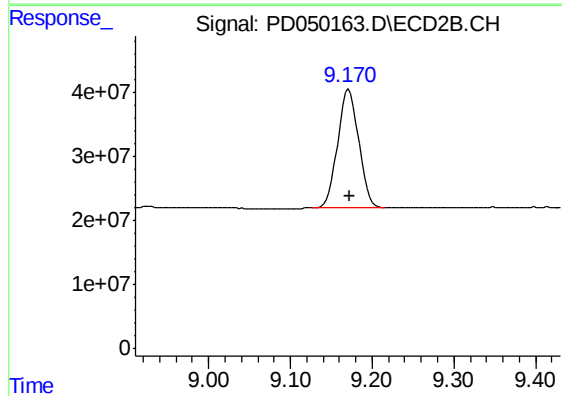

#28 Decachlorobiphenyl

R.T.: 9.172 min
Delta R.T.: 0.000 min
Response: 332076844
Conc: 19.19 ng/ml