

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
 Data File : PD050164.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2018 22:07
 Operator : AJ\SJ
 Sample : MIREX-MDL-W-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MIREX-MDL-W-03

Manual Integrations
 APPROVED

Sohil
 11/2/2018 6:25:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 05:38:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.234	4.061	11068633	488.3E6	17.079	17.569
28)	SA Decachlor...	9.020	9.173	11001649	327.2E6	18.191	18.908
Target Compounds							
22)	Mirex	8.161	8.273	418937	14514181	0.754m	0.989 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
Data File : PD050164.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 22:07
Operator : AJ\SJ
Sample : MIREX-MDL-W-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-W-03


Manual Integrations
APPROVED

Sohil
11/2/2018 6:25:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 05:38:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

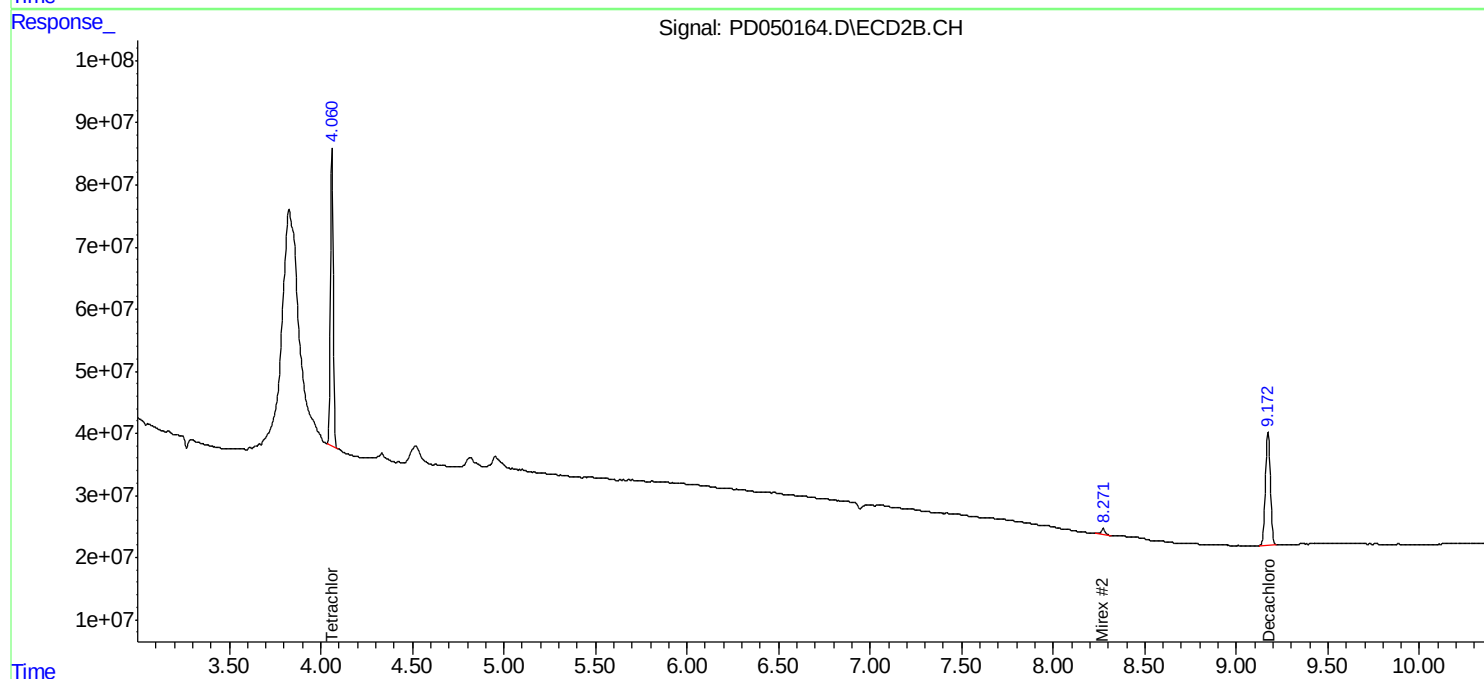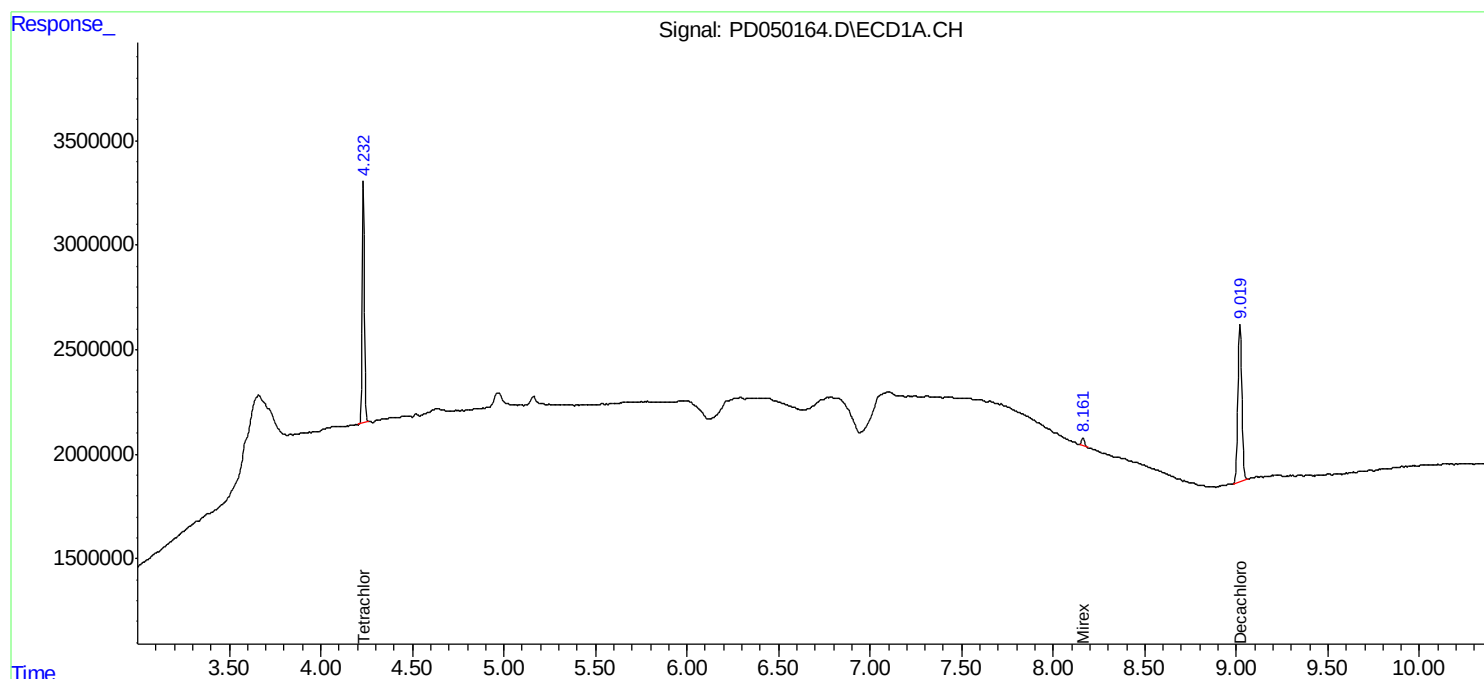

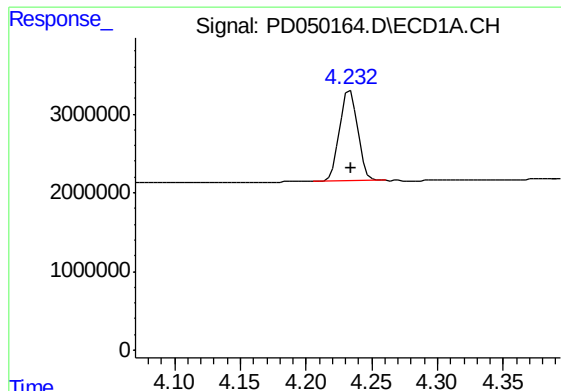


#1 Tetrachloro-m-xylene

R.T.: 4.234 min
Delta R.T.: 0.000 min
Response: 11068633
Conc: 17.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-W-03


Manual Integrations
APPROVED

Sohil
11/2/2018 6:25:25 PM

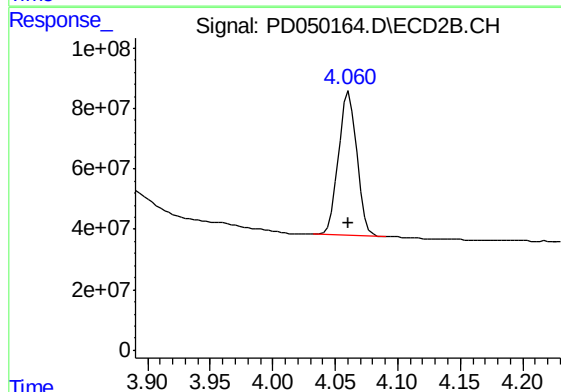


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 488268764
Conc: 17.57 ng/ml

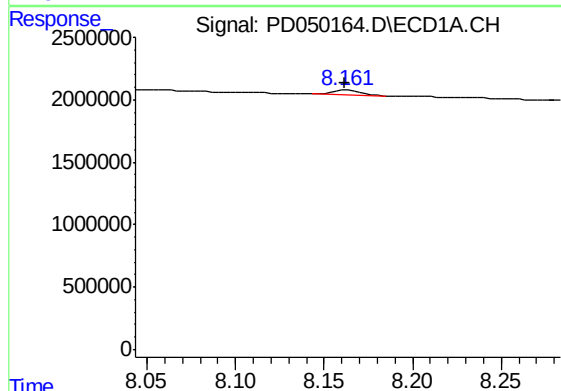


#22 Mirex

R.T.: 8.161 min
Delta R.T.: 0.000 min
Response: 418937
Conc: 0.75 ng/ml m

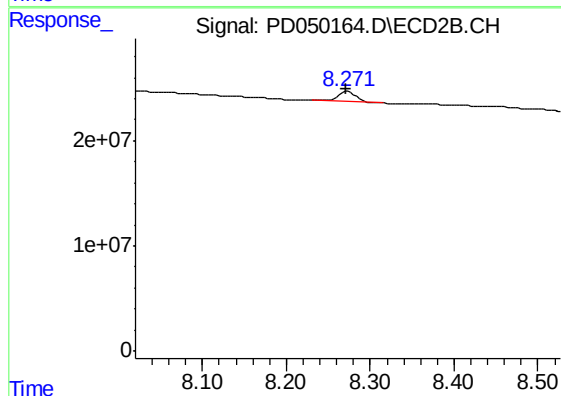

#22 Mirex

R.T.: 8.273 min
Delta R.T.: 0.001 min
Response: 14514181
Conc: 0.99 ng/ml

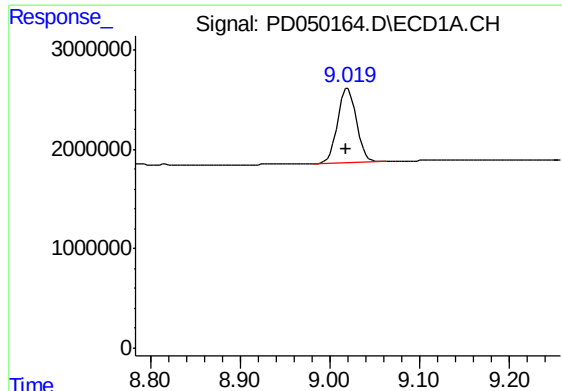


#28 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.002 min
Response: 11001649
Conc: 18.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
MIREX-MDL-W-03

Manual Integrations
APPROVED

Sohil
11/2/2018 6:25:25 PM

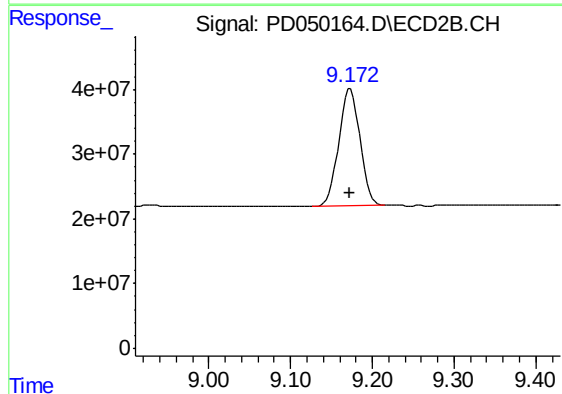

#28 Decachlorobiphenyl

R.T.: 9.173 min
Delta R.T.: 0.000 min
Response: 327204044
Conc: 18.91 ng/ml