

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
 Data File : PD050166.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2018 22:35
 Operator : AJ\SJ
 Sample : PSTDCCC050
 Misc : FOR MIREX
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 05:39:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.061	32201981	1336.7E6	49.687	48.098
28)	SA Decachlor...	9.018	9.173	30712120	845.2E6	50.782	48.839
Target Compounds							
22)	Mirex	8.163	8.274	28338437	729.9E6	50.992	49.723



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110218\
Data File : PD050166.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 22:35
Operator : AJ\SJ
Sample : PSTDCCC050
Misc : FOR MIREX
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 05:39:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

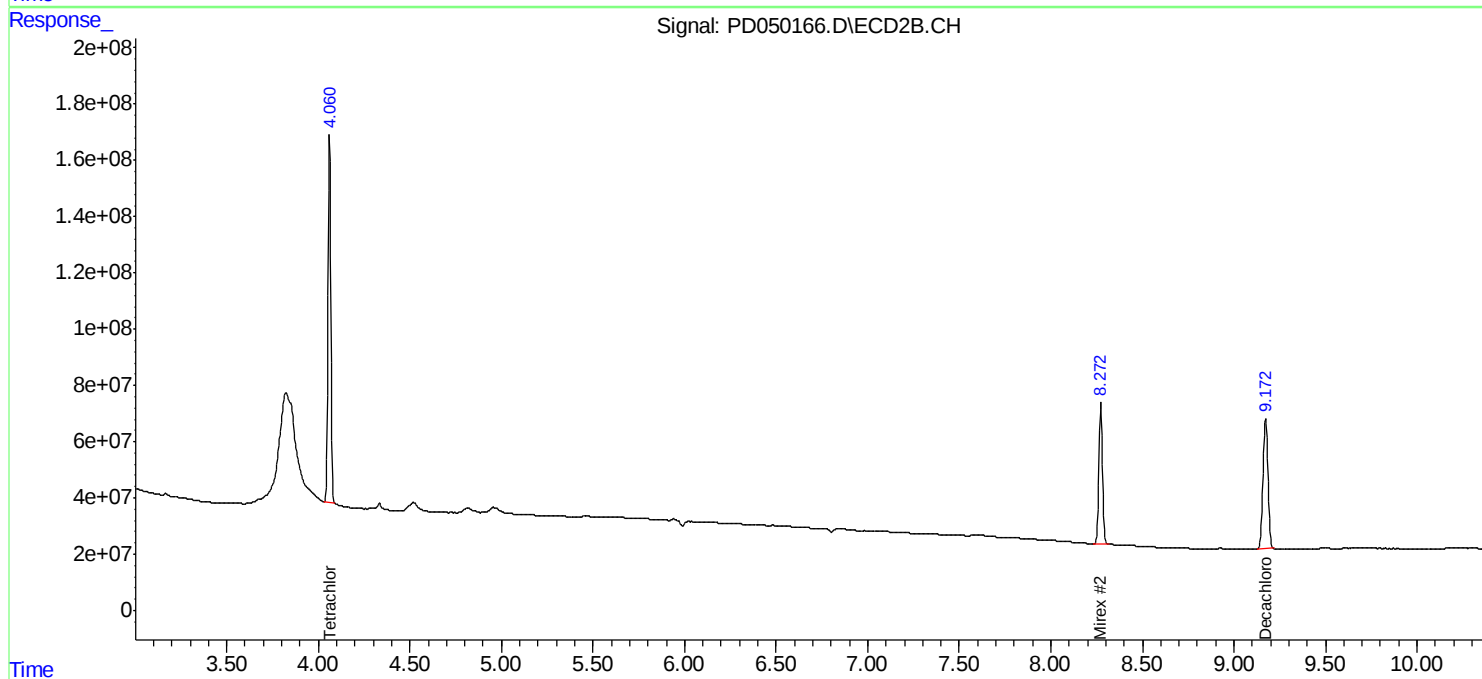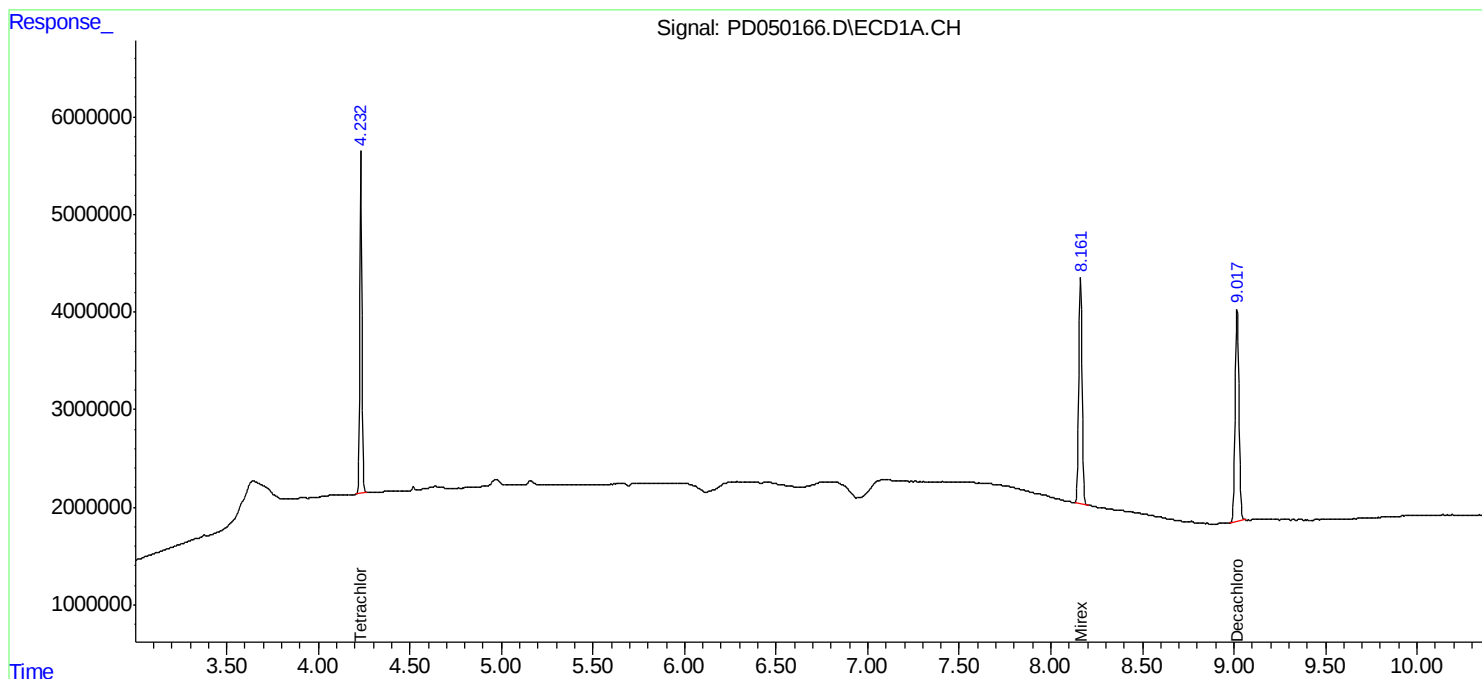


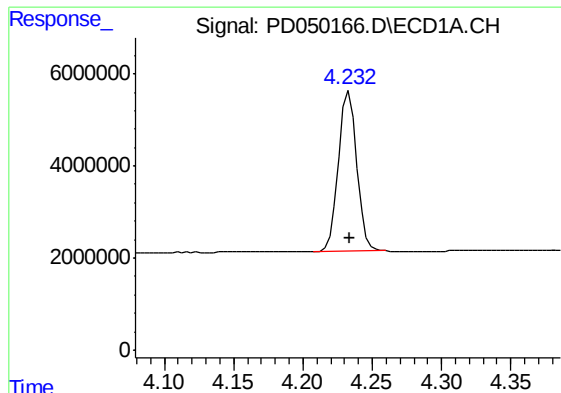

#1 Tetrachloro-m-xylene


R.T.: 4.233 min
Delta R.T.: 0.000 min
Response: 32201981
Conc: 49.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

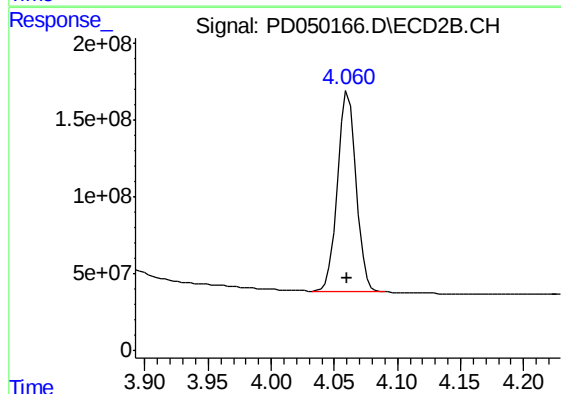


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 1336740943
Conc: 48.10 ng/ml

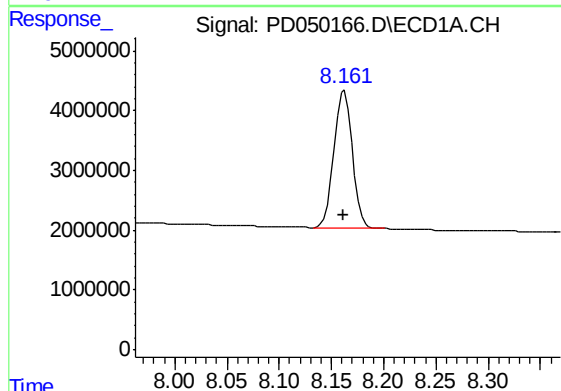


#22 Mirex

R.T.: 8.163 min
Delta R.T.: 0.000 min
Response: 28338437
Conc: 50.99 ng/ml

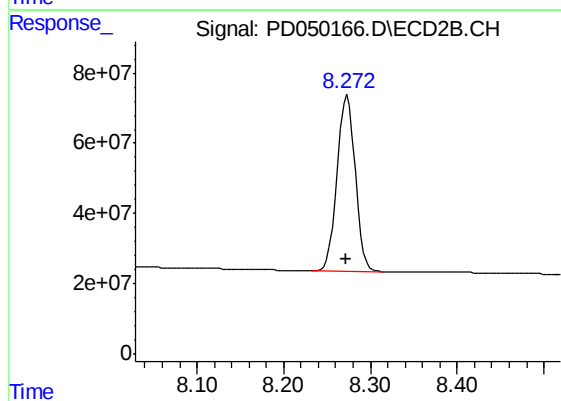

#22 Mirex


R.T.: 8.274 min
Delta R.T.: 0.002 min
Response: 729905643
Conc: 49.72 ng/ml

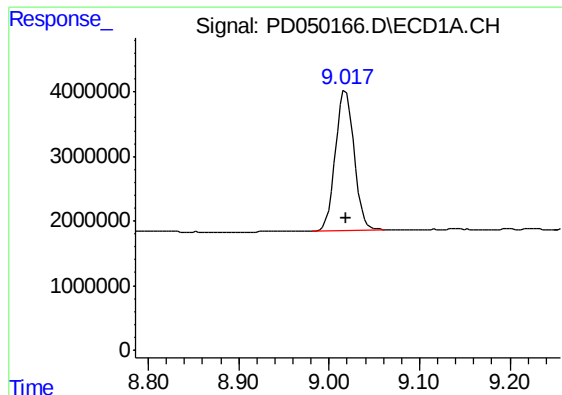

#28 Decachlorobiphenyl

R.T.: 9.018 min
Delta R.T.: 0.000 min
Response: 30712120
Conc: 50.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

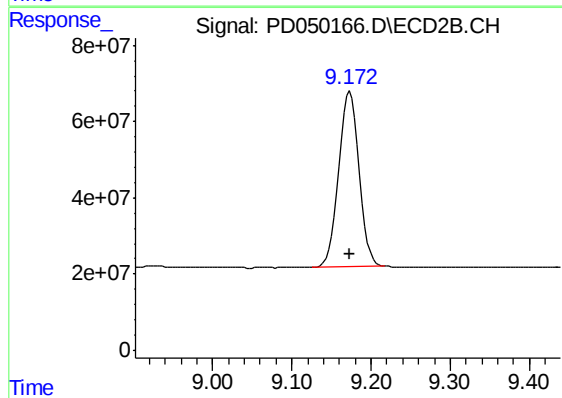

#28 Decachlorobiphenyl

R.T.: 9.173 min
Delta R.T.: 0.001 min
Response: 845170611
Conc: 48.84 ng/ml