

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110219\
 Data File : PD055790.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 11:12
 Operator : SG\AJ
 Sample : K5111-03
 Misc : CHLOR MDL 25 PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 11:51:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:48:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.962	16026965	23425678	18.800	19.451
28)	SA Decachlor...	7.964	8.999	17924978	26540282	18.947	19.072
Target Compounds							
10)	B gamma-Chl...	0.000	6.059	0	5604048	N.D.	3.251 #
11)	B alpha-Chl...	0.000	6.132	0	6888535	N.D.	4.010 #
25)	Chlordane-3	0.000	6.059	0	5604048	N.D.	25.592 #
26)	Chlordane-4	0.000	6.132	0	6888535	N.D.	26.187 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110219\
Data File : PD055790.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 11:12
Operator : SG\AJ
Sample : K5111-03
Misc : CHLOR MDL 25 PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 11:51:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:48:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

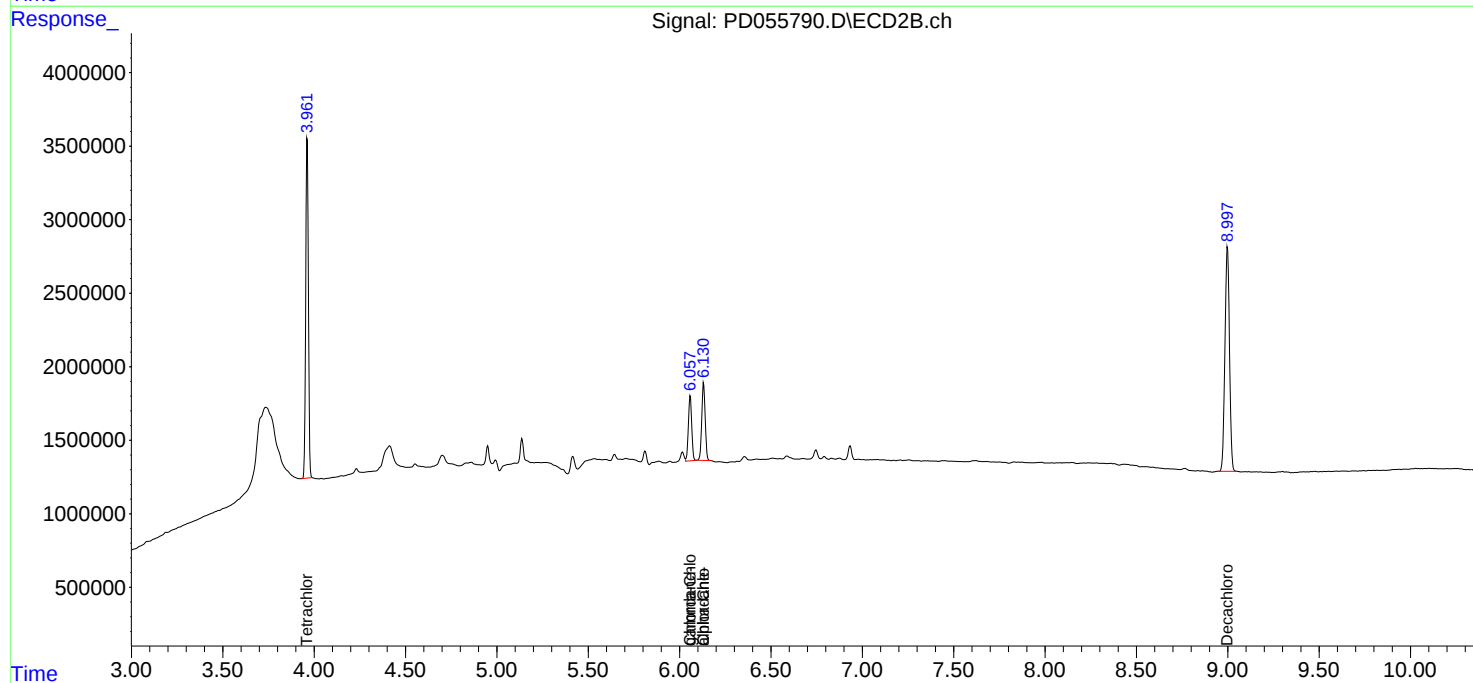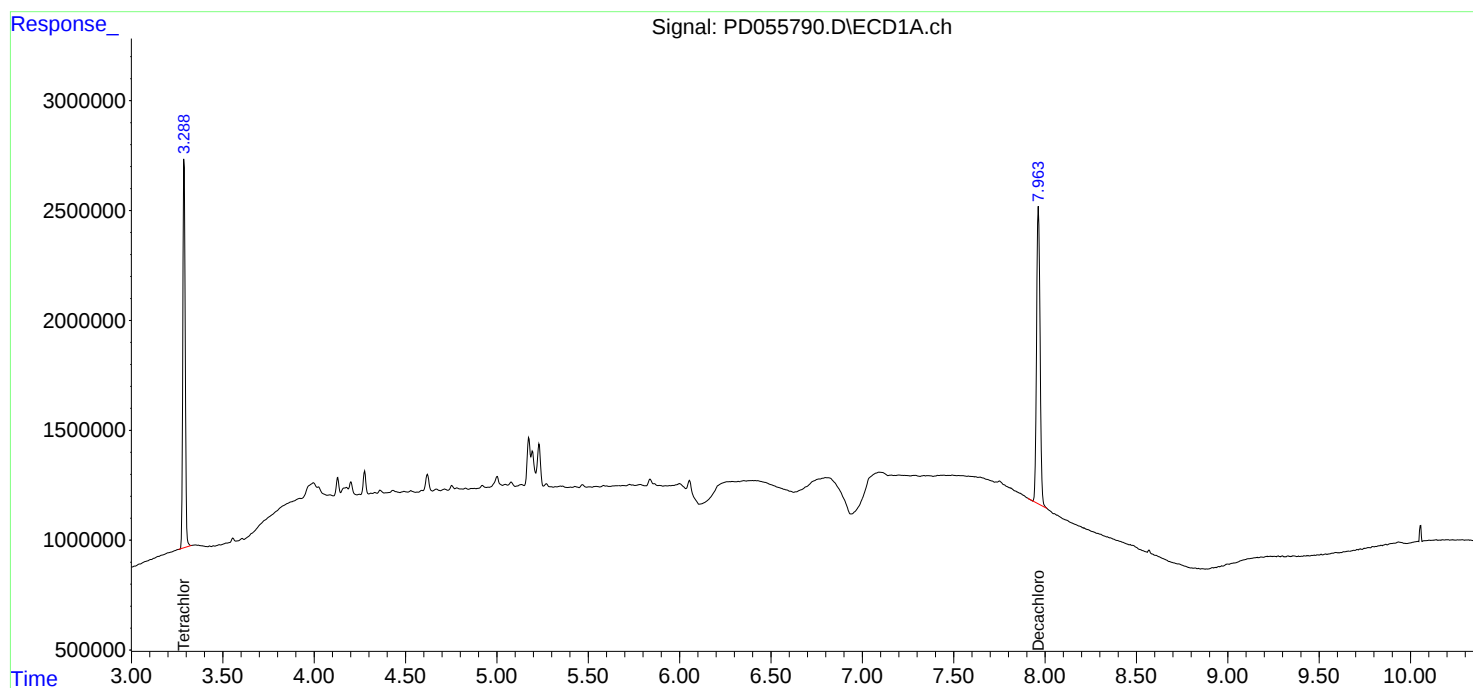


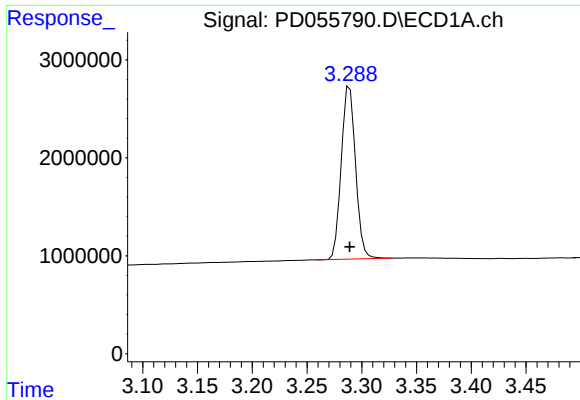

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 16026965
Conc: 18.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

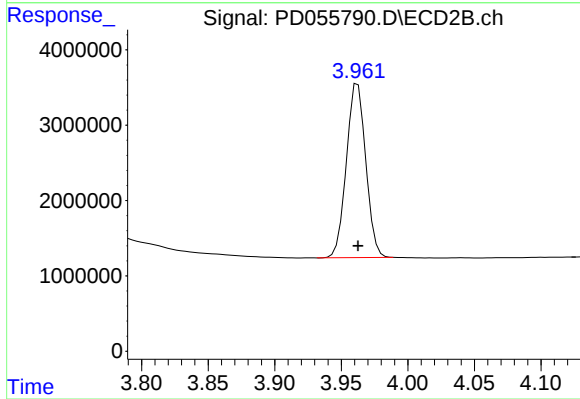


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 23425678
Conc: 19.45 ng/ml

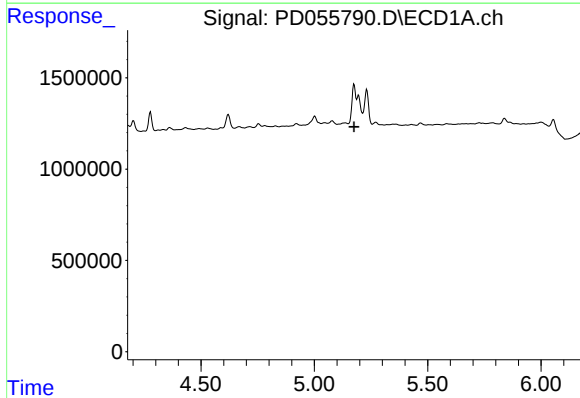


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.176 min
Response: 0
Conc: N.D.

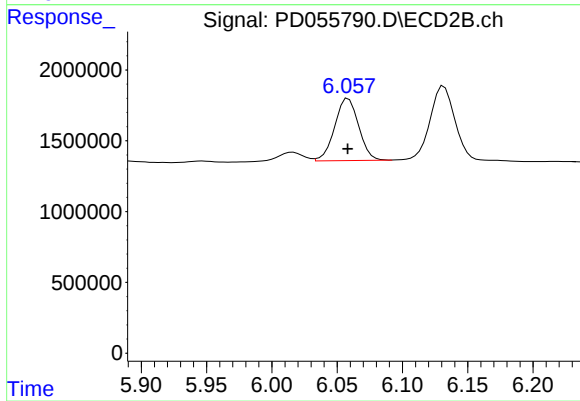

#10 gamma-Chlordane


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 5604048
Conc: 3.25 ng/ml

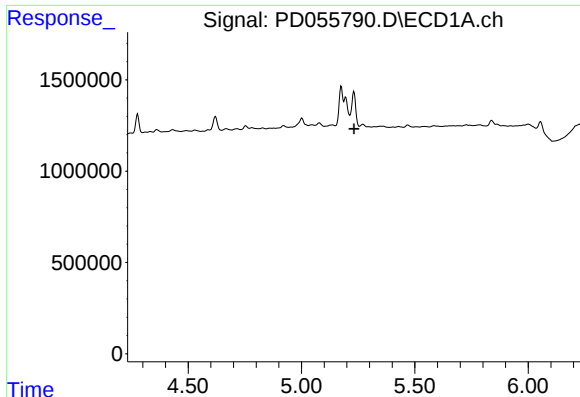

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

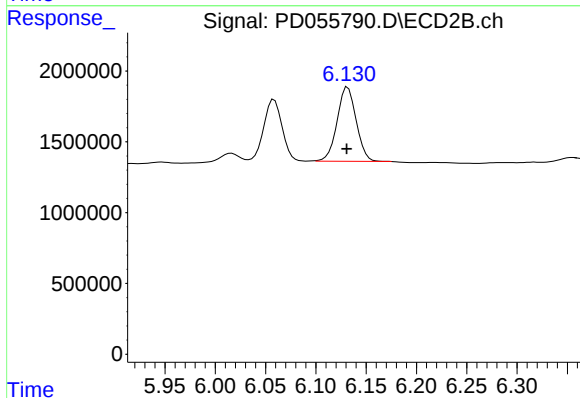


#11 alpha-Chlordane

R.T.: 6.132 min
Delta R.T.: 0.000 min
Response: 6888535
Conc: 4.01 ng/ml

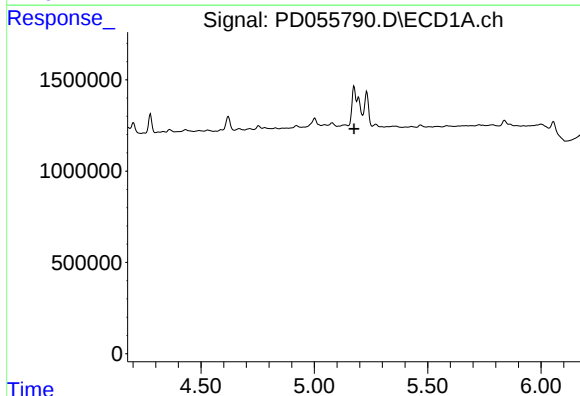


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.176 min
Response: 0
Conc: N.D.

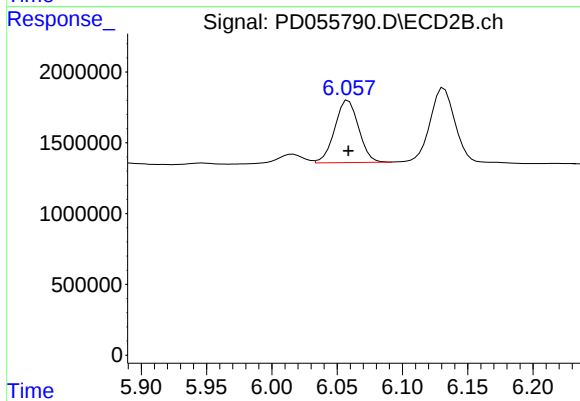

#25 Chlordane-3


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 5604048
Conc: 25.59 ng/ml

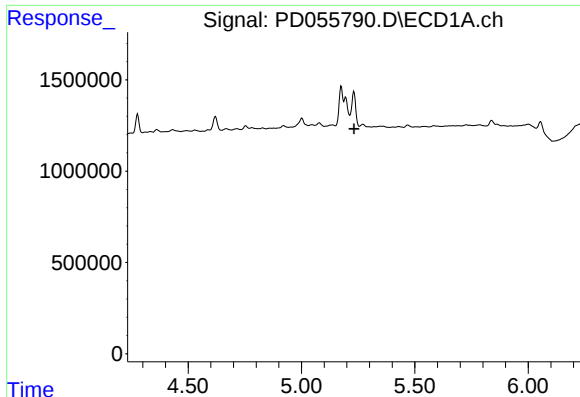

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

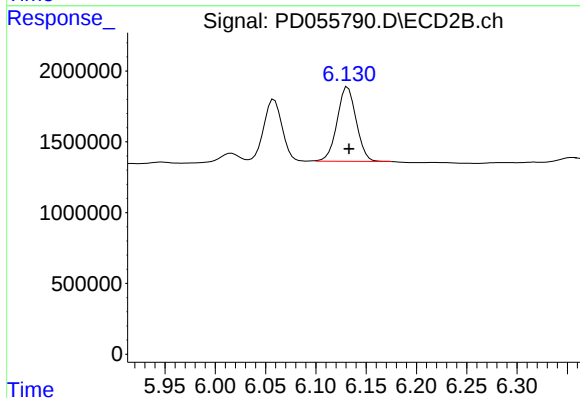


#26 Chlordane-4

R.T.: 6.132 min
Delta R.T.: -0.001 min
Response: 6888535
Conc: 26.19 ng/ml

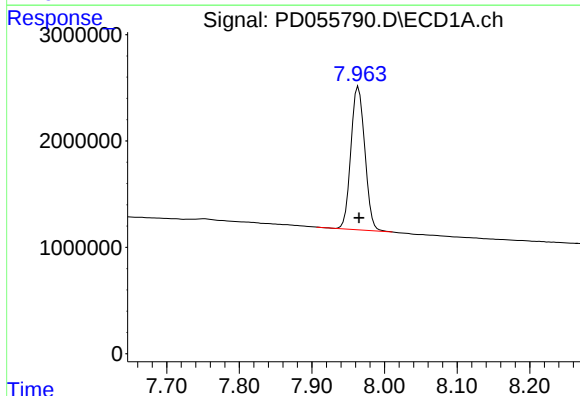

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 17924978
Conc: 18.95 ng/ml

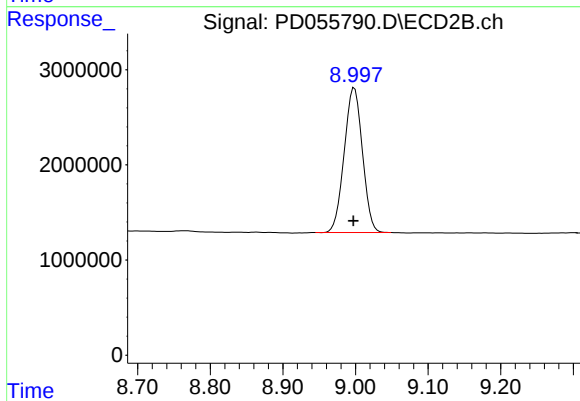

#28 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: 0.002 min
Response: 26540282
Conc: 19.07 ng/ml