

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110219\
 Data File : PD055791.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 11:26
 Operator : SG\AJ
 Sample : K5111-09
 Misc : CHLOR MDL 25 PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 11:51:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:48:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.962	15919040	23227709	18.673	19.287
28)	SA Decachlor...	7.964	8.998	18034761	26473854	19.063	19.024
Target Compounds							
10)	B gamma-Chl...	0.000	6.059	0	5556479	N.D.	3.223 #
11)	B alpha-Chl...	0.000	6.132	0	6801659	N.D.	3.959 #
25)	Chlordane-3	0.000	6.059	0	5556479	N.D.	25.374 #
26)	Chlordane-4	0.000	6.132	0	6801659	N.D.	25.857 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110219\
Data File : PD055791.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 11:26
Operator : SG\AJ
Sample : K5111-09
Misc : CHLOR MDL 25 PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 11:51:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:48:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

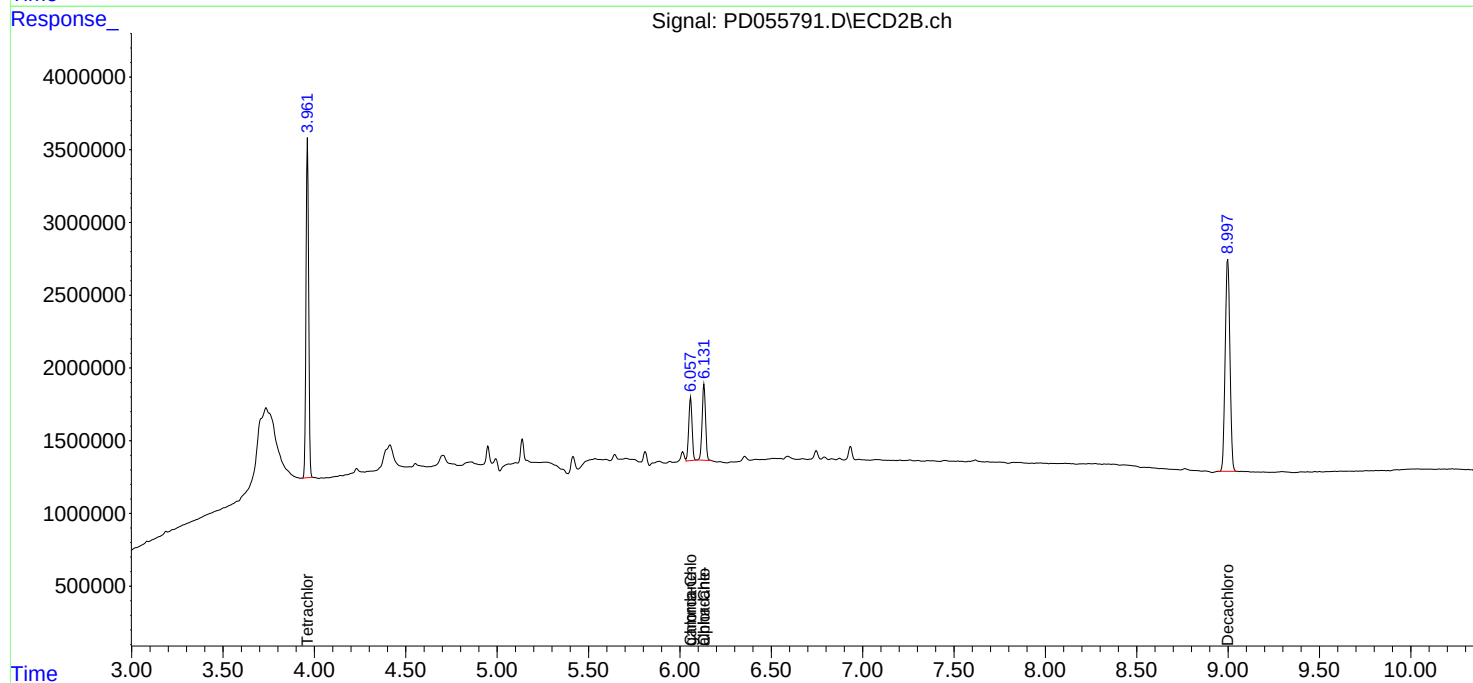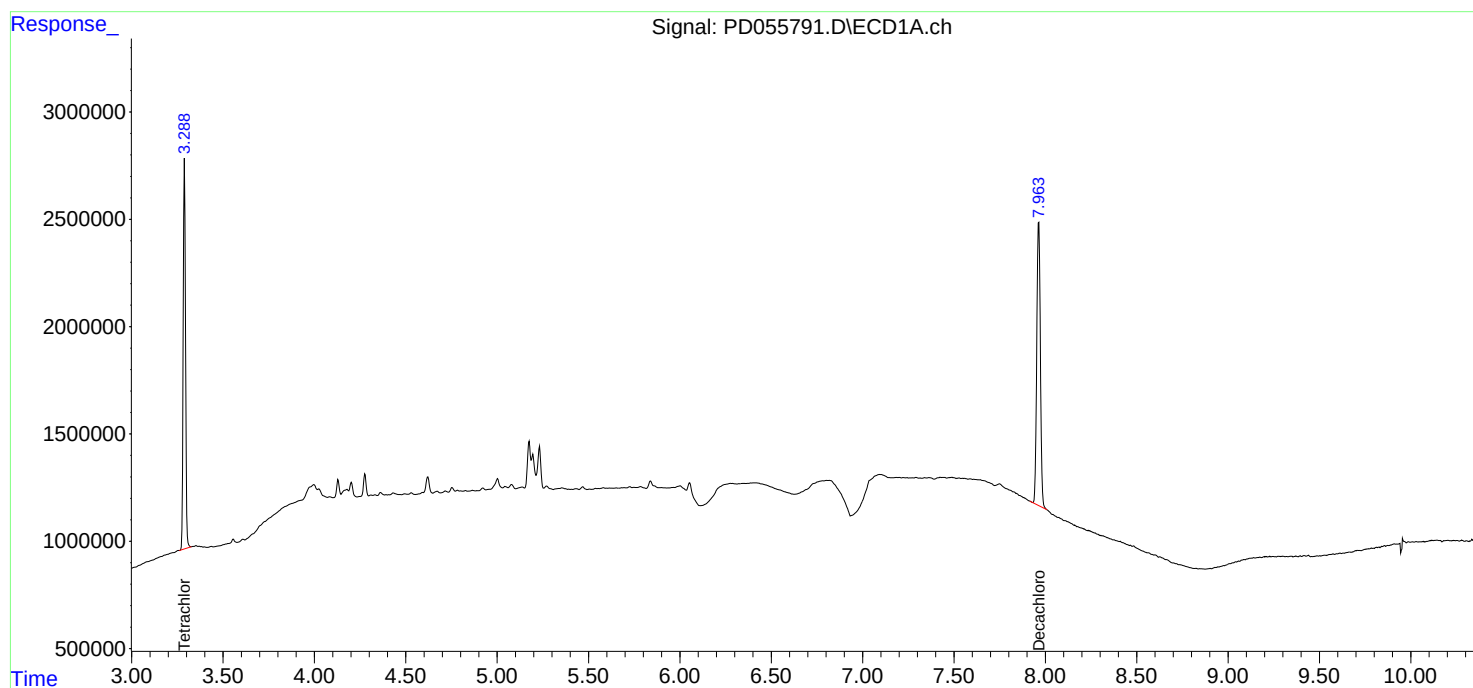


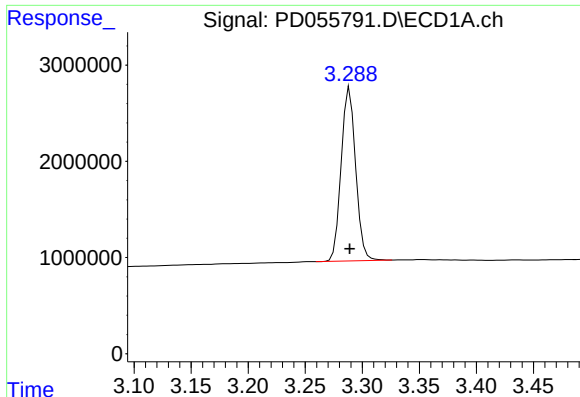

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 15919040
Conc: 18.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

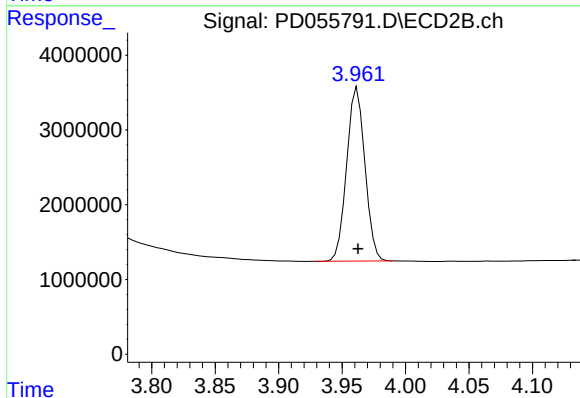


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 23227709
Conc: 19.29 ng/ml

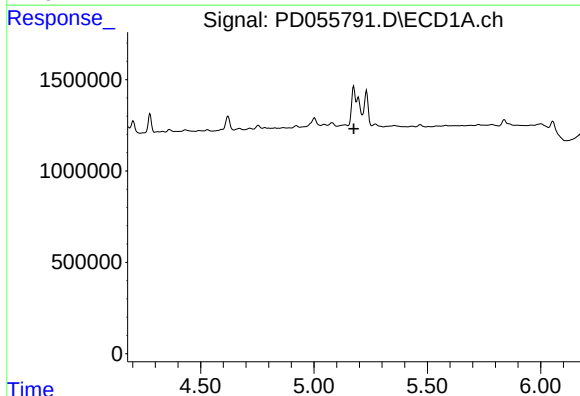


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.176 min
Response: 0
Conc: N.D.

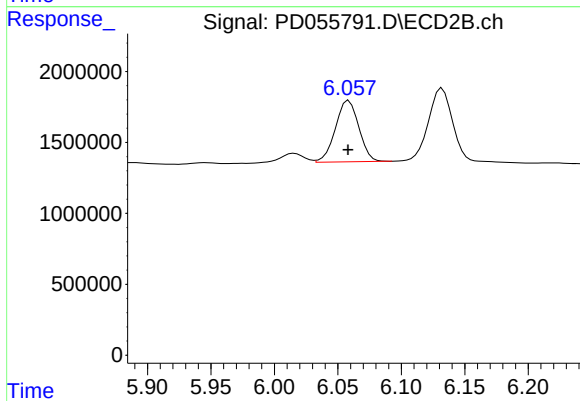

#10 gamma-Chlordane


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 5556479
Conc: 3.22 ng/ml

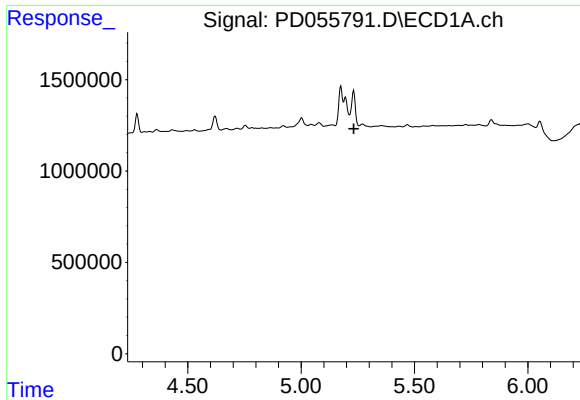

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

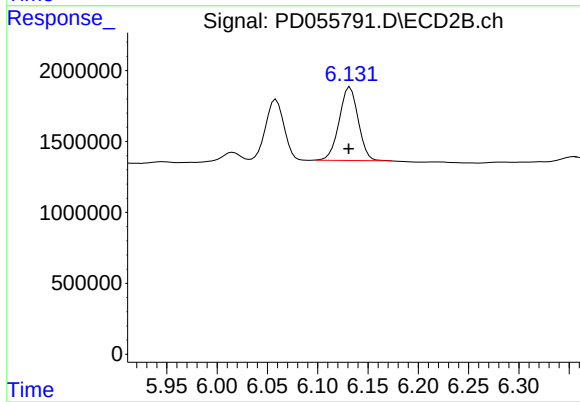


#11 alpha-Chlordane

R.T.: 6.132 min
Delta R.T.: 0.001 min
Response: 6801659
Conc: 3.96 ng/ml

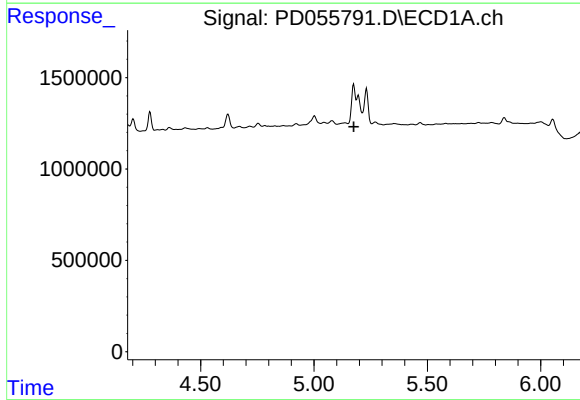


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.176 min
Response: 0
Conc: N.D.

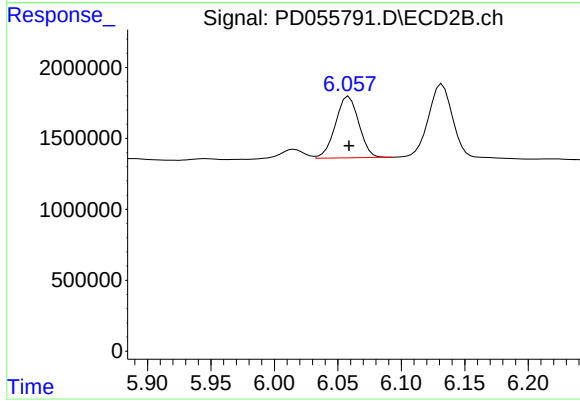

#25 Chlordane-3


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 5556479
Conc: 25.37 ng/ml

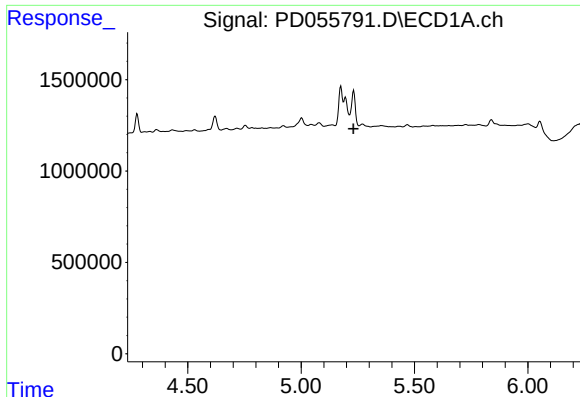

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

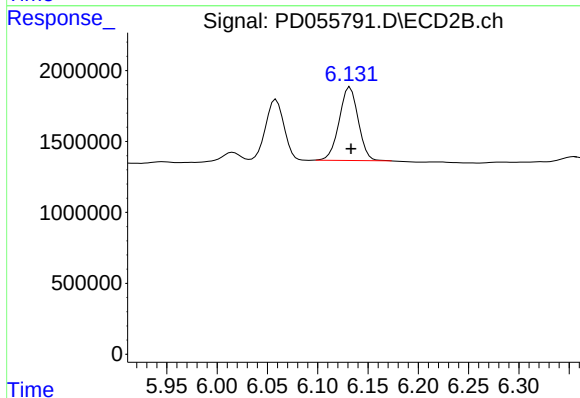


#26 Chlordane-4

R.T.: 6.132 min
Delta R.T.: 0.000 min
Response: 6801659
Conc: 25.86 ng/ml

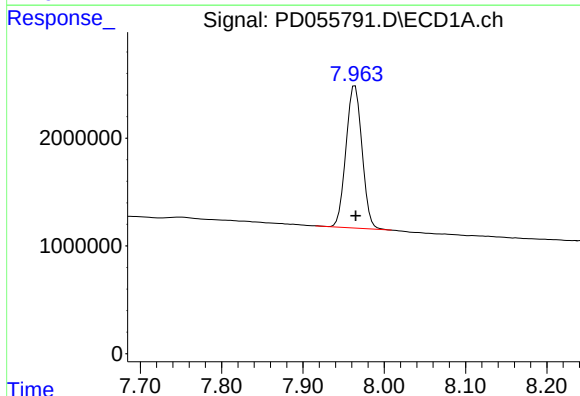

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 18034761
Conc: 19.06 ng/ml

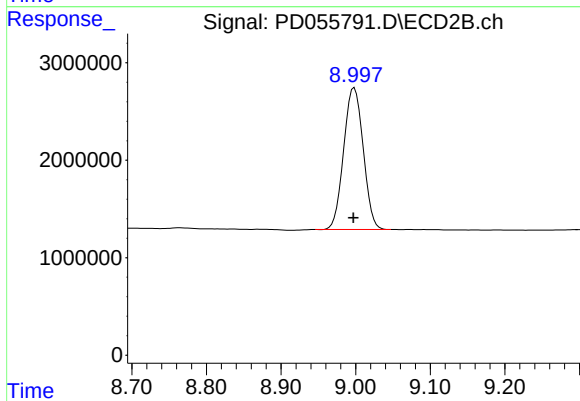

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.001 min
Response: 26473854
Conc: 19.02 ng/ml