

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110219\
 Data File : PD055795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 12:22
 Operator : SG\AJ
 Sample : K4839-11DL 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-CHLR-WPDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 12:54:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 31 06:48:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.962	12400935	14655314	14.546	12.169
28)	SA Decachlor...	7.964	8.998	12680129	18271789	13.403	13.130
Target Compounds							
23)	Chlordane-1	4.130	4.950	22598799	37688778	871.408	812.151
24)	Chlordane-2	4.621	5.416	25487053	39267402	801.424	747.527
25)	Chlordane-3	5.176	6.059	78206722	152.9E6	813.245	698.240
26)	Chlordane-4	5.233	6.133	69739009	180.4E6	829.264	685.847
27)	Chlordane-5	6.056	6.934	23235266	38266800	765.234	820.835



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110219\
Data File : PD055795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 12:22
Operator : SG\AJ
Sample : K4839-11DL 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 12:54:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110119.M
Quant Title : GC Extractables
QLast Update : Thu Oct 31 06:48:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

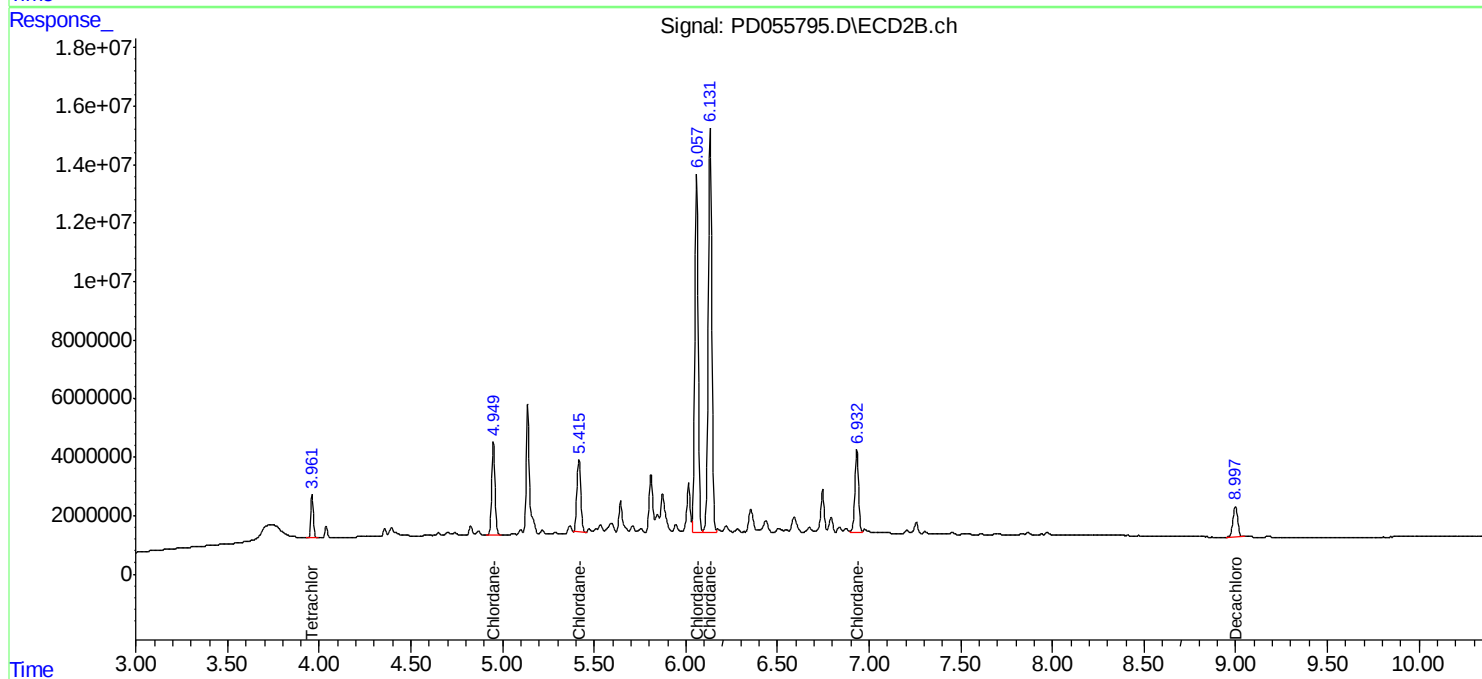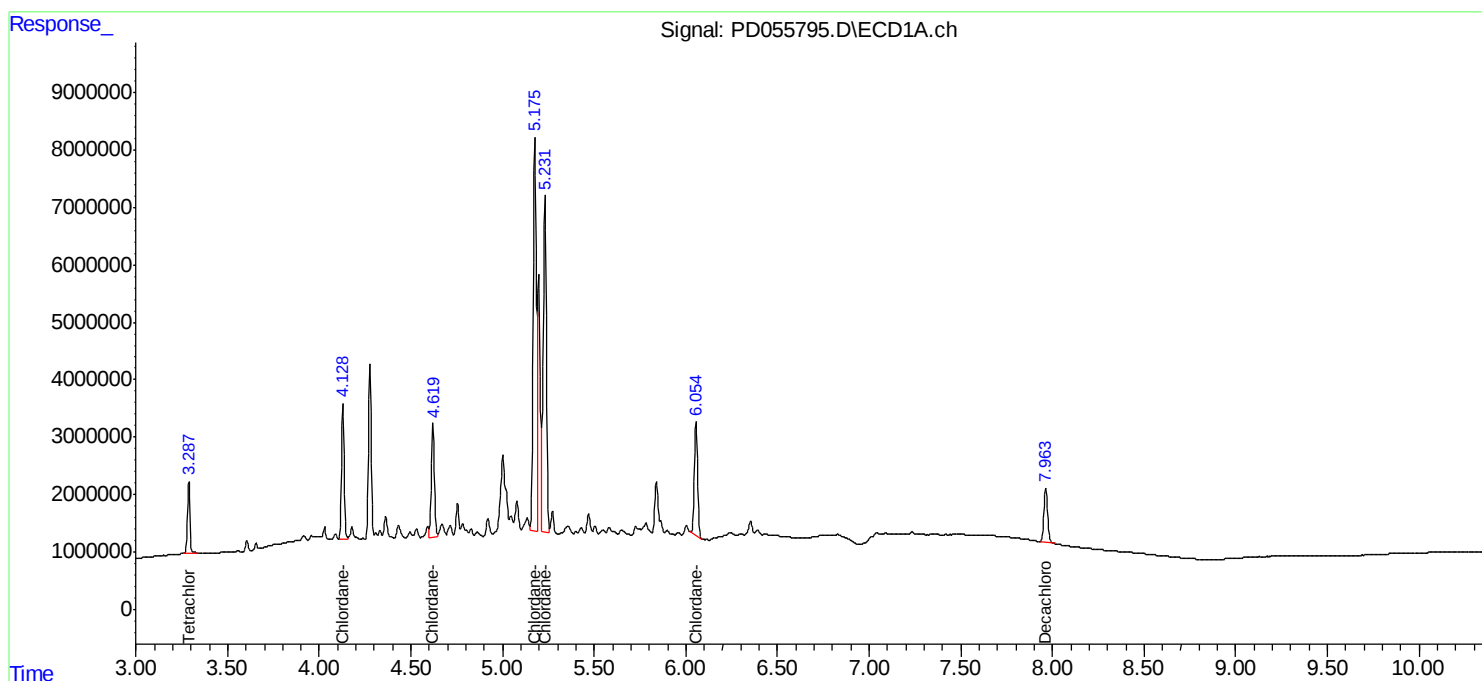


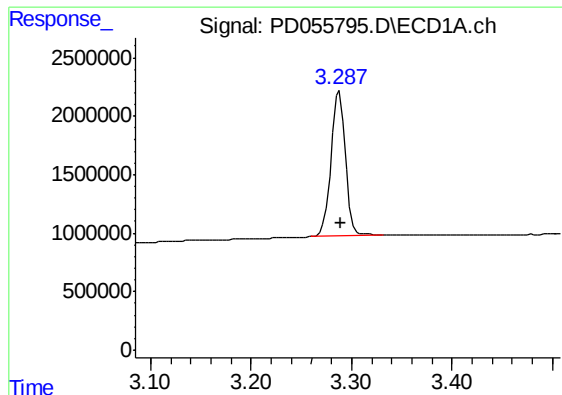

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 12400935
Conc: 14.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

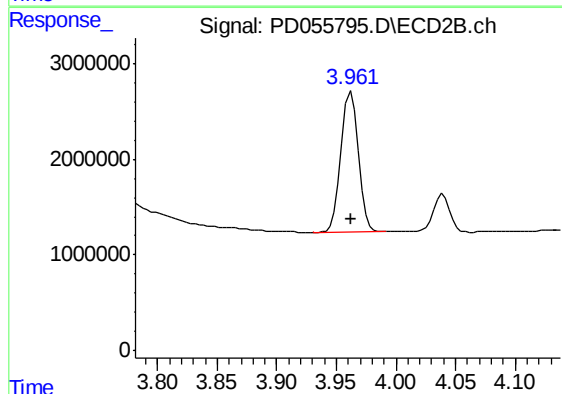


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 14655314
Conc: 12.17 ng/ml

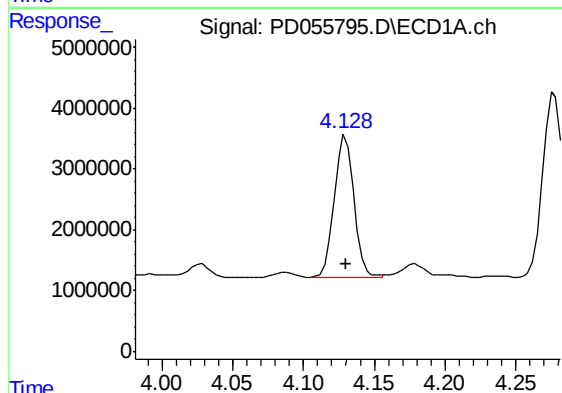


#23 Chlordane-1

R.T.: 4.130 min
Delta R.T.: 0.000 min
Response: 22598799
Conc: 871.41 ng/ml

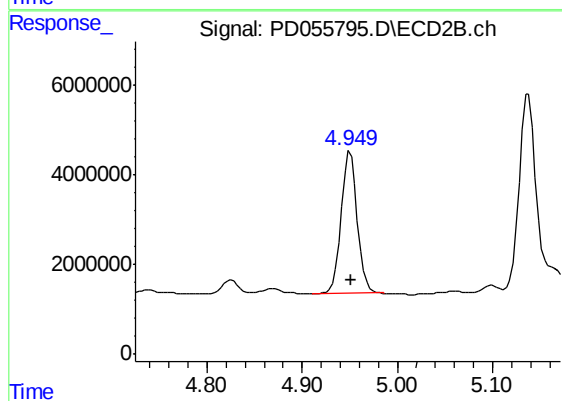

#23 Chlordane-1


R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 37688778
Conc: 812.15 ng/ml

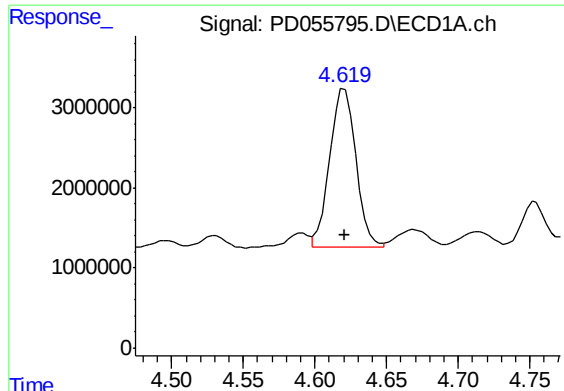

#24 Chlordane-2


R.T.: 4.621 min
Delta R.T.: 0.000 min
Response: 25487053
Conc: 801.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

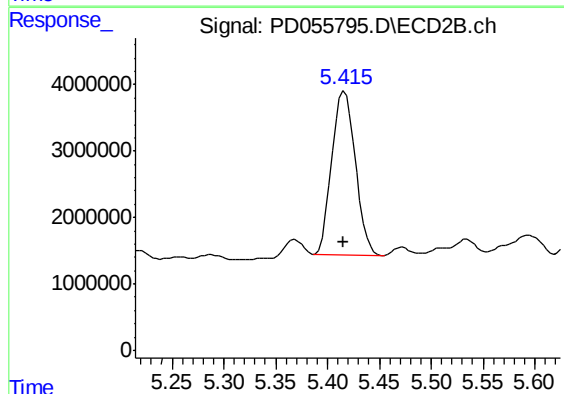


#24 Chlordane-2

R.T.: 5.416 min
Delta R.T.: 0.000 min
Response: 39267402
Conc: 747.53 ng/ml

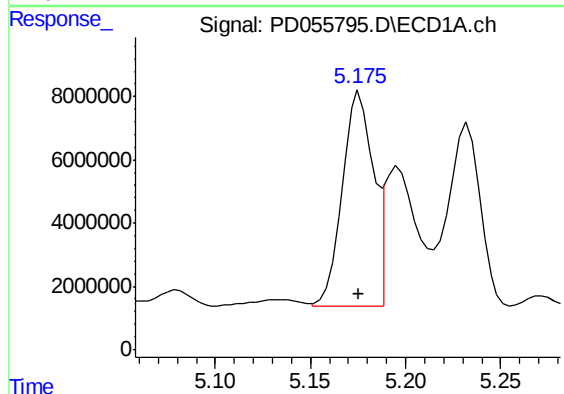


#25 Chlordane-3

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 78206722
Conc: 813.24 ng/ml

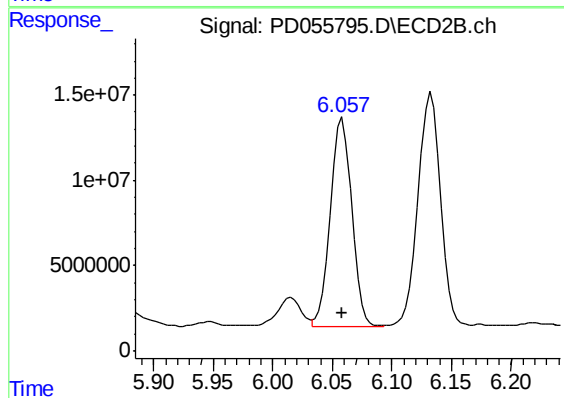

#25 Chlordane-3


R.T.: 6.059 min
Delta R.T.: 0.000 min
Response: 152900528
Conc: 698.24 ng/ml

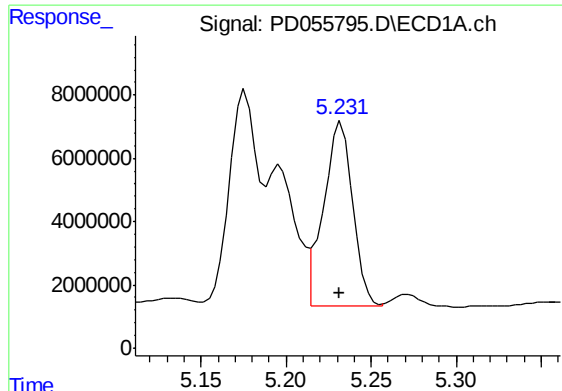

#26 Chlordane-4


R.T.: 5.233 min
Delta R.T.: 0.001 min
Response: 69739009
Conc: 829.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

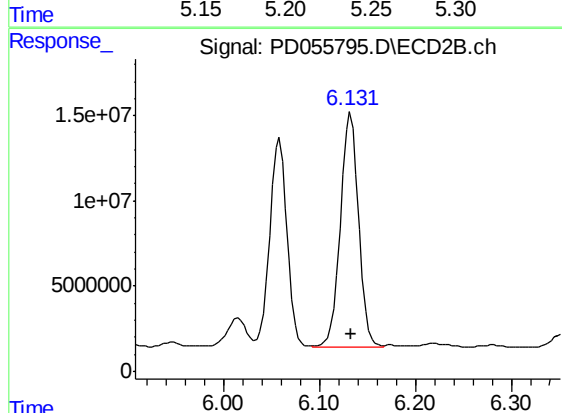


#26 Chlordane-4

R.T.: 6.133 min
Delta R.T.: 0.000 min
Response: 180411376
Conc: 685.85 ng/ml

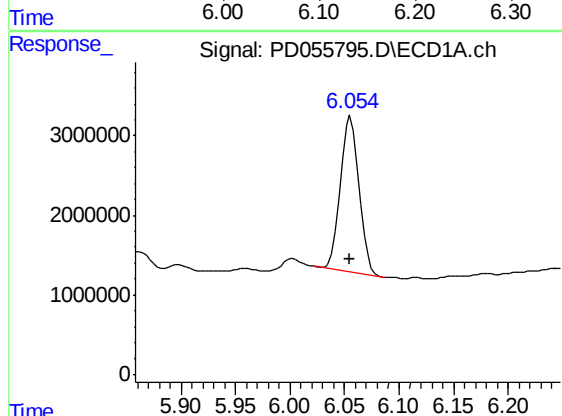


#27 Chlordane-5

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 23235266
Conc: 765.23 ng/ml

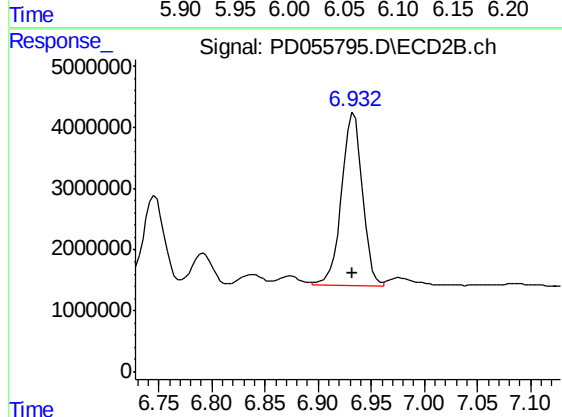

#27 Chlordane-5


R.T.: 6.934 min
Delta R.T.: 0.000 min
Response: 38266800
Conc: 820.83 ng/ml

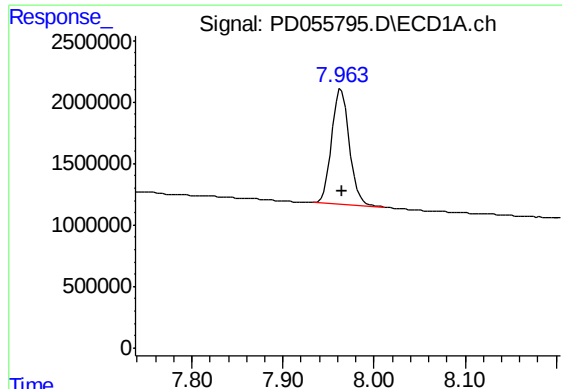

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 12680129
Conc: 13.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

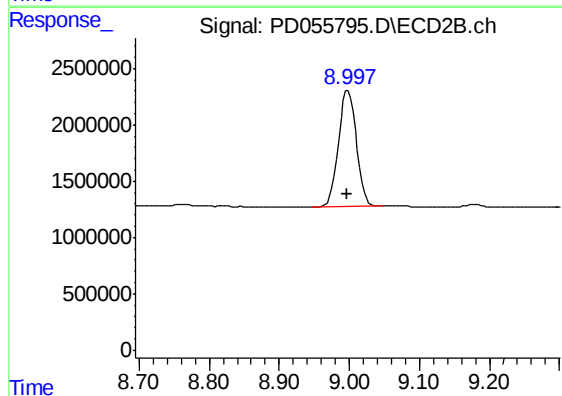

#28 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.000 min
Response: 18271789
Conc: 13.13 ng/ml