

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110220\
 Data File : PD060010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2020 08:55
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:40:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110220.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 03 01:26:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) A	alpha-BHC	3.916f	0.000	15535953	0	11.830	N.D.	#
5) MB	Aldrin	4.790	0.000	451577	0	0.383	N.D.	#
6) B	beta-BHC	4.497	0.000	843181	0	1.596	N.D.	#
8) B	Heptachlo...	0.000	5.924f	0	1470940	N.D.	0.460	#
12) B	4,4'-DDE	0.000	6.390f	0	21569	N.D.	0.006	#
23)	Chlordane-1	4.383	0.000	809477	0	27.584	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110220\
Data File : PD060010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2020 08:55
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:40:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110220.M
Quant Title : GC Extractables
QLast Update : Tue Nov 03 01:26:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

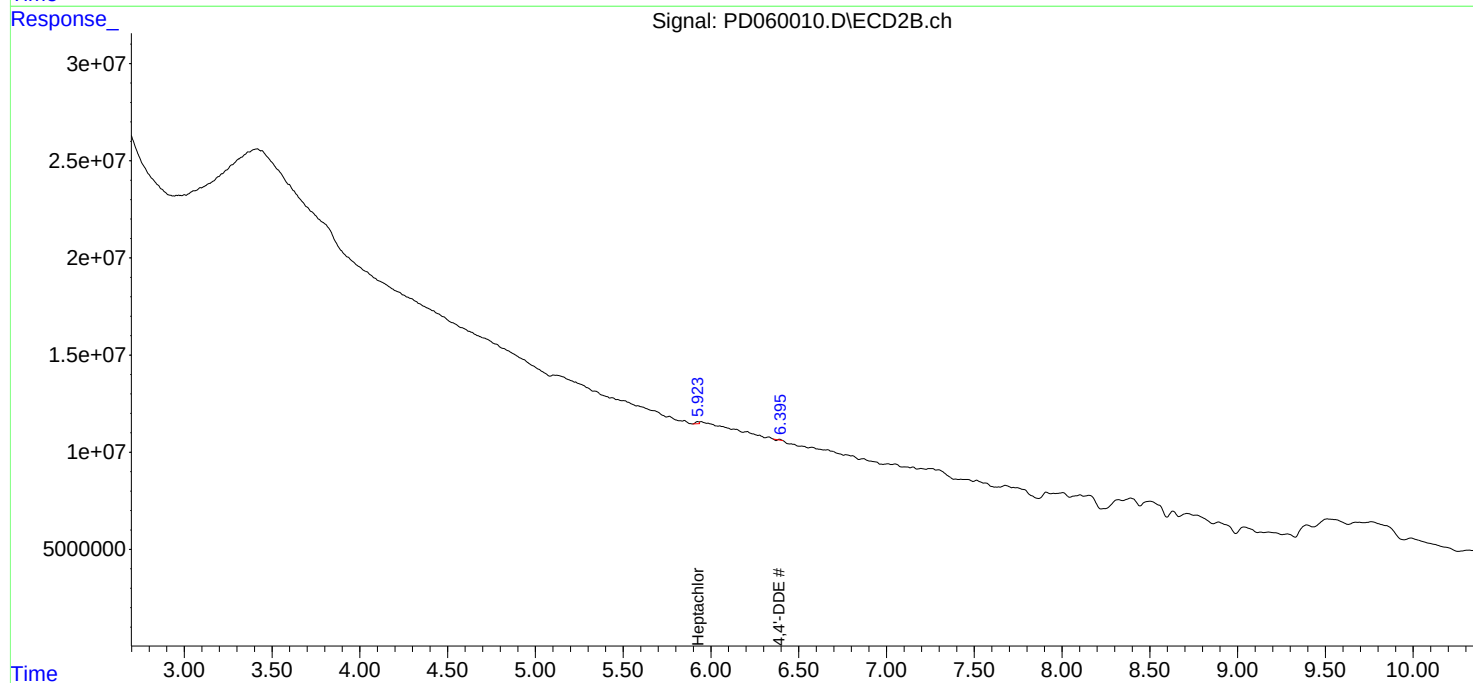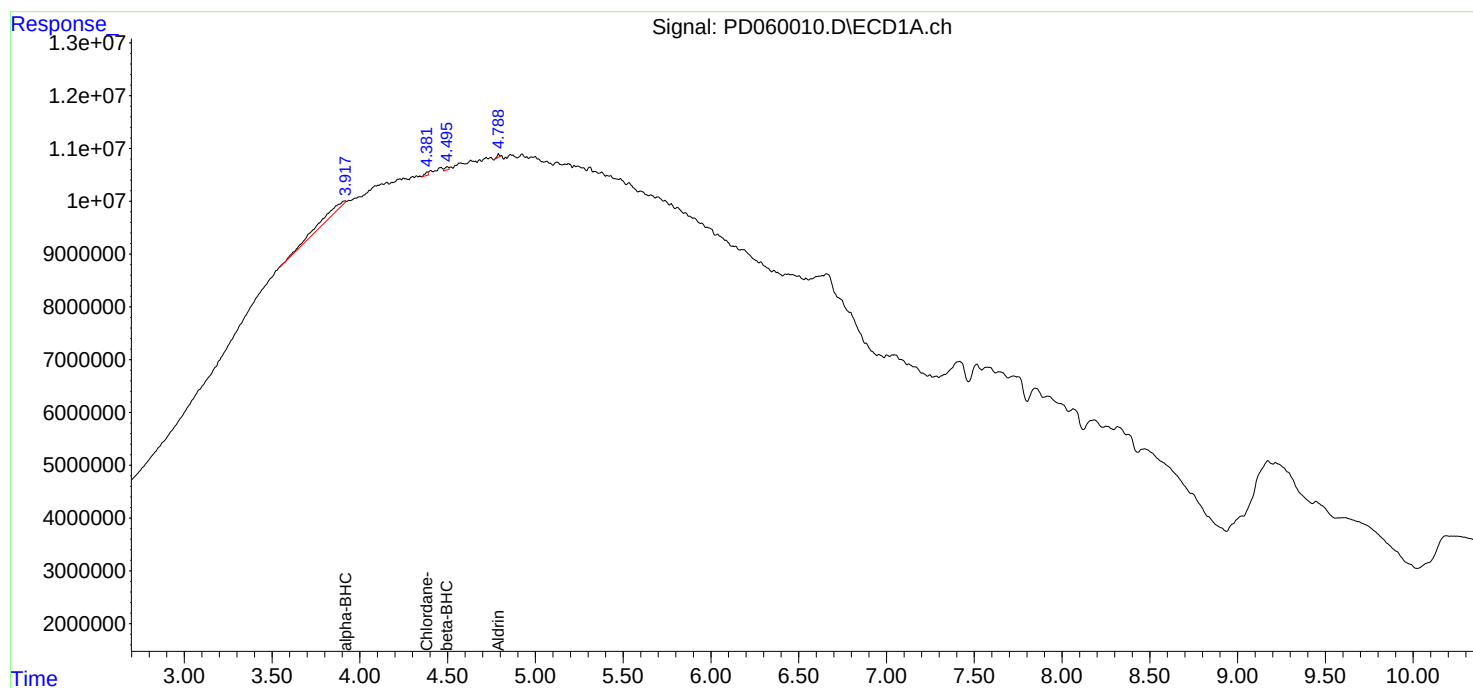


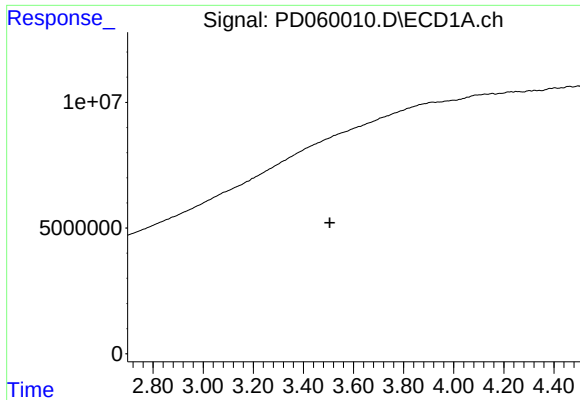

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

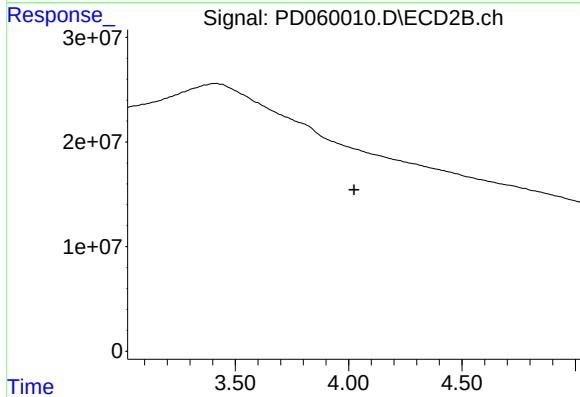


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.024 min
Response: 0
Conc: N.D.

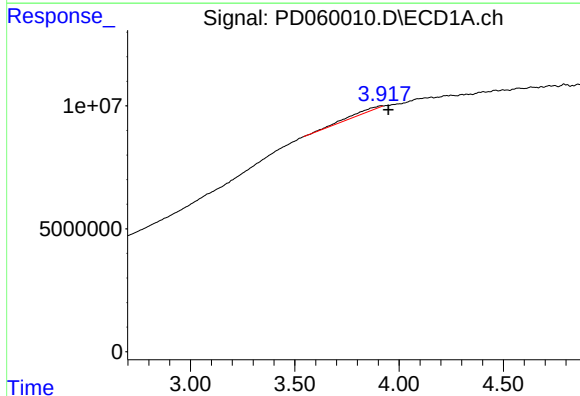


#2 alpha-BHC

R.T.: 3.916 min
Delta R.T.: -0.031 min
Response: 15535953
Conc: 11.83 ng/ml

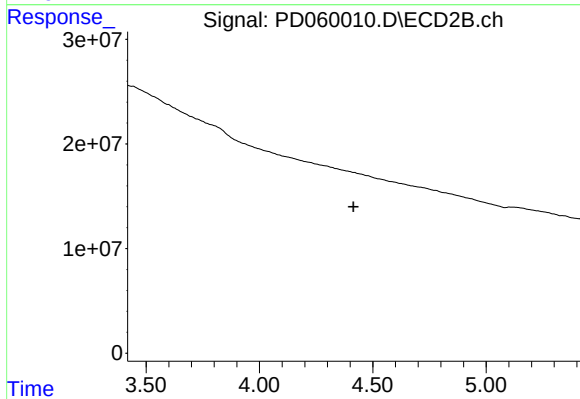

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.415 min
Response: 0
Conc: N.D.

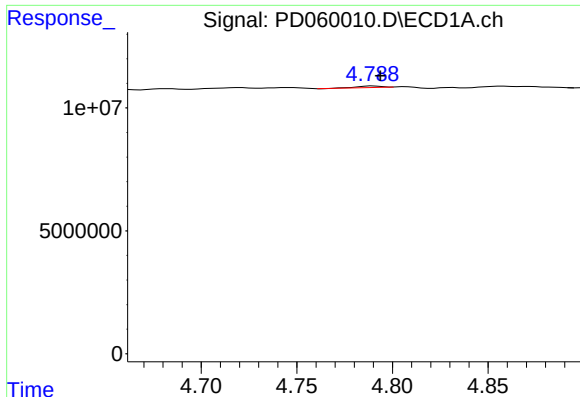

#5 Aldrin


R.T.: 4.790 min
Delta R.T.: -0.004 min
Response: 451577
Conc: 0.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

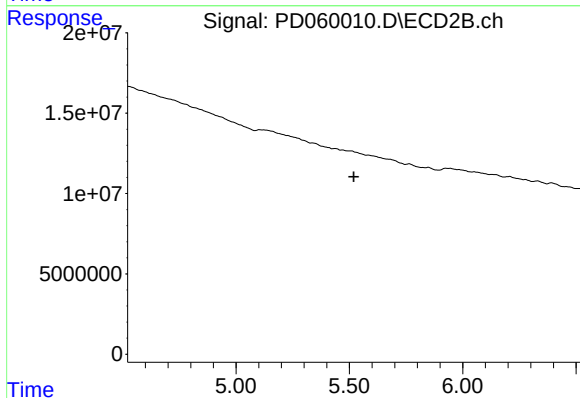


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.520 min
Response: 0
Conc: N.D.

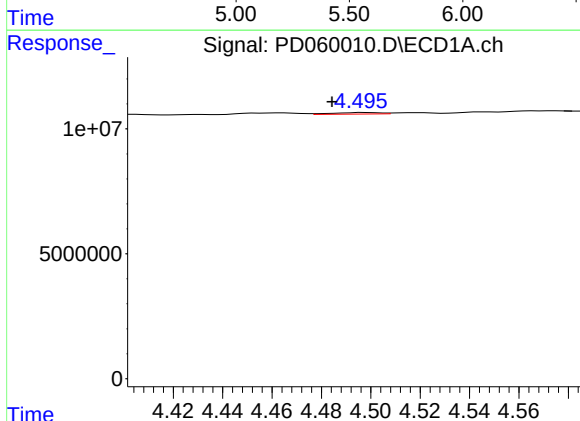


#6 beta-BHC

R.T.: 4.497 min
Delta R.T.: 0.013 min
Response: 843181
Conc: 1.60 ng/ml

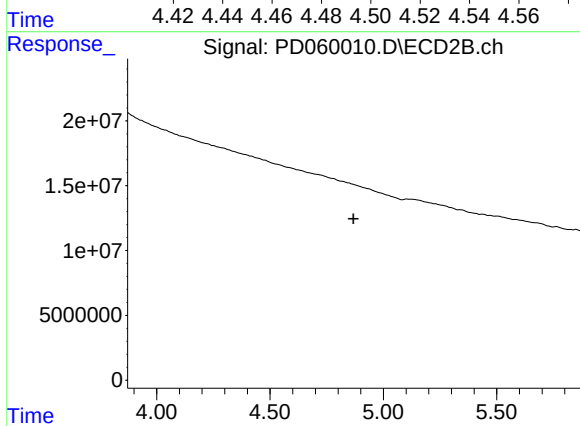

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.869 min
Response: 0
Conc: N.D.

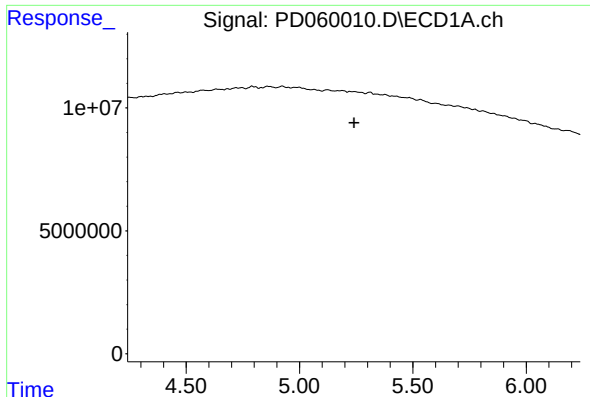

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.240 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

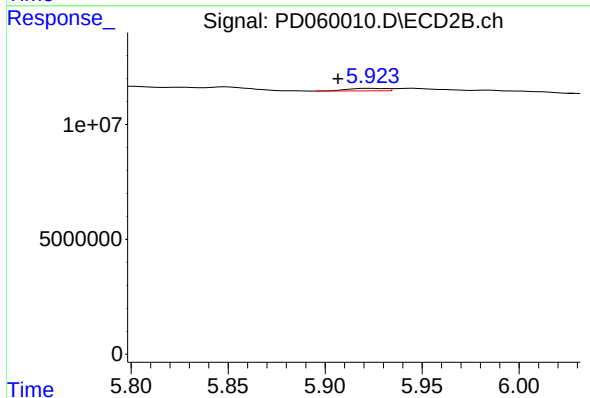


#8 Heptachlor epoxide

R.T.: 5.924 min
Delta R.T.: 0.017 min
Response: 1470940
Conc: 0.46 ng/ml

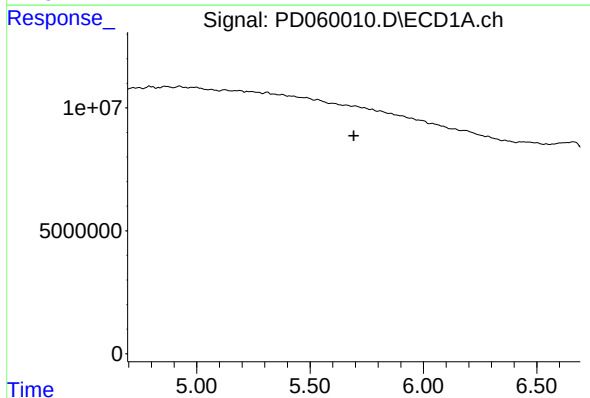


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.693 min
Response: 0
Conc: N.D.

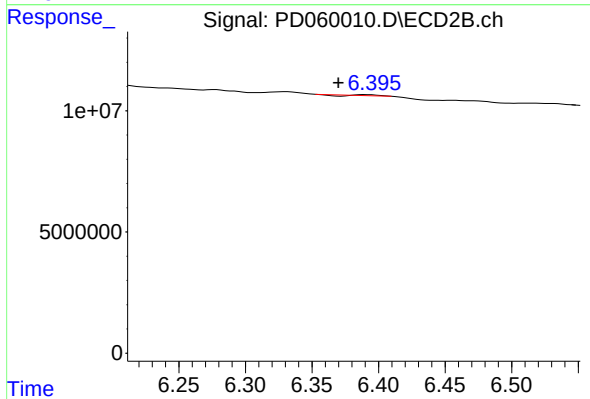

#12 4,4'-DDE


R.T.: 6.390 min
Delta R.T.: 0.020 min
Response: 21569
Conc: 0.01 ng/ml

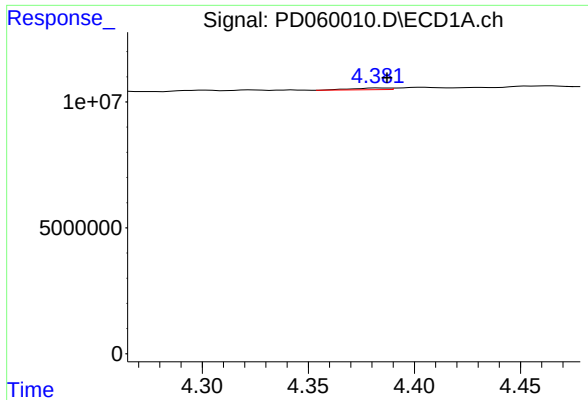

#23 Chlordane-1


R.T.: 4.383 min
Delta R.T.: -0.004 min
Response: 809477
Conc: 27.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

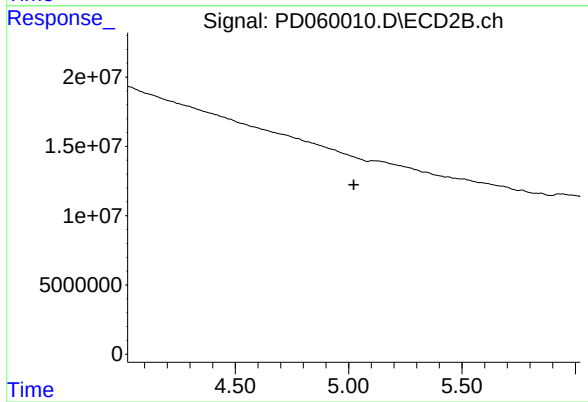


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.023 min
Response: 0
Conc: N.D.

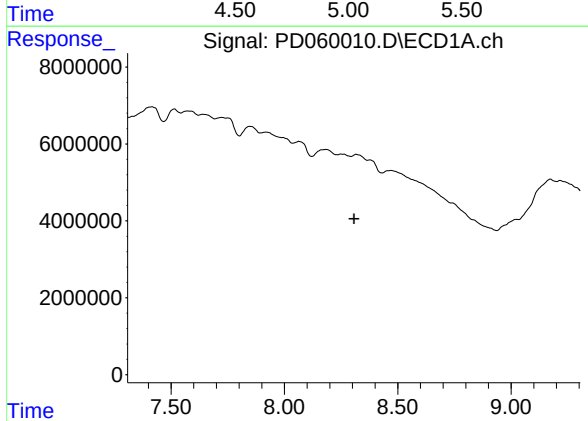

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.307 min
Response: 0
Conc: N.D.

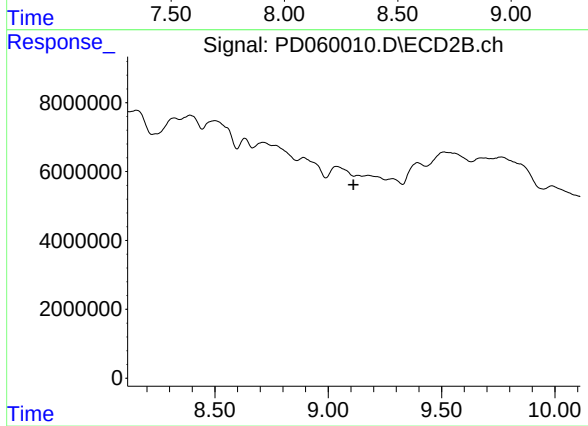

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.112 min
Response: 0
Conc: N.D.