

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110220\
 Data File : PD060011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2020 09:09
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:41:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110220.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 03 01:26:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.507	4.024	17418219	60351599	21.082	20.420
28)	SA Decachlor...	8.309	9.112	18293499	44857238	21.734	19.779
Target Compounds							
5)	MB Aldrin	0.000	5.528	0	1306105	N.D.	0.345 #
9)	A Endosulfan I	0.000	6.244f	0	175956	N.D.	0.054 #
10)	B gamma-Chl...	0.000	6.145	0	3901884	N.D.	1.102 #
17)	MA 4,4'-DDT	0.000	7.162	0	754074	N.D.	0.266 #
21)	B Endrin ke...	0.000	7.785f	0	1710959	N.D.	0.554 #
22)	Mirex	0.000	8.211	0	1493407	N.D.	0.819 #
25)	Chlordane-3	0.000	6.145	0	3901884	N.D.	9.219 #
26)	Chlordane-4	0.000	6.244f	0	175956	N.D.	0.351 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110220\
Data File : PD060011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2020 09:09
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:41:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110220.M
Quant Title : GC Extractables
QLast Update : Tue Nov 03 01:26:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

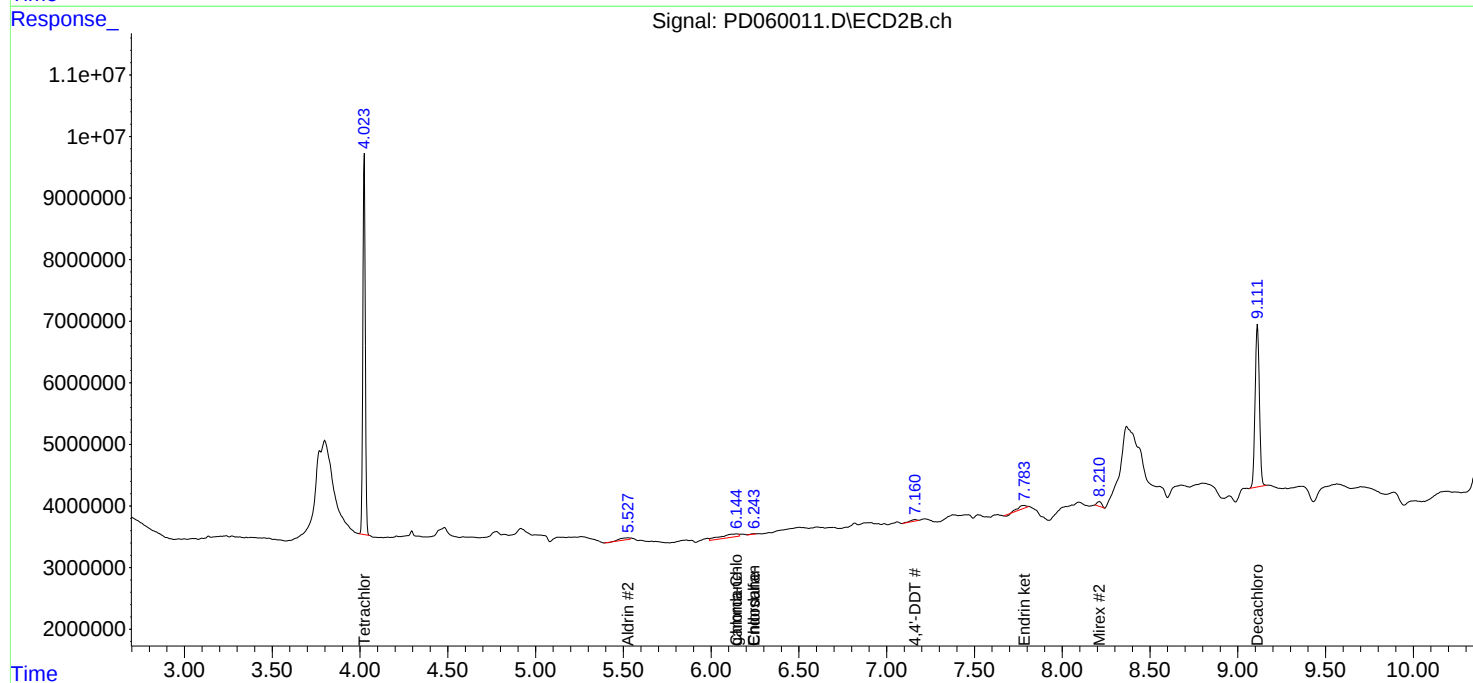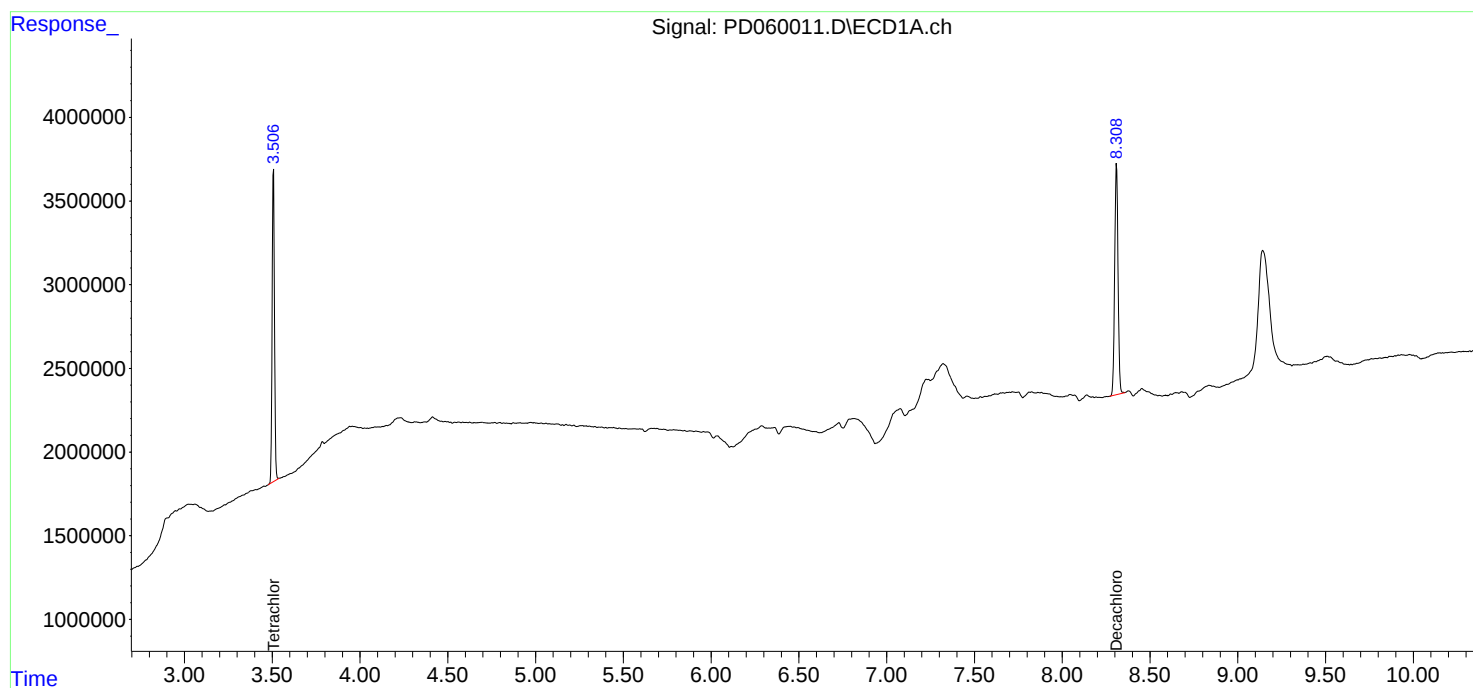


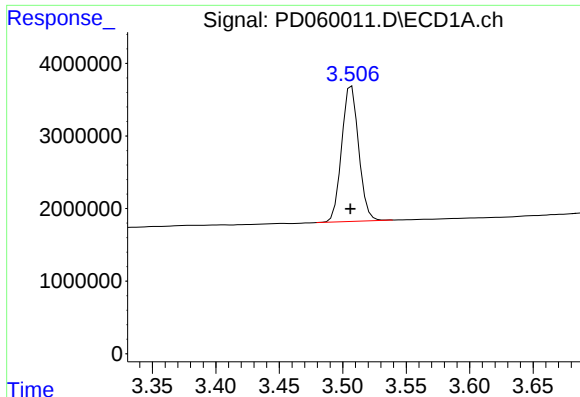

#1 Tetrachloro-m-xylene


R.T.: 3.507 min
Delta R.T.: 0.001 min
Response: 17418219
Conc: 21.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

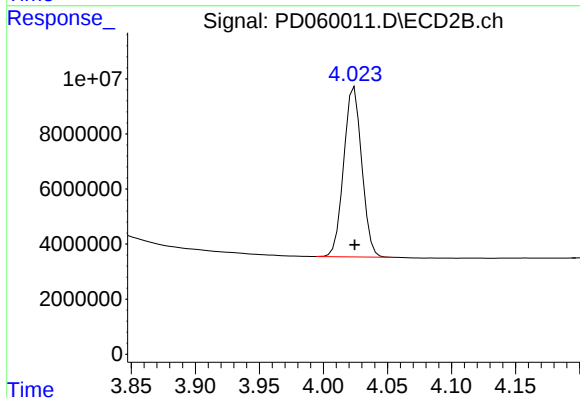


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 60351599
Conc: 20.42 ng/ml

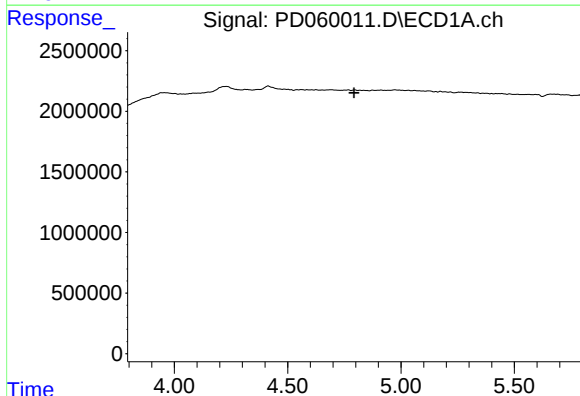


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.794 min
Response: 0
Conc: N.D.

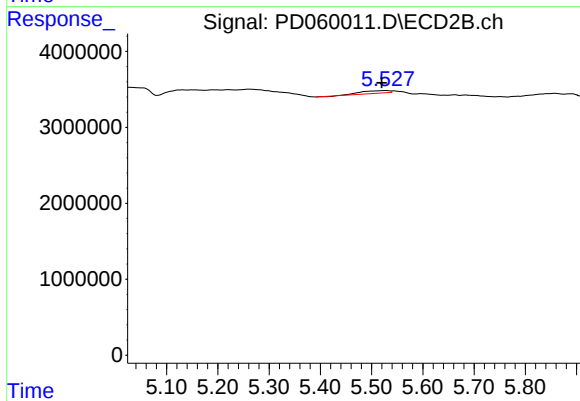

#5 Aldrin


R.T.: 5.528 min
Delta R.T.: 0.008 min
Response: 1306105
Conc: 0.34 ng/ml

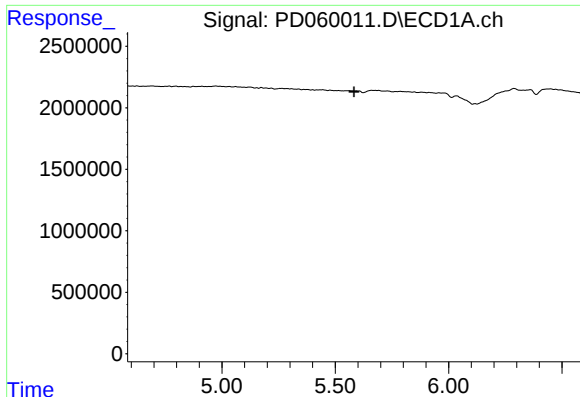

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

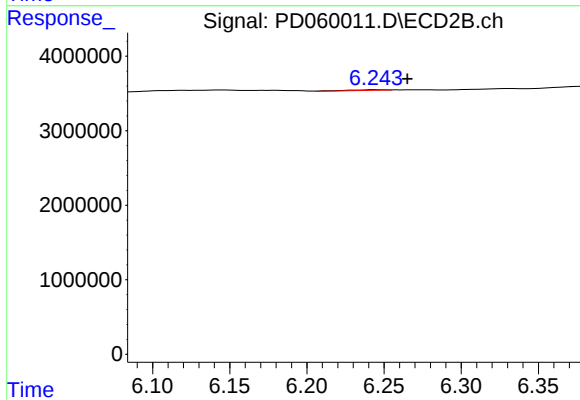


#9 Endosulfan I

R.T.: 6.244 min
Delta R.T.: -0.021 min
Response: 175956
Conc: 0.05 ng/ml

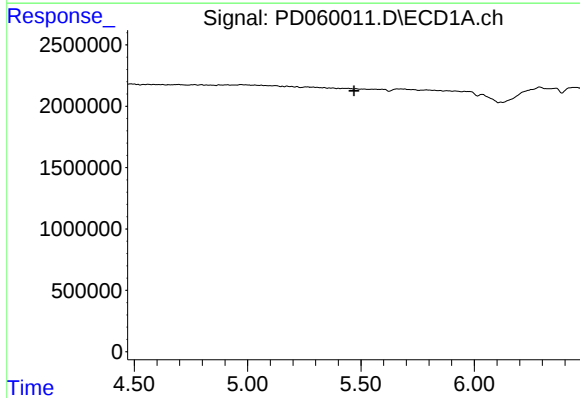


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.470 min
Response: 0
Conc: N.D.

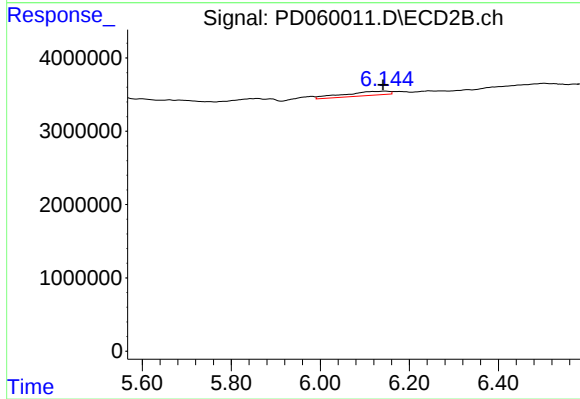

#10 gamma-Chlordane


R.T.: 6.145 min
Delta R.T.: 0.004 min
Response: 3901884
Conc: 1.10 ng/ml

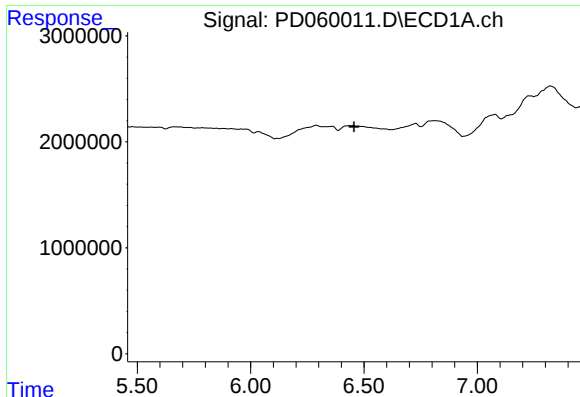

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

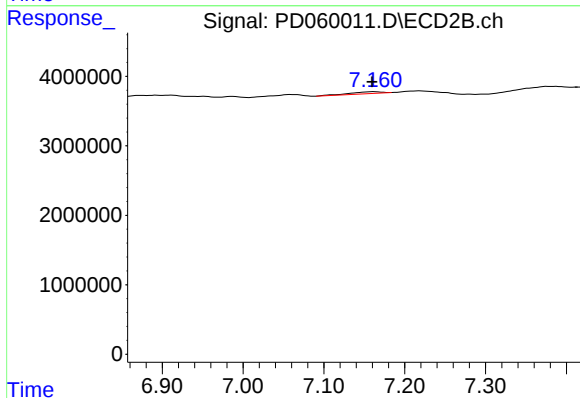


#17 4,4'-DDT

R.T.: 7.162 min
Delta R.T.: 0.002 min
Response: 754074
Conc: 0.27 ng/ml

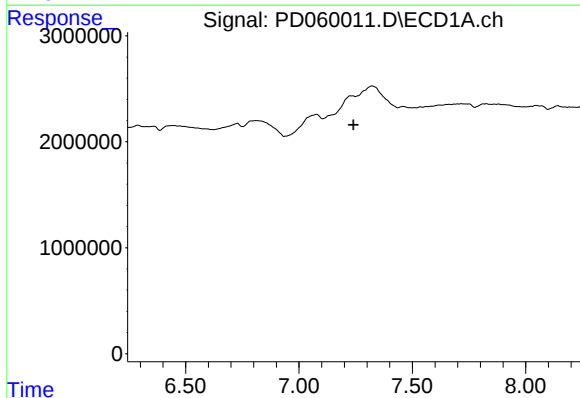


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.241 min
Response: 0
Conc: N.D.

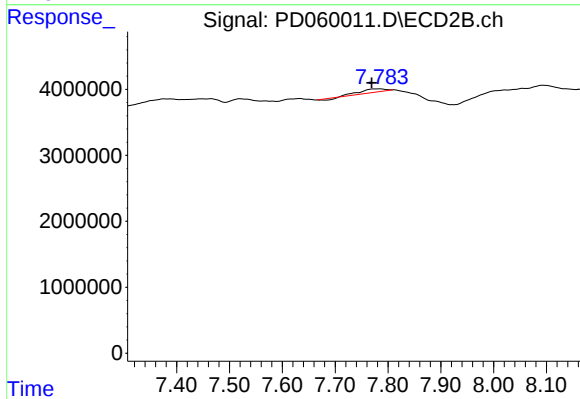

#21 Endrin ketone


R.T.: 7.785 min
Delta R.T.: 0.016 min
Response: 1710959
Conc: 0.55 ng/ml

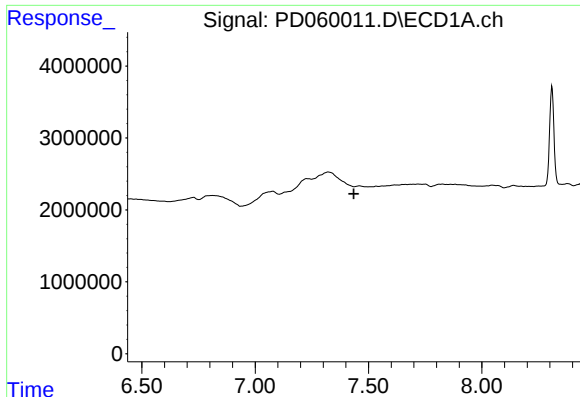

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

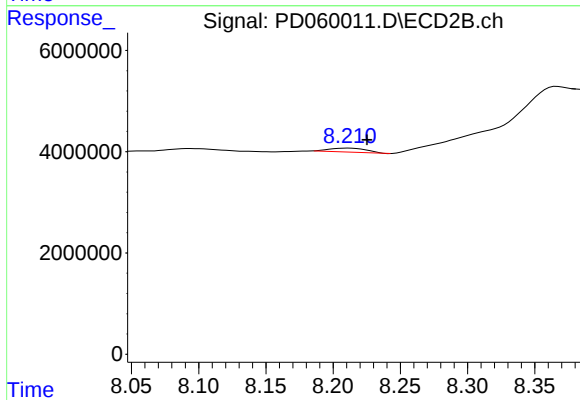


#22 Mirex

R.T.: 8.211 min
Delta R.T.: -0.015 min
Response: 1493407
Conc: 0.82 ng/ml

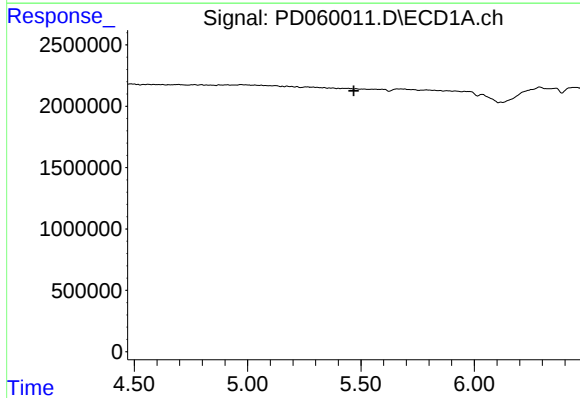


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

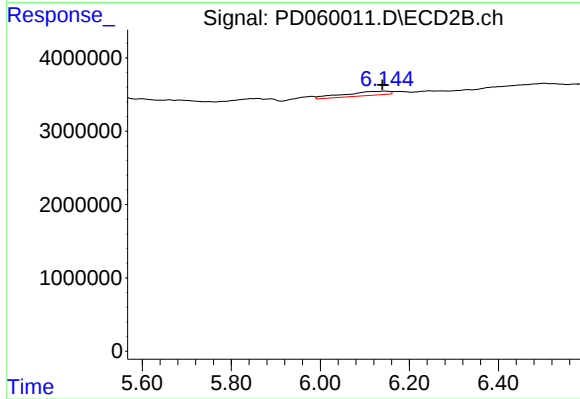

#25 Chlordane-3


R.T.: 6.145 min
Delta R.T.: 0.005 min
Response: 3901884
Conc: 9.22 ng/ml

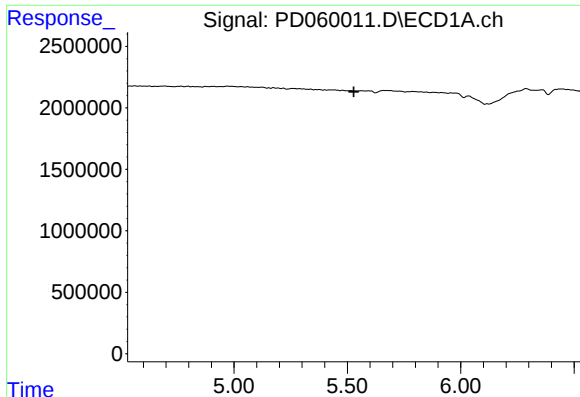

#26 Chlorodane-4


R.T.: 0.000 min
Exp R.T.: 5.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

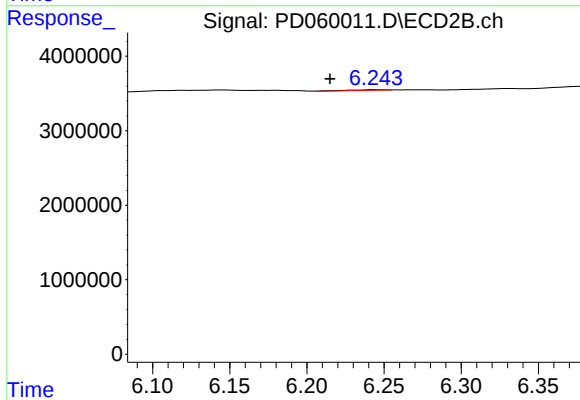


#26 Chlorodane-4

R.T.: 6.244 min
Delta R.T.: 0.029 min
Response: 175956
Conc: 0.35 ng/ml

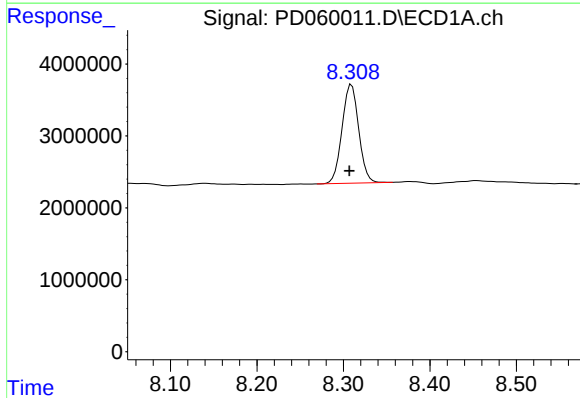

#28 Decachlorobiphenyl

R.T.: 8.309 min
Delta R.T.: 0.003 min
Response: 18293499
Conc: 21.73 ng/ml

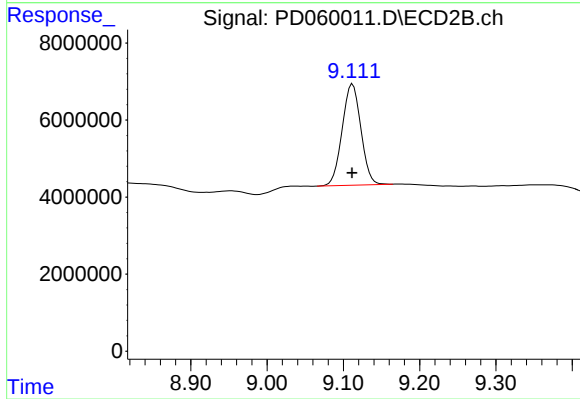

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 44857238
Conc: 19.78 ng/ml