

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110220\
 Data File : PD060014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2020 13:17
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:41:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110220.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 03 01:26:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	0.000	5.216	0	2669085	N.D.	0.657 #
5) MB	Aldrin	0.000	5.523	0	1859635	N.D.	0.491 #
9) A	Endosulfan I	0.000	6.287f	0	2708237	N.D.	0.831 #
10) B	gamma-Chl...	0.000	6.167f	0	7162910	N.D.	2.024 #
17) MA	4,4'-DDT	0.000	7.168	0	766590	N.D.	0.270 #
18) B	Endrin al...	0.000	7.047f	0	3950945	N.D.	1.562 #
22)	Mirex	7.458f	0.000	2631507	0	3.358	N.D. #
25)	Chlordane-3	0.000	6.167f	0	7162910	N.D.	16.924 #
27)	Chlordane-5	0.000	7.012	0	3042535	N.D.	32.871 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110220\
Data File : PD060014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2020 13:17
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:41:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110220.M
Quant Title : GC Extractables
QLast Update : Tue Nov 03 01:26:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

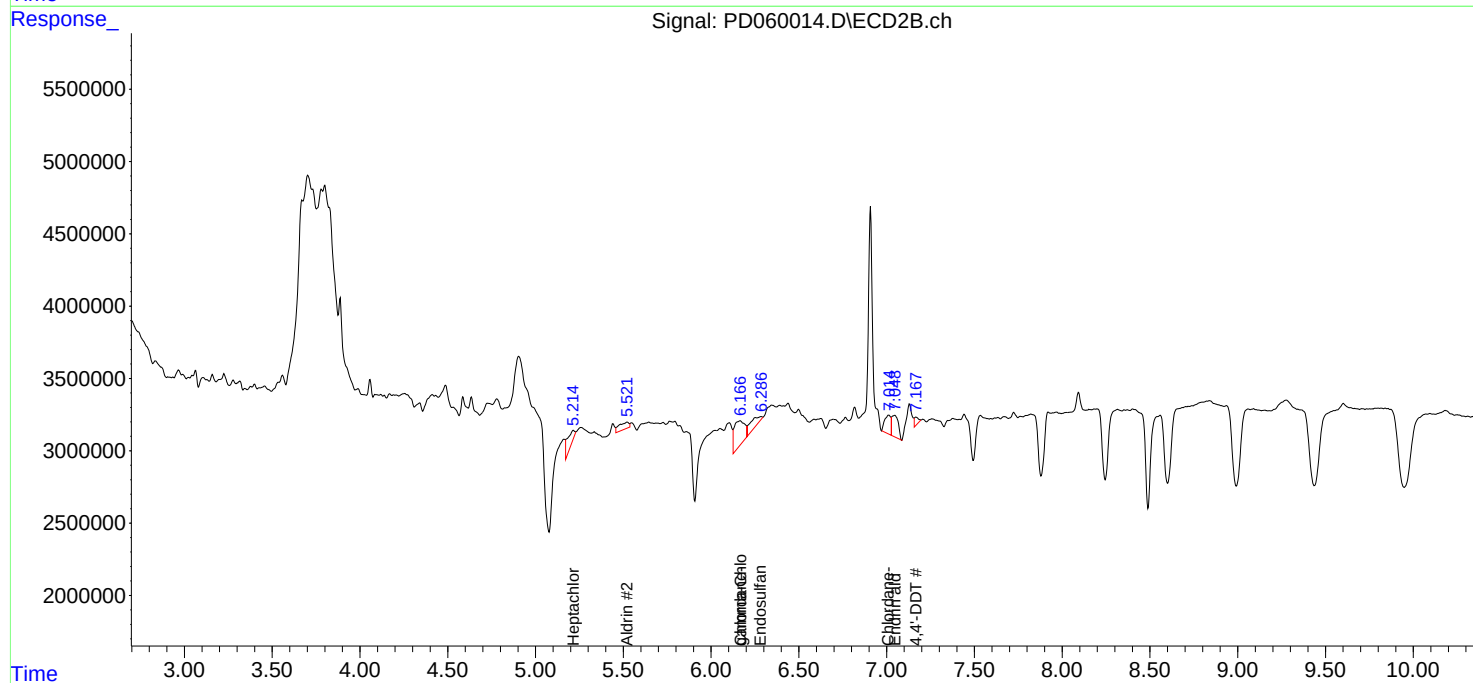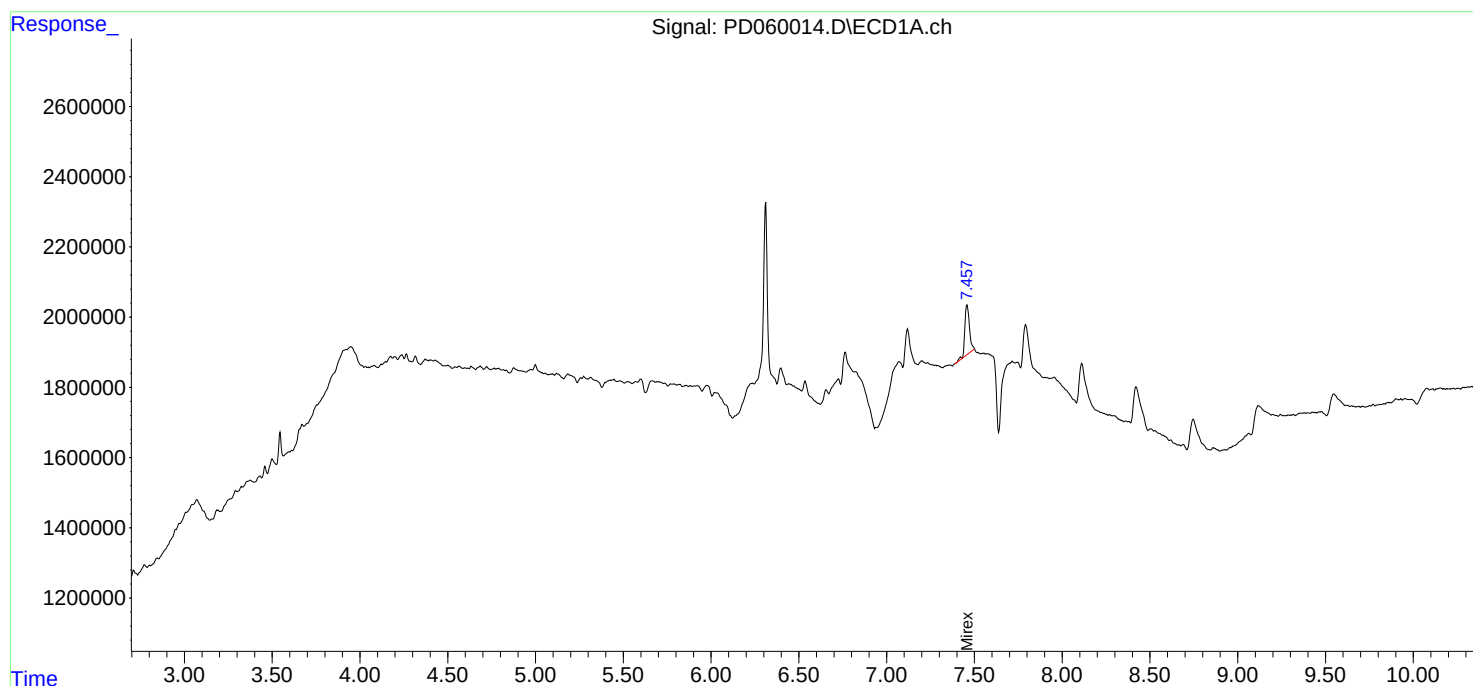


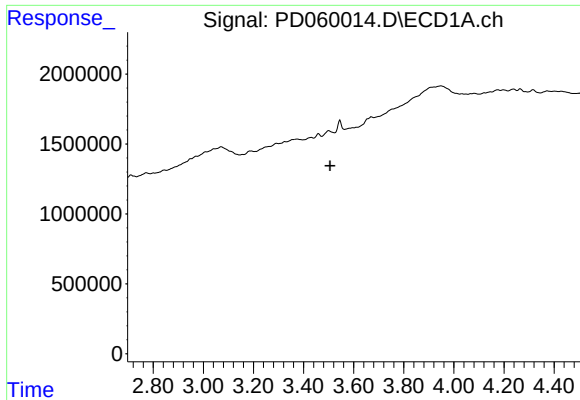

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

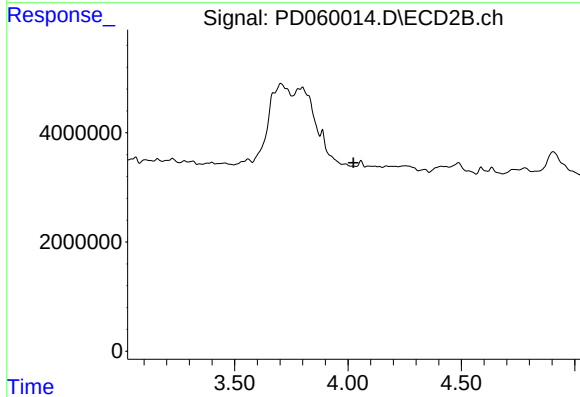


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.024 min
Response: 0
Conc: N.D.

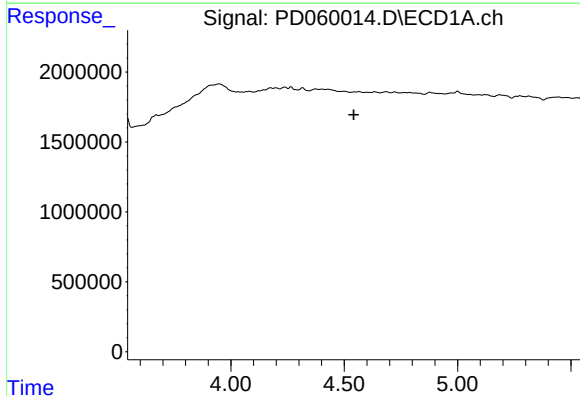


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.542 min
Response: 0
Conc: N.D.

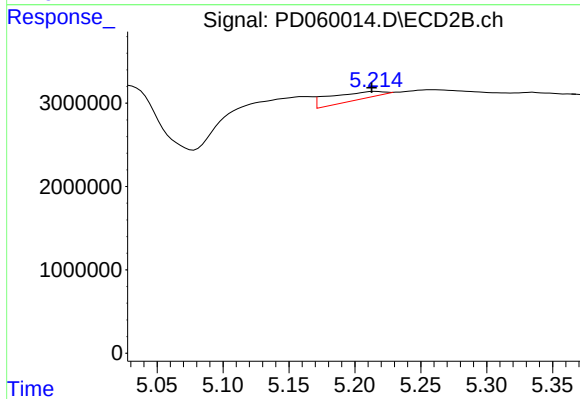

#4 Heptachlor


R.T.: 5.216 min
Delta R.T.: 0.003 min
Response: 2669085
Conc: 0.66 ng/ml

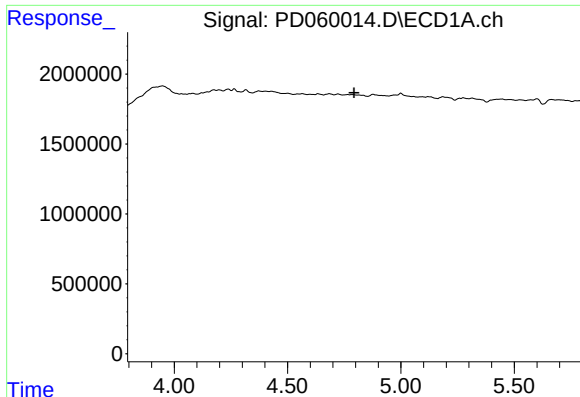

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

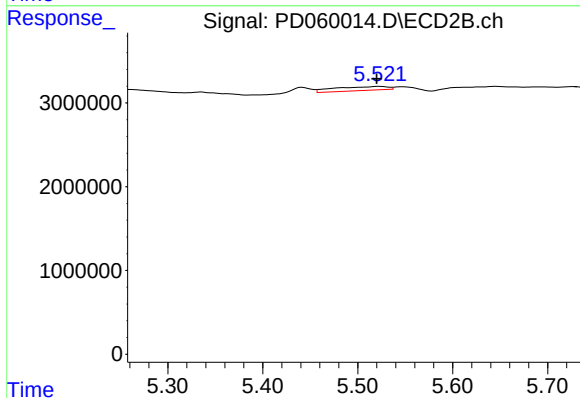


#5 Aldrin

R.T.: 5.523 min
Delta R.T.: 0.003 min
Response: 1859635
Conc: 0.49 ng/ml

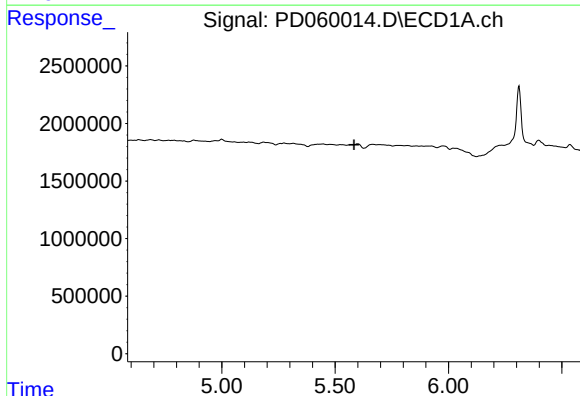


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.583 min
Response: 0
Conc: N.D.

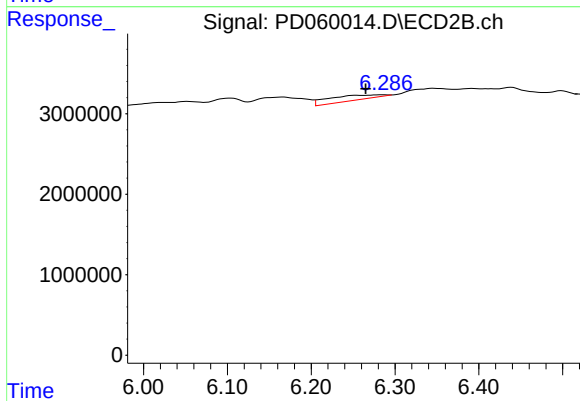

#9 Endosulfan I


R.T.: 6.287 min
Delta R.T.: 0.022 min
Response: 2708237
Conc: 0.83 ng/ml

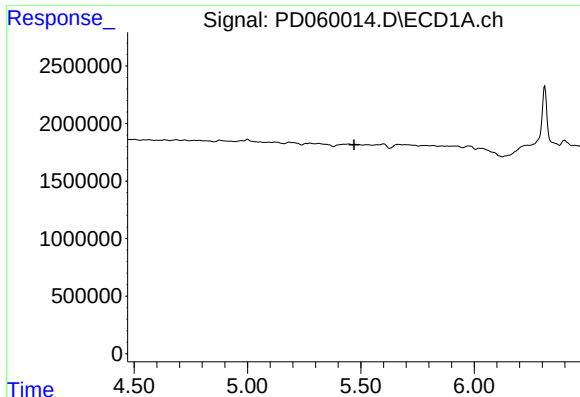

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

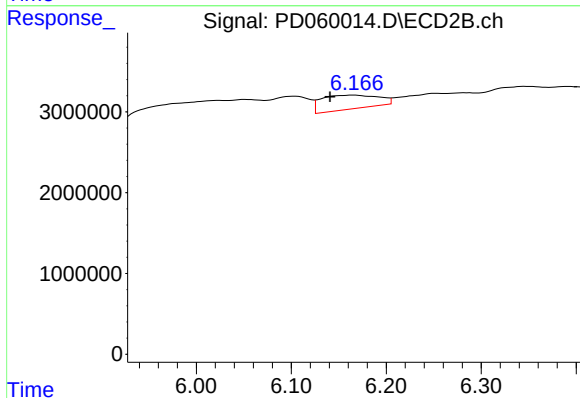


#10 gamma-Chlordane

R.T.: 6.167 min
Delta R.T.: 0.026 min
Response: 7162910
Conc: 2.02 ng/ml

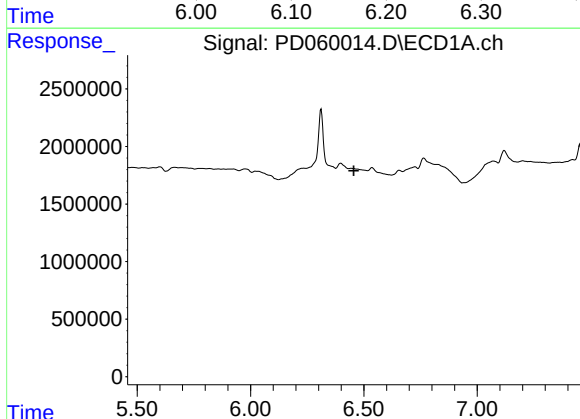


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.456 min
Response: 0
Conc: N.D.

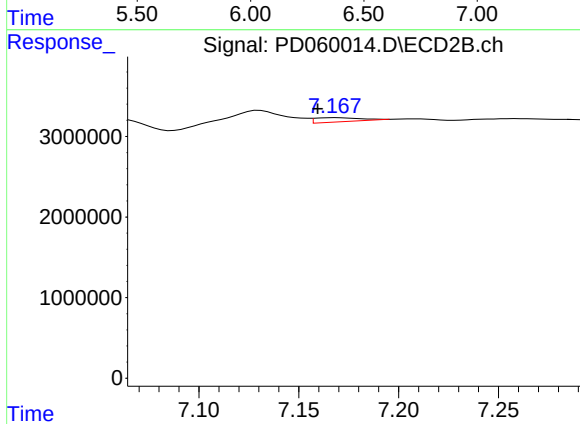

#17 4,4'-DDT


R.T.: 7.168 min
Delta R.T.: 0.008 min
Response: 766590
Conc: 0.27 ng/ml

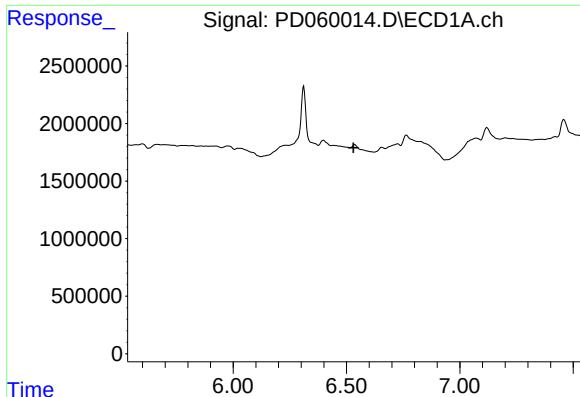

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.531 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

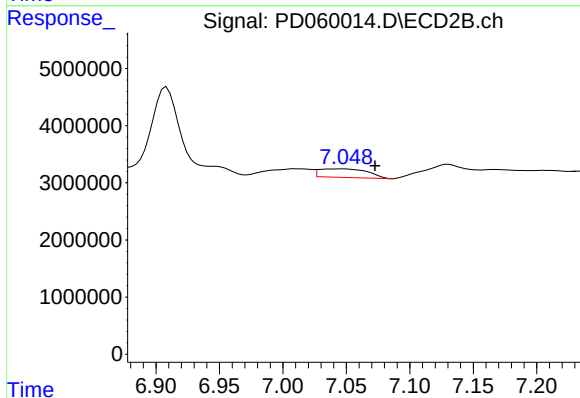


#18 Endrin aldehyde

R.T.: 7.047 min
Delta R.T.: -0.026 min
Response: 3950945
Conc: 1.56 ng/ml

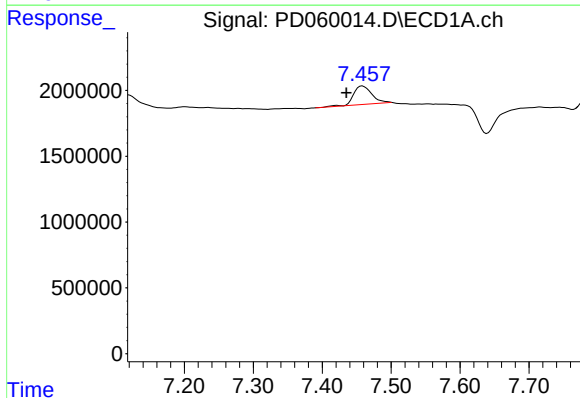


#22 Mirex

R.T.: 7.458 min
Delta R.T.: 0.023 min
Response: 2631507
Conc: 3.36 ng/ml

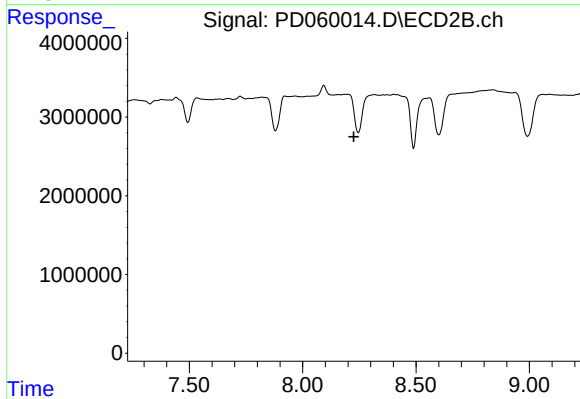

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.225 min
Response: 0
Conc: N.D.

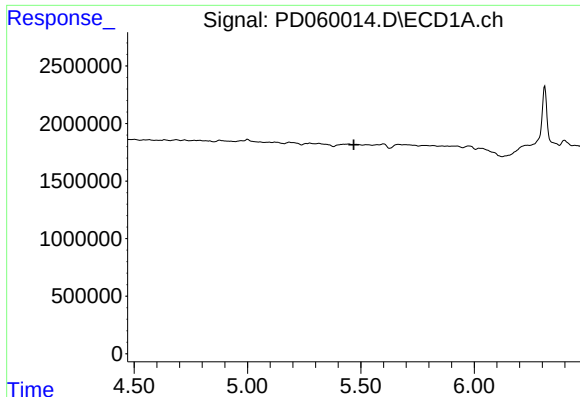

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

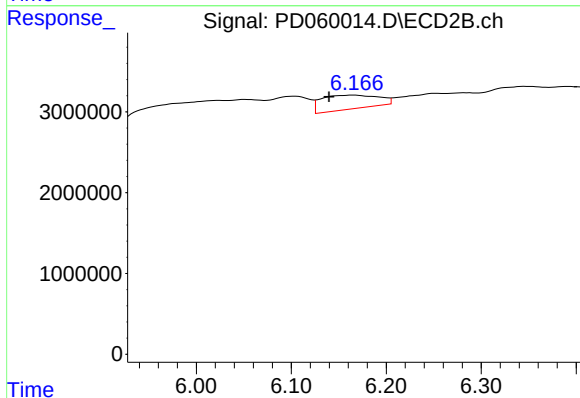


#25 Chlordane-3

R.T.: 6.167 min
Delta R.T.: 0.027 min
Response: 7162910
Conc: 16.92 ng/ml

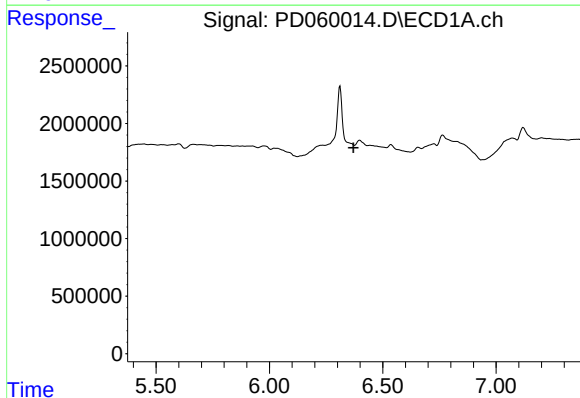


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.371 min
Response: 0
Conc: N.D.

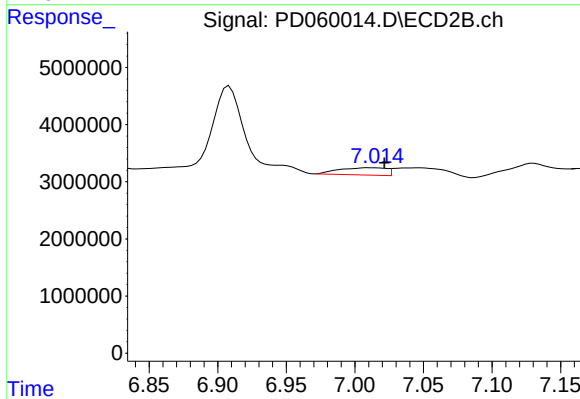

#27 Chlordane-5


R.T.: 7.012 min
Delta R.T.: -0.010 min
Response: 3042535
Conc: 32.87 ng/ml

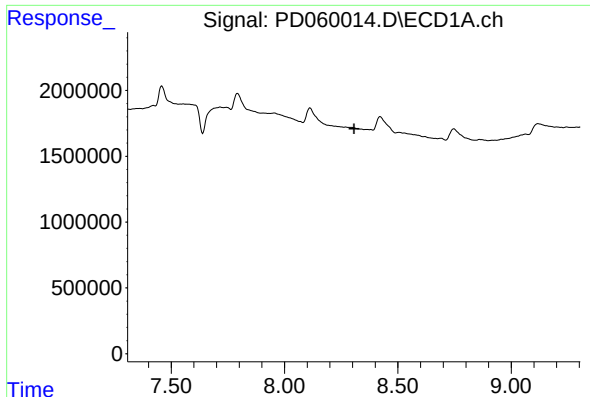

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.307 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

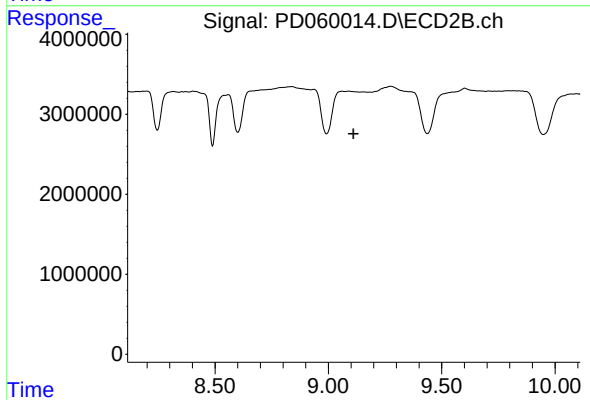

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.112 min
Response: 0
Conc: N.D.