

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110220\
 Data File : PD060015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2020 13:31
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:42:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110220.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 03 01:26:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.506	4.024	16526074	58235614	20.002	19.704
28)	SA Decachlor...	8.308	9.112	17171659	45610256	20.401	20.111
Target Compounds							
5)	MB Aldrin	0.000	5.511	0	6052788	N.D.	1.599 #
10)	B gamma-Chl...	0.000	6.169f	0	1487901	N.D.	0.420 #
11)	B alpha-Chl...	0.000	6.185f	0	173789	N.D.	0.049 #
17)	MA 4,4'-DDT	0.000	7.130f	0	1351229	N.D.	0.477 #
24)	Chlordane-2	0.000	5.511f	0	6052788	N.D.	55.322 #
25)	Chlordane-3	0.000	6.111f	0	9745775	N.D.	23.026 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110220\
Data File : PD060015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2020 13:31
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:42:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110220.M
Quant Title : GC Extractables
QLast Update : Tue Nov 03 01:26:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

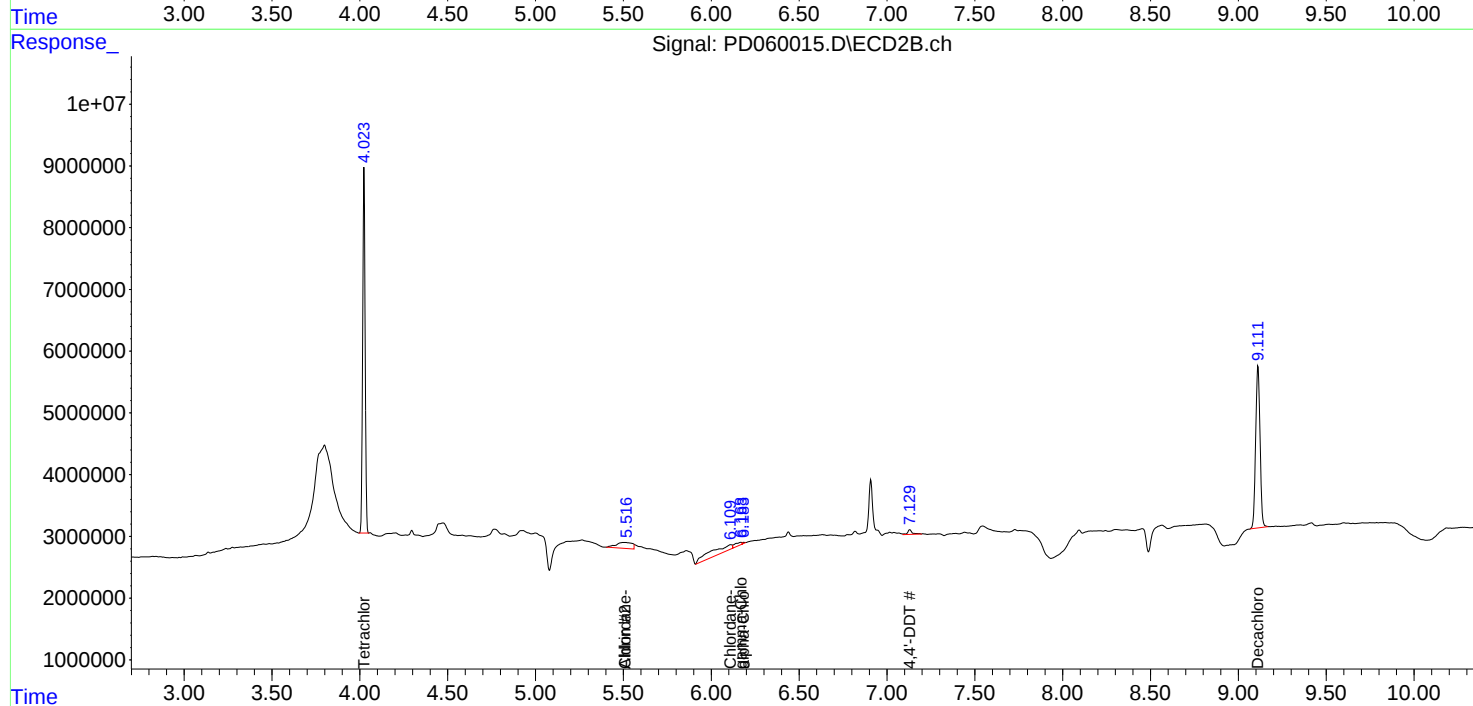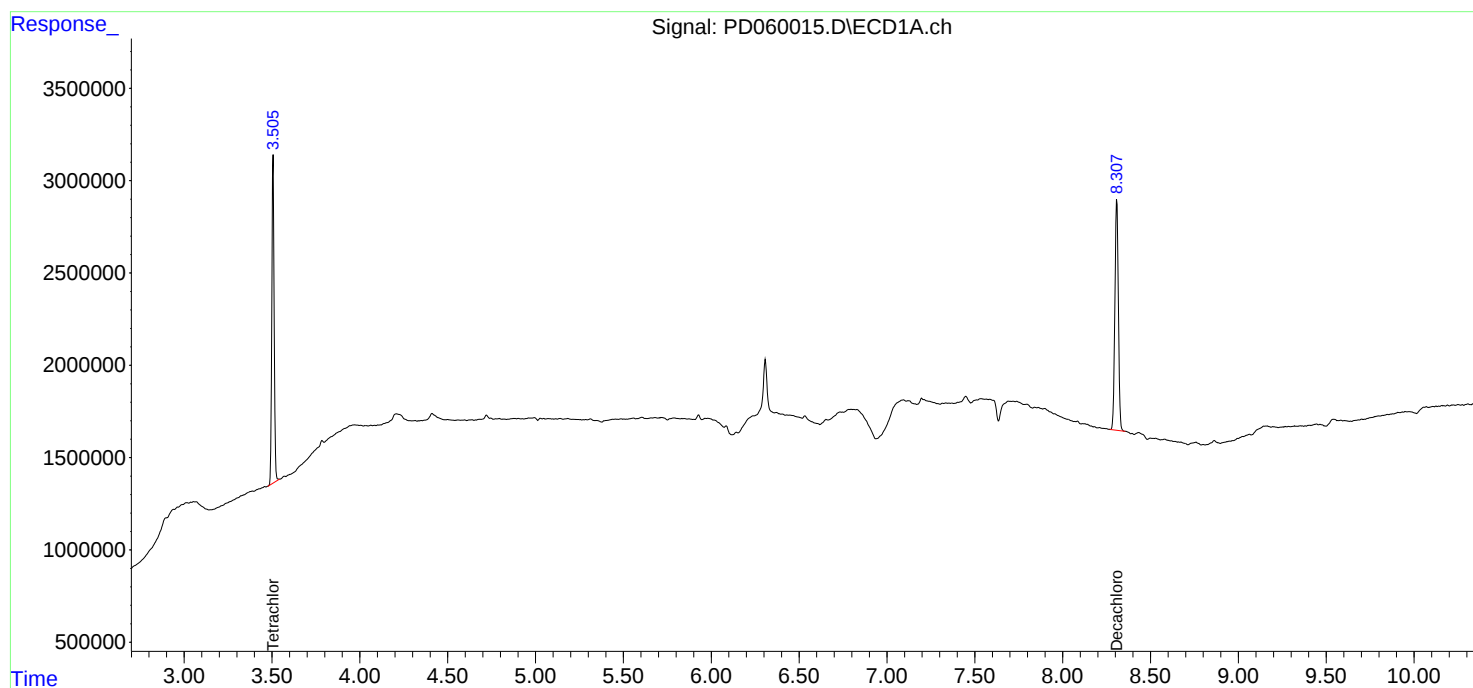


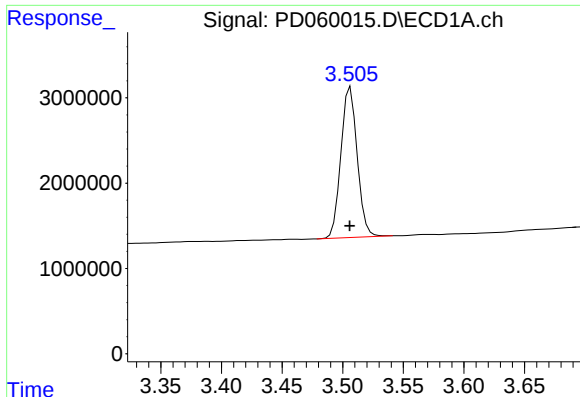

#1 Tetrachloro-m-xylene


R.T.: 3.506 min
Delta R.T.: 0.000 min
Response: 16526074
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

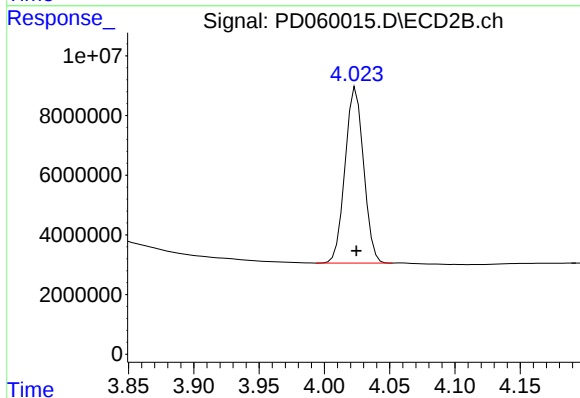


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 58235614
Conc: 19.70 ng/ml

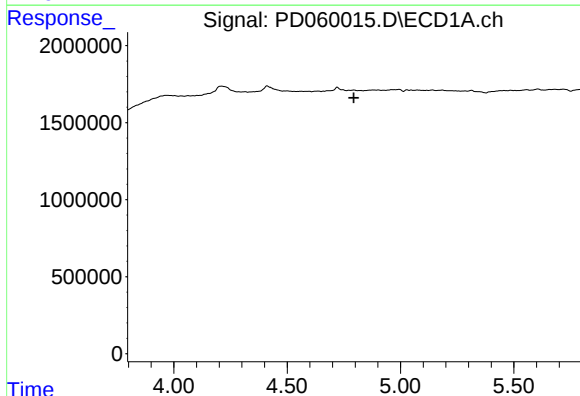


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.794 min
Response: 0
Conc: N.D.

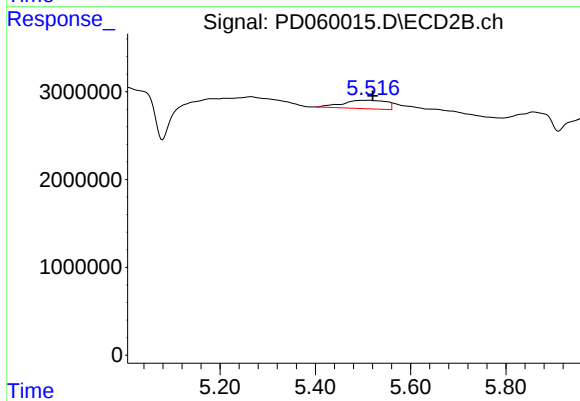

#5 Aldrin


R.T.: 5.511 min
Delta R.T.: -0.009 min
Response: 6052788
Conc: 1.60 ng/ml

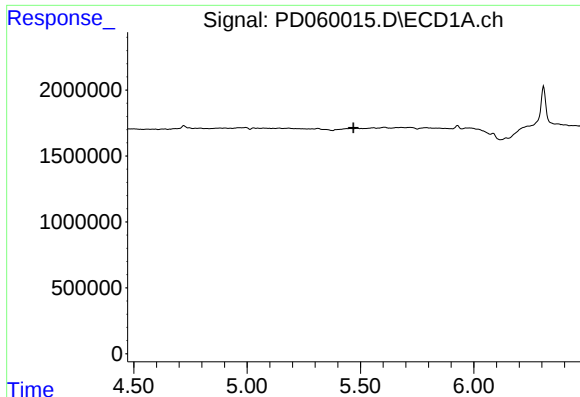

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

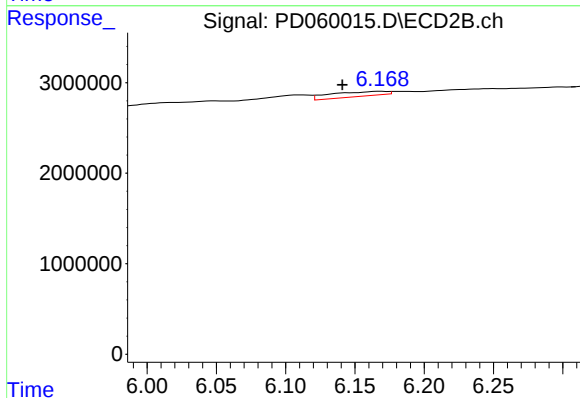


#10 gamma-Chlordane

R.T.: 6.169 min
Delta R.T.: 0.028 min
Response: 1487901
Conc: 0.42 ng/ml

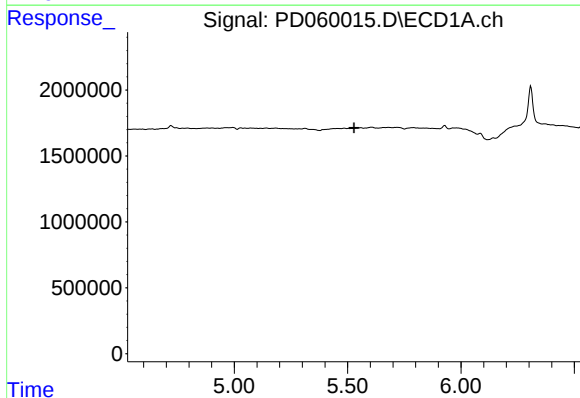


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.529 min
Response: 0
Conc: N.D.

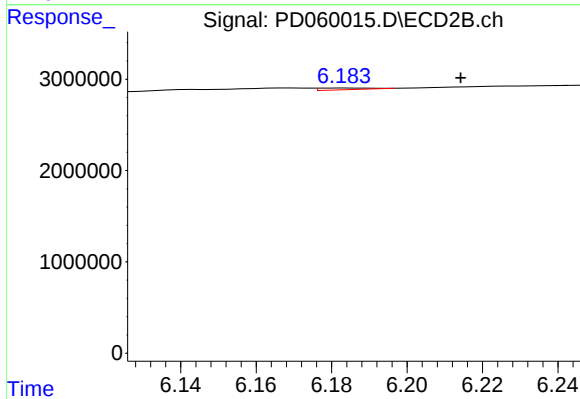

#11 alpha-Chlordane


R.T.: 6.185 min
Delta R.T.: -0.030 min
Response: 173789
Conc: 0.05 ng/ml

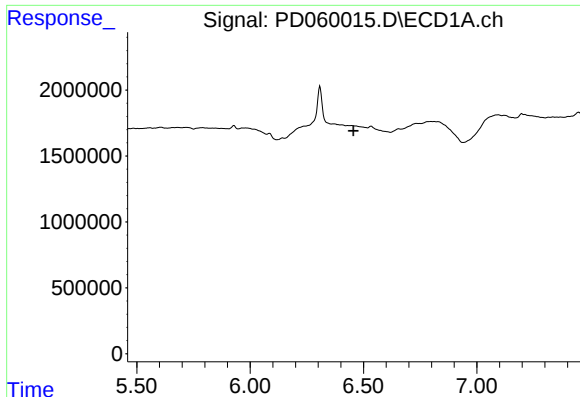

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

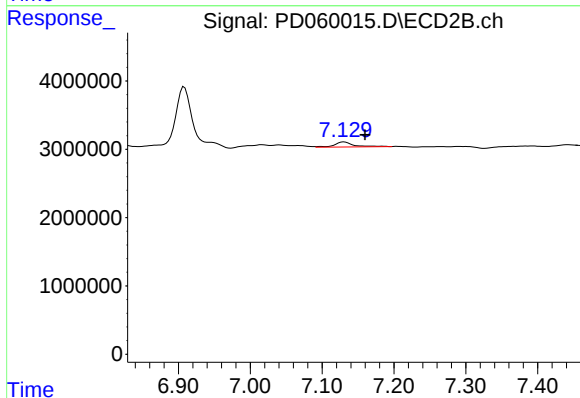


#17 4,4'-DDT

R.T.: 7.130 min
Delta R.T.: -0.029 min
Response: 1351229
Conc: 0.48 ng/ml

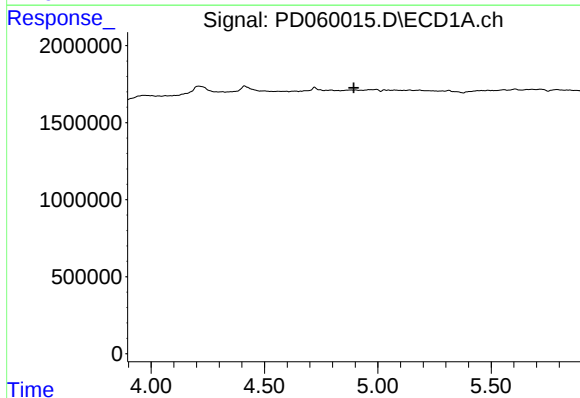


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.893 min
Response: 0
Conc: N.D.

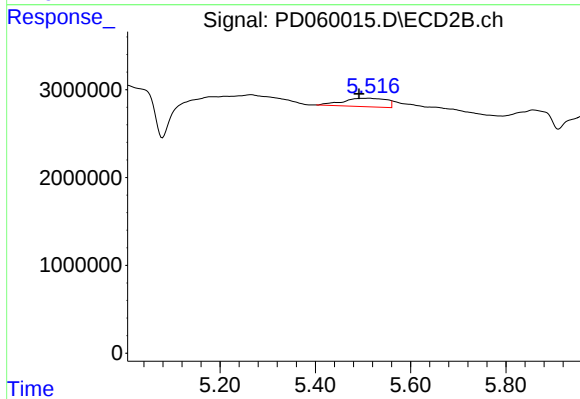

#24 Chlordane-2


R.T.: 5.511 min
Delta R.T.: 0.020 min
Response: 6052788
Conc: 55.32 ng/ml

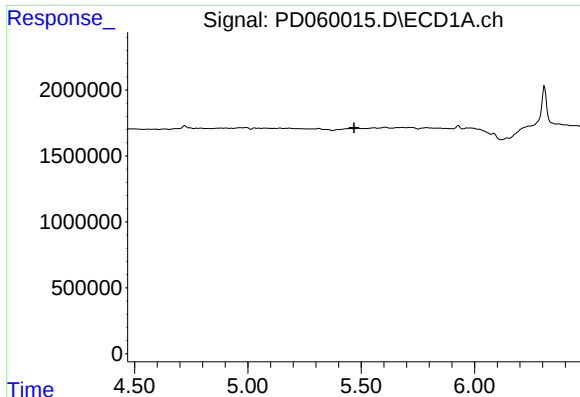

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

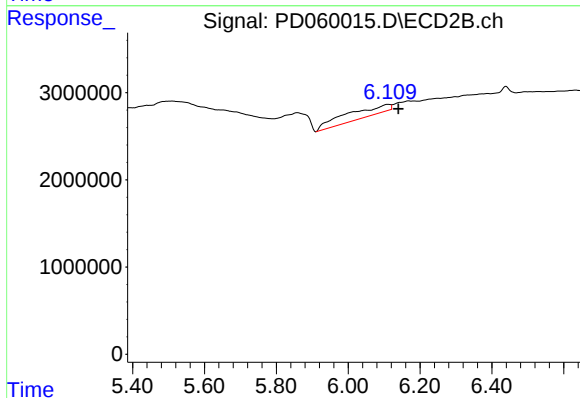


#25 Chlordane-3

R.T.: 6.111 min
Delta R.T.: -0.029 min
Response: 9745775
Conc: 23.03 ng/ml

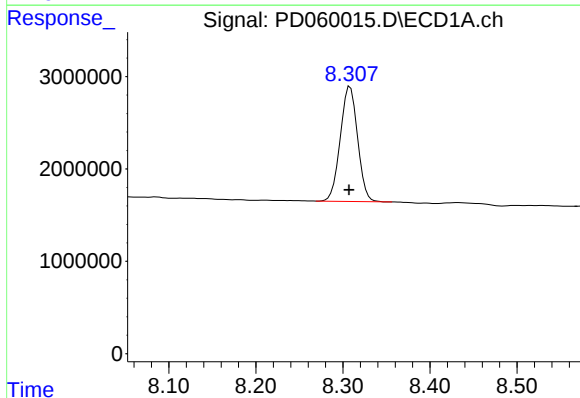

#28 Decachlorobiphenyl

R.T.: 8.308 min
Delta R.T.: 0.001 min
Response: 17171659
Conc: 20.40 ng/ml

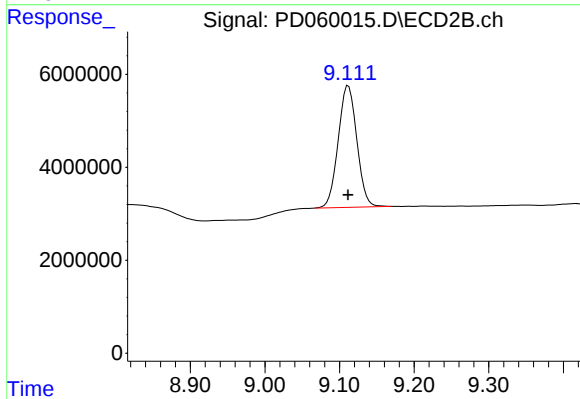

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 45610256
Conc: 20.11 ng/ml