

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110220\
 Data File : PD060026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2020 16:11
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:43:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110220.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 03 01:26:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.511	4.024	16811273	59856952	20.347	20.253
28)	SA Decachlor...	8.312	9.115	17908307	47514831	21.276	20.951
Target Compounds							
3)	MA gamma-BHC...	0.000	4.705	0	980656	N.D.	0.229 #
9)	A Endosulfan I	0.000	6.244f	0	1308009	N.D.	0.401 #
10)	B gamma-Chl...	0.000	6.163f	0	5655482	N.D.	1.598 #
11)	B alpha-Chl...	0.000	6.216	0	696638	N.D.	0.198 #
17)	MA 4,4'-DDT	0.000	7.131f	0	986496	N.D.	0.348 #
25)	Chlordane-3	0.000	6.163f	0	5655482	N.D.	13.362 #
26)	Chlordane-4	0.000	6.216	0	696638	N.D.	1.391 #
27)	Chlordane-5	0.000	7.013	0	1899179	N.D.	20.519 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110220\
Data File : PD060026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2020 16:11
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:43:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110220.M
Quant Title : GC Extractables
QLast Update : Tue Nov 03 01:26:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

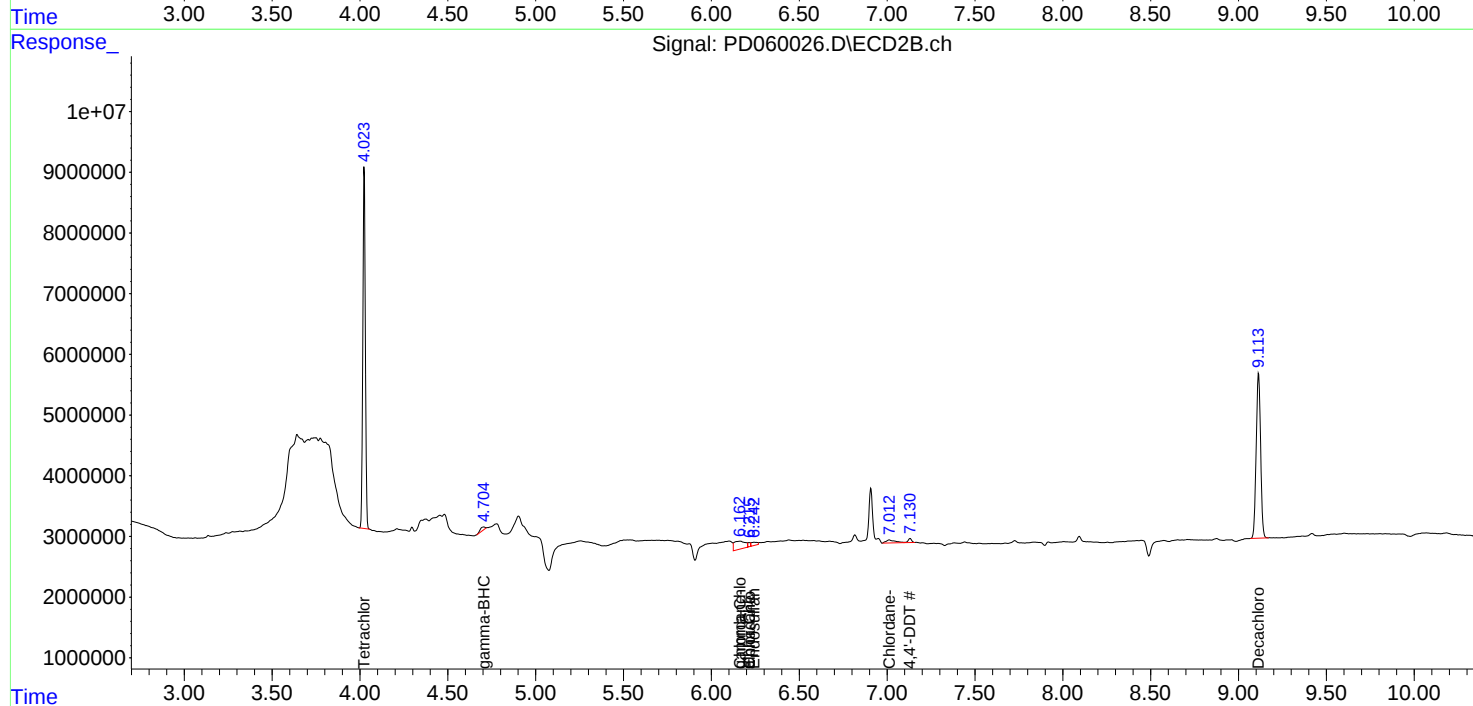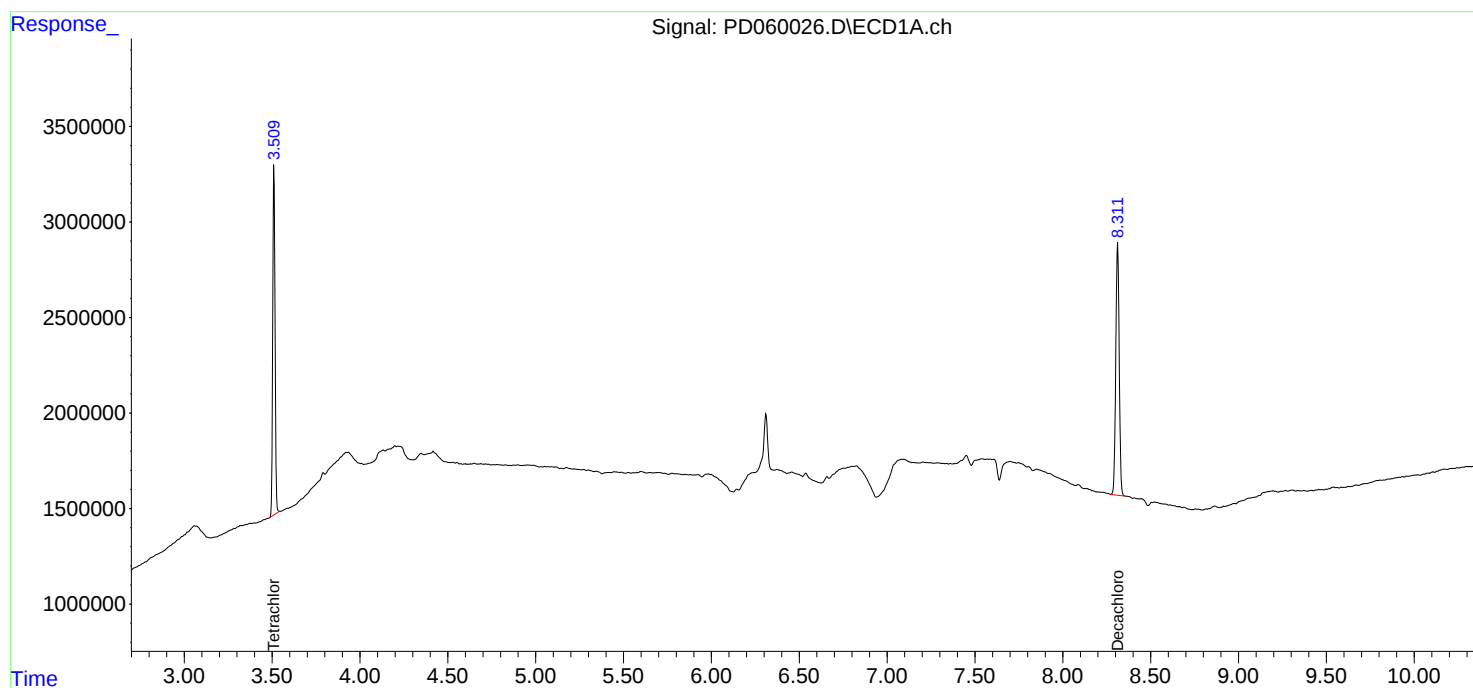


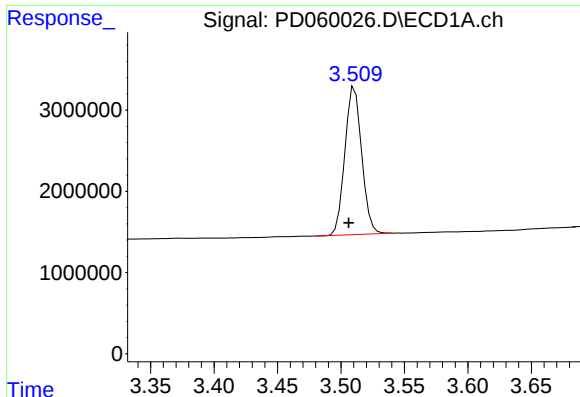

#1 Tetrachloro-m-xylene


R.T.: 3.511 min
Delta R.T.: 0.005 min
Response: 16811273
Conc: 20.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

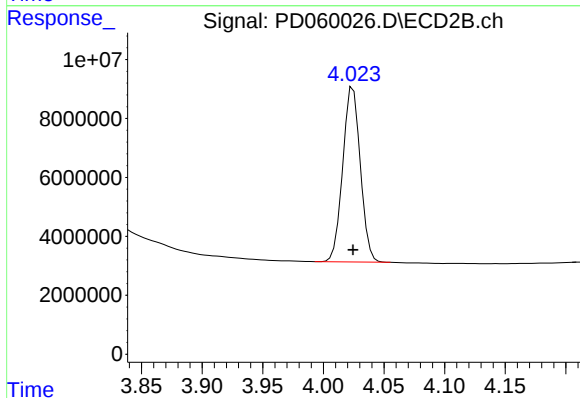


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 59856952
Conc: 20.25 ng/ml

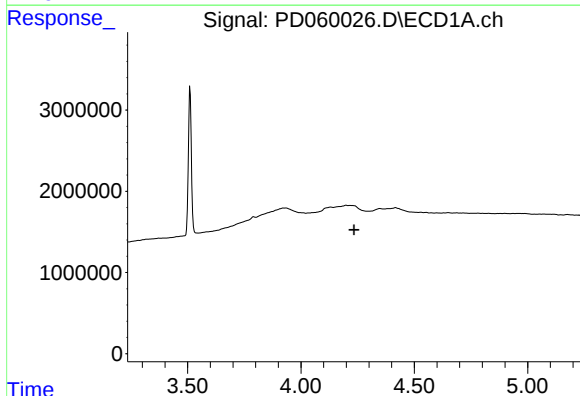


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.234 min
Response: 0
Conc: N.D.

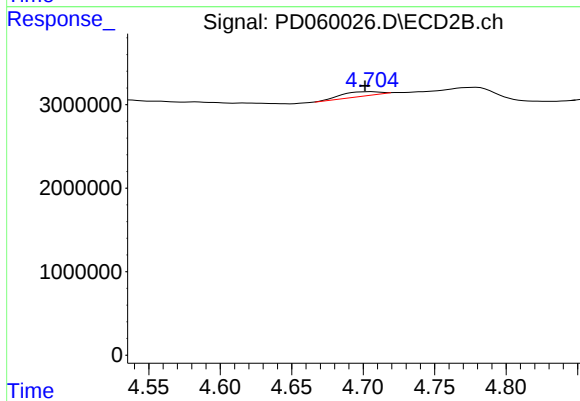

#3 gamma-BHC (Lindane)


R.T.: 4.705 min
Delta R.T.: 0.004 min
Response: 980656
Conc: 0.23 ng/ml

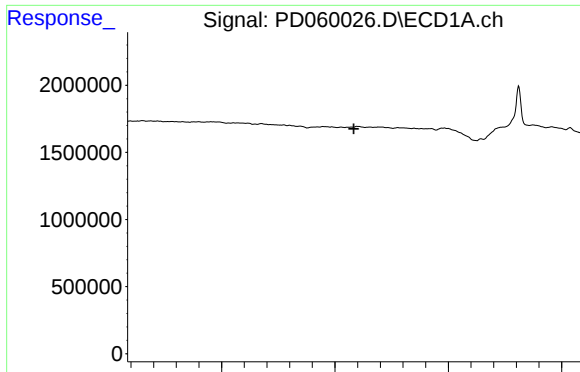

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.583 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

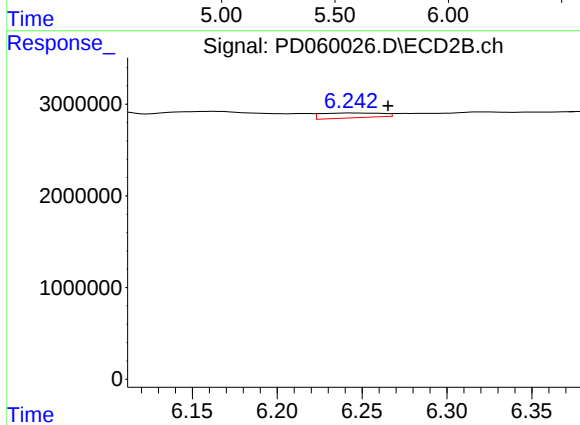


#9 Endosulfan I

R.T.: 6.244 min
Delta R.T.: -0.021 min
Response: 1308009
Conc: 0.40 ng/ml

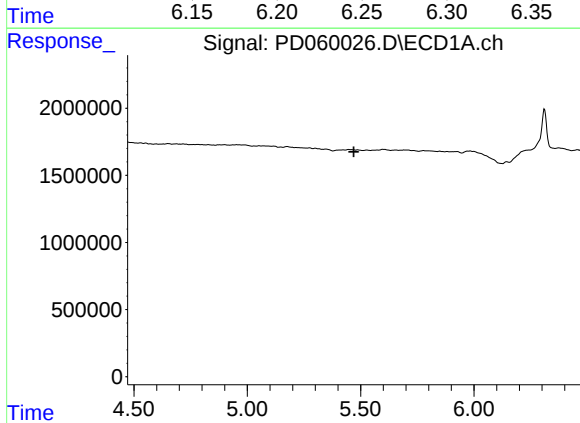


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.470 min
Response: 0
Conc: N.D.

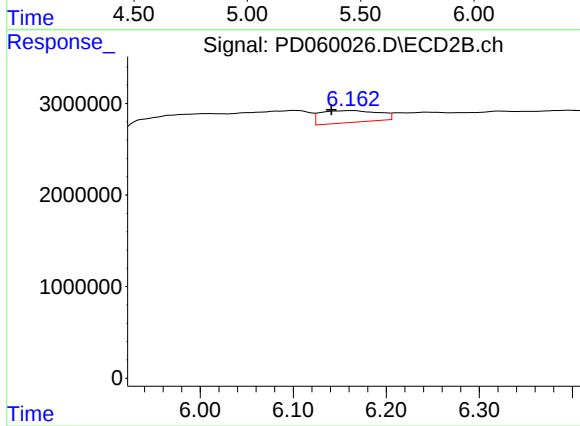

#10 gamma-Chlordane


R.T.: 6.163 min
Delta R.T.: 0.022 min
Response: 5655482
Conc: 1.60 ng/ml

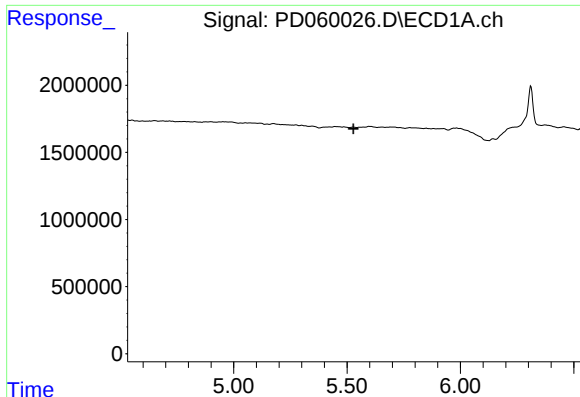

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

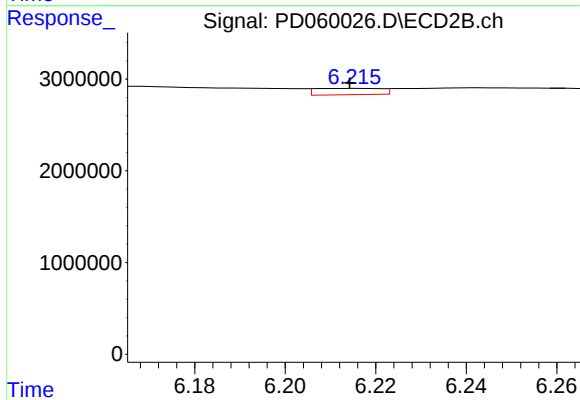


#11 alpha-Chlordane

R.T.: 6.216 min
Delta R.T.: 0.002 min
Response: 696638
Conc: 0.20 ng/ml

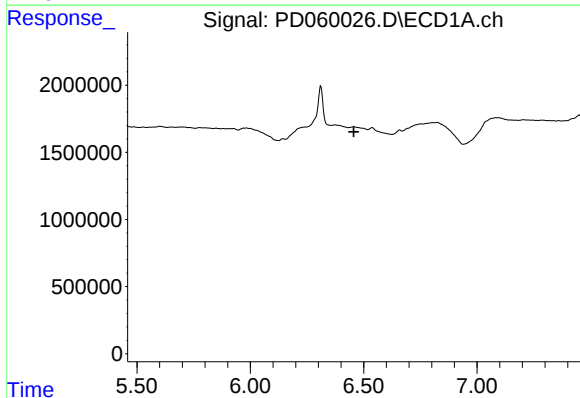


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.456 min
Response: 0
Conc: N.D.

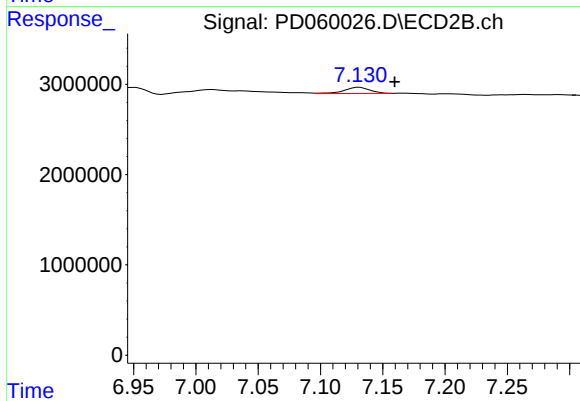

#17 4,4'-DDT


R.T.: 7.131 min
Delta R.T.: -0.028 min
Response: 986496
Conc: 0.35 ng/ml

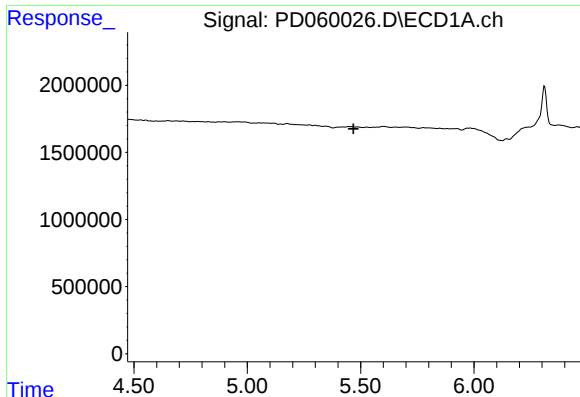

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

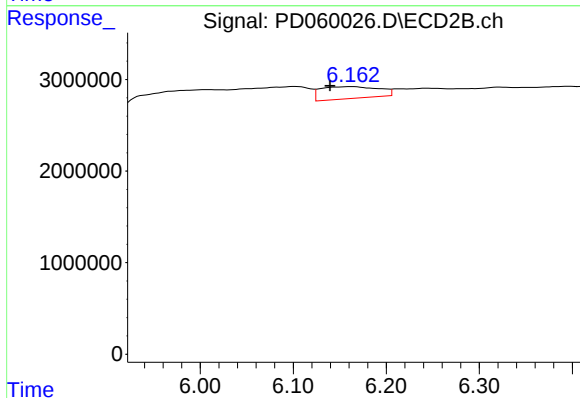


#25 Chlordane-3

R.T.: 6.163 min
Delta R.T.: 0.023 min
Response: 5655482
Conc: 13.36 ng/ml

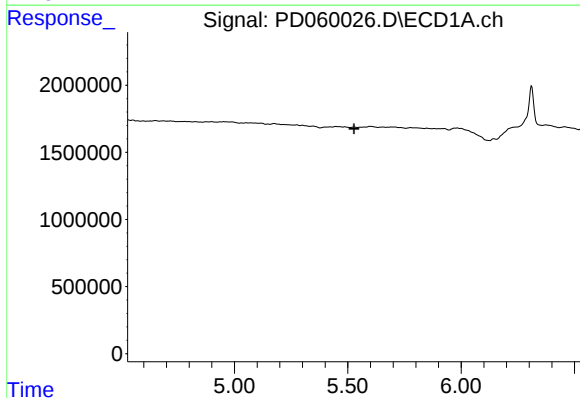


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.528 min
Response: 0
Conc: N.D.

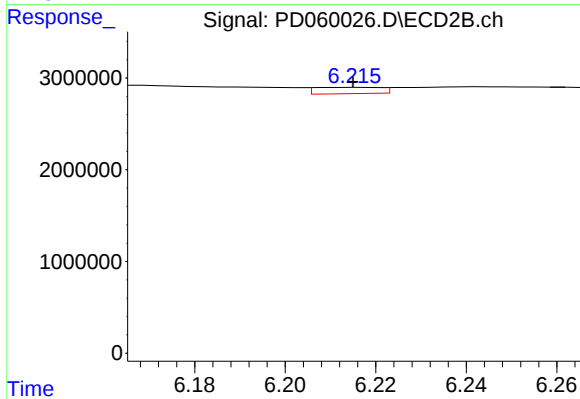

#26 Chlordane-4


R.T.: 6.216 min
Delta R.T.: 0.001 min
Response: 696638
Conc: 1.39 ng/ml

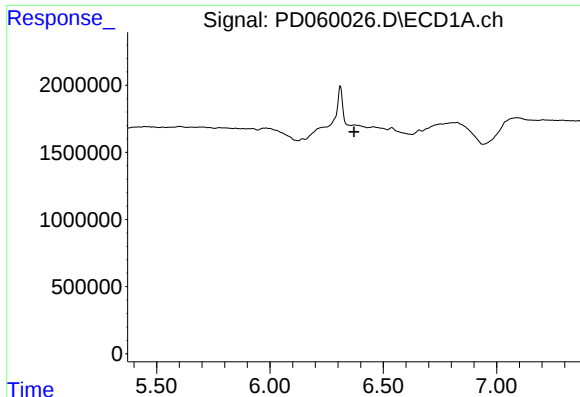

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

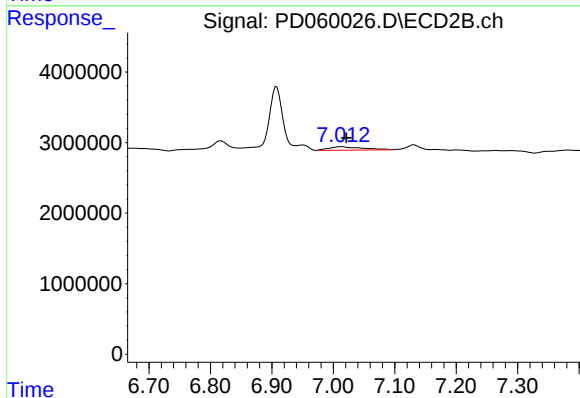


#27 Chlordane-5

R.T.: 7.013 min
Delta R.T.: -0.008 min
Response: 1899179
Conc: 20.52 ng/ml

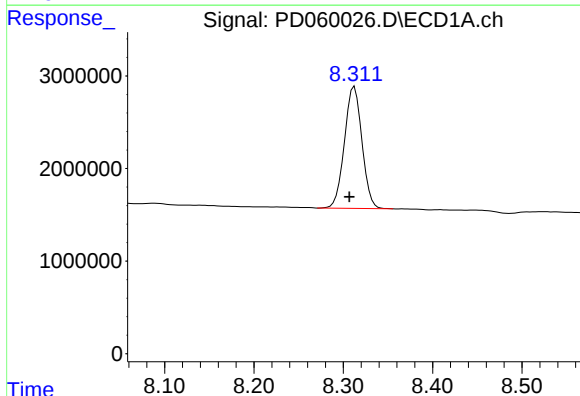

#28 Decachlorobiphenyl

R.T.: 8.312 min
Delta R.T.: 0.006 min
Response: 17908307
Conc: 21.28 ng/ml

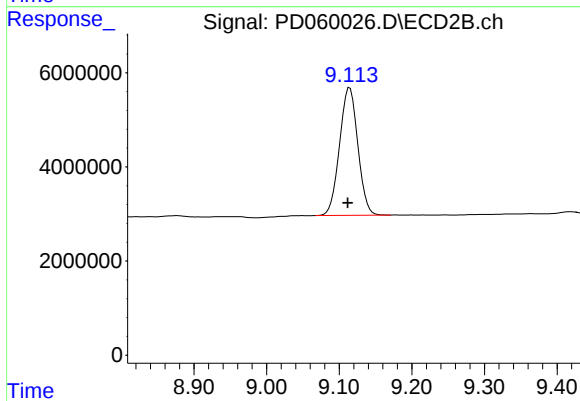

#28 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.003 min
Response: 47514831
Conc: 20.95 ng/ml