

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110220\
 Data File : PD060023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2020 15:24
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:23:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110220.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 03 01:23:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.505	4.024	45411420	141.1E6	50.000	50.000
28)	SA Decachlor...	8.306	9.110	40230797	105.8E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.387	5.023	14673089	56550300	500.000	500.000
24)	Chlordane-2	4.893	5.492	15483903	54704869	500.000	500.000
25)	Chlordane-3	5.469	6.140	45892714	211.6E6	500.000	500.000
26)	Chlordane-4	5.528	6.215	37994120	250.4E6	500.000	500.000
27)	Chlordane-5	6.371	7.021	16900626	46279611	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110220\
Data File : PD060023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2020 15:24
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:23:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110220.M
Quant Title : GC Extractables
QLast Update : Tue Nov 03 01:23:28 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

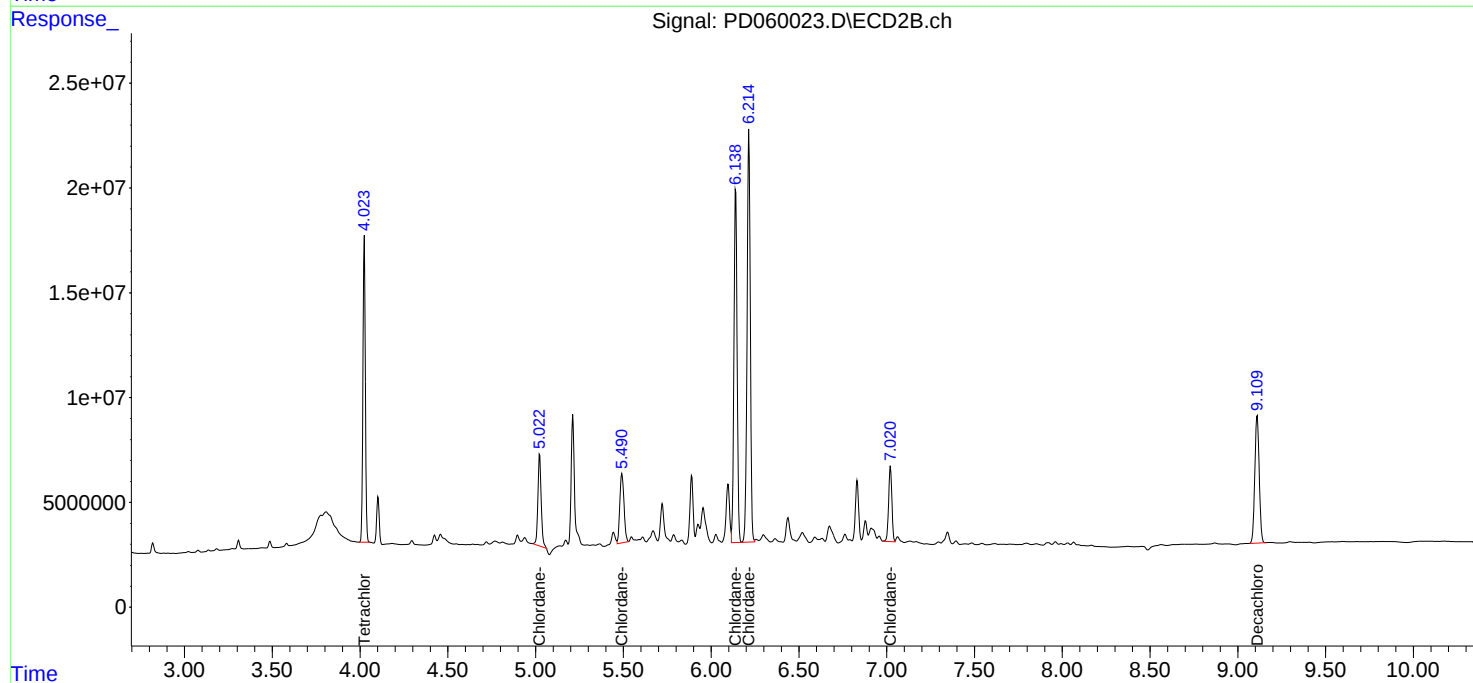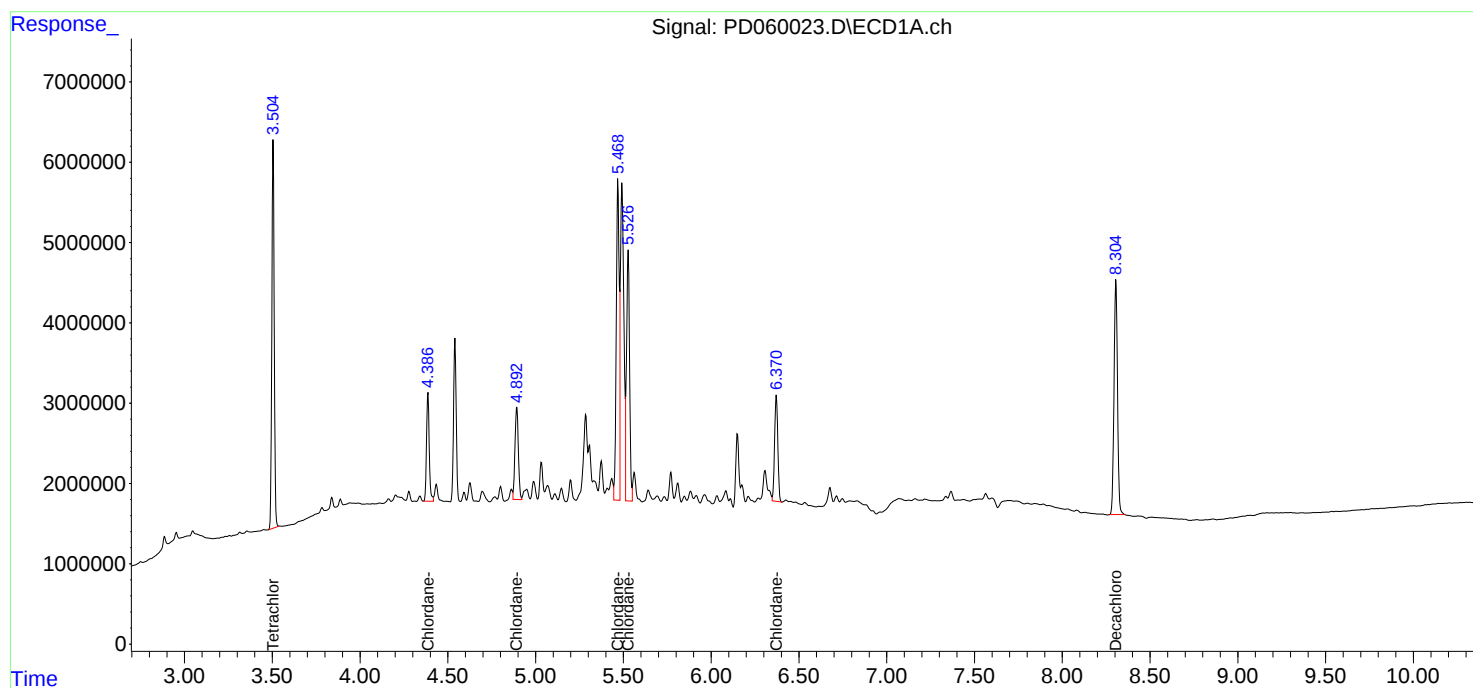


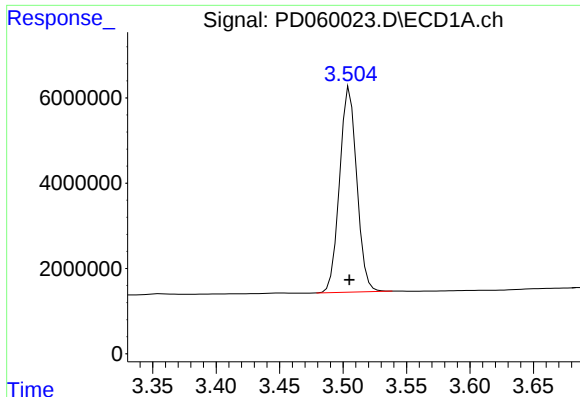

#1 Tetrachloro-m-xylene


R.T.: 3.505 min
Delta R.T.: 0.000 min
Response: 45411420
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

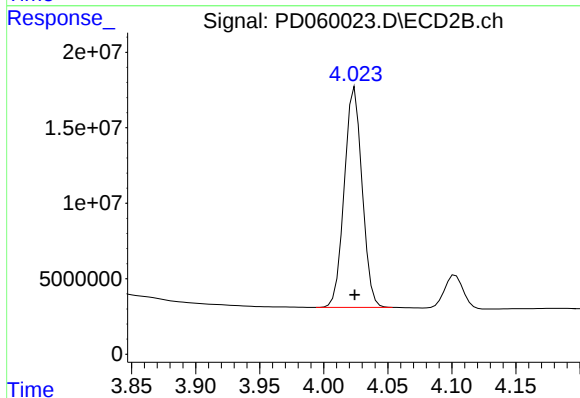


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 141072386
Conc: 50.00 ng/ml

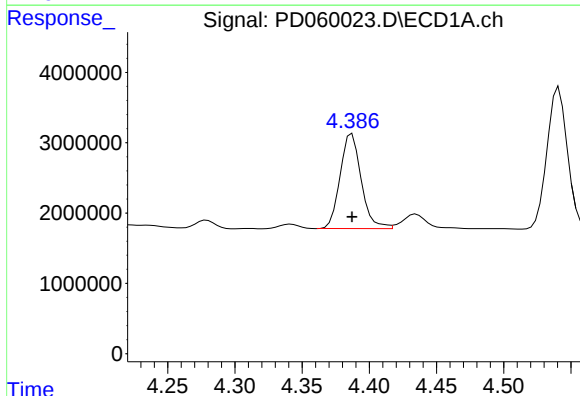


#23 Chlordane-1

R.T.: 4.387 min
Delta R.T.: 0.000 min
Response: 14673089
Conc: 500.00 ng/ml

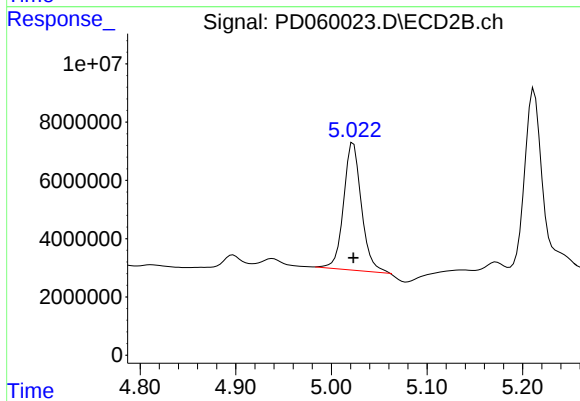

#23 Chlordane-1


R.T.: 5.023 min
Delta R.T.: 0.000 min
Response: 56550300
Conc: 500.00 ng/ml

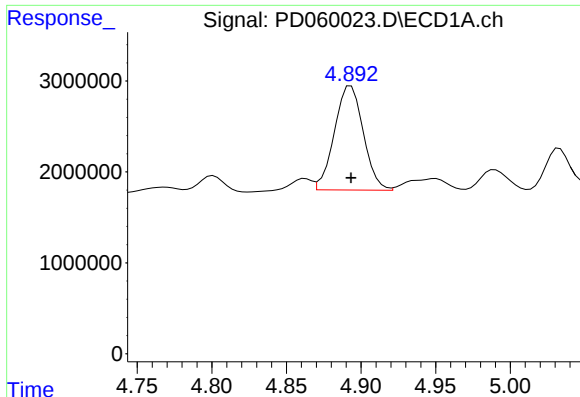

#24 Chlordane-2


R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 15483903
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

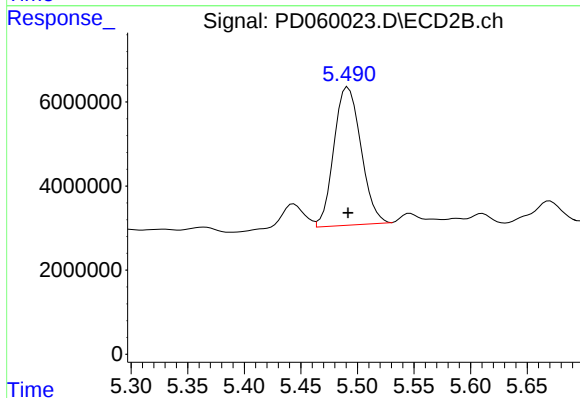


#24 Chlordane-2

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 54704869
Conc: 500.00 ng/ml

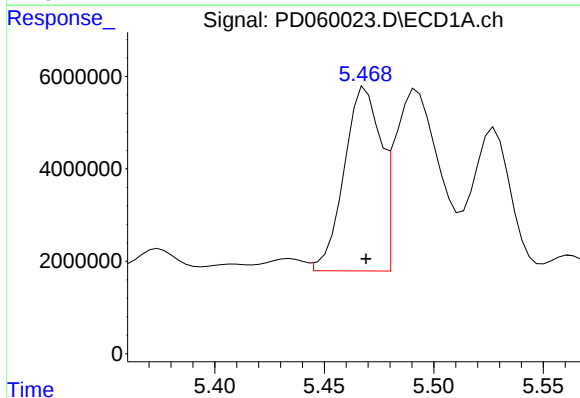


#25 Chlordane-3

R.T.: 5.469 min
Delta R.T.: 0.000 min
Response: 45892714
Conc: 500.00 ng/ml

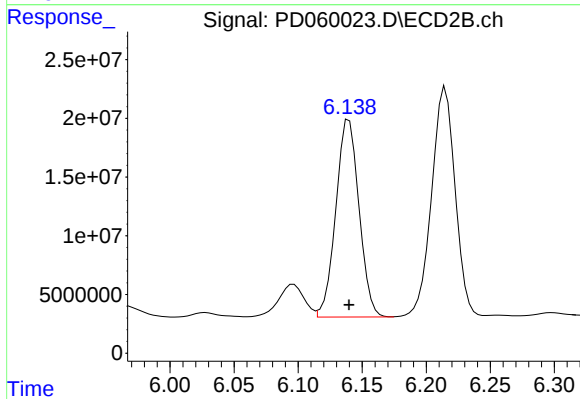

#25 Chlordane-3


R.T.: 6.140 min
Delta R.T.: 0.000 min
Response: 211625829
Conc: 500.00 ng/ml

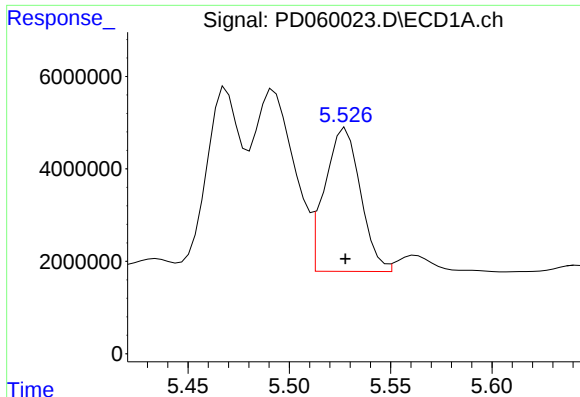

#26 Chlordane-4


R.T.: 5.528 min
Delta R.T.: 0.000 min
Response: 37994120
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

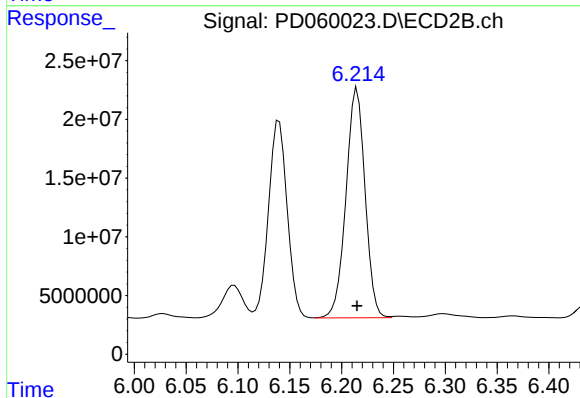


#26 Chlordane-4

R.T.: 6.215 min
Delta R.T.: 0.000 min
Response: 250439818
Conc: 500.00 ng/ml

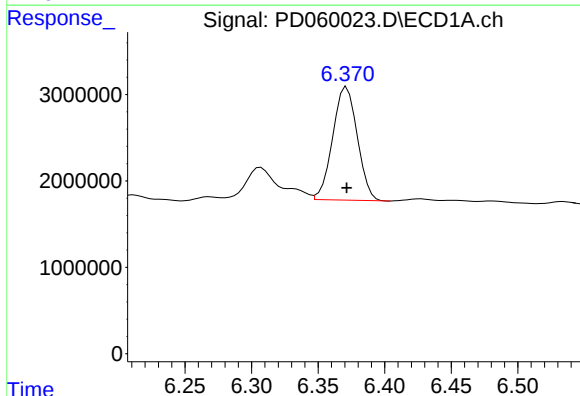


#27 Chlordane-5

R.T.: 6.371 min
Delta R.T.: 0.000 min
Response: 16900626
Conc: 500.00 ng/ml

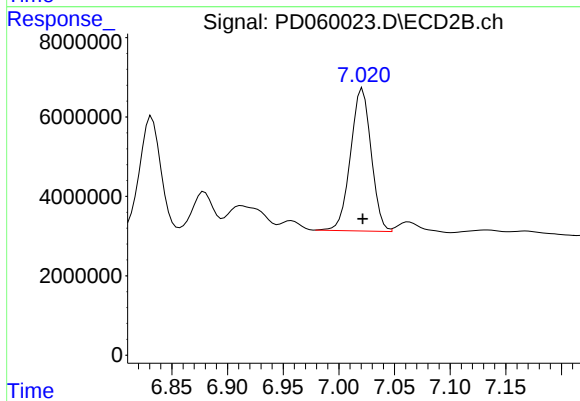

#27 Chlordane-5


R.T.: 7.021 min
Delta R.T.: 0.000 min
Response: 46279611
Conc: 500.00 ng/ml

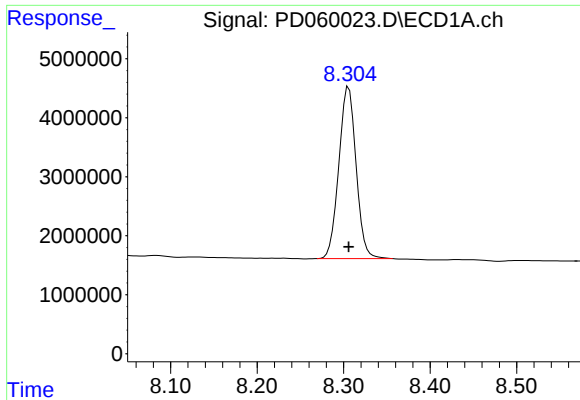

#28 Decachlorobiphenyl

R.T.: 8.306 min
Delta R.T.: 0.000 min
Response: 40230797
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

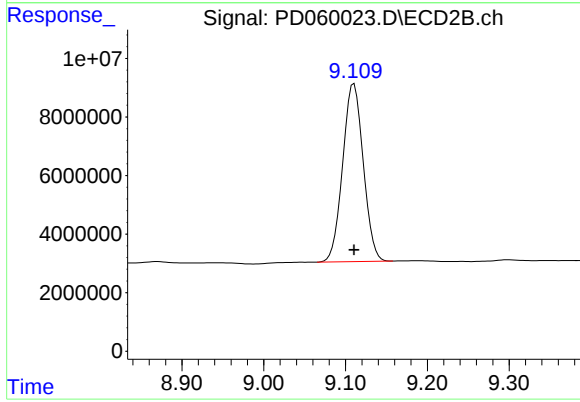

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 105833813
Conc: 50.00 ng/ml