

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110222\
 Data File : PD072777.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2022 14:52
 Operator : AR\AJ
 Sample : PB148764BS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS764

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/03/2022
 Supervised By : Ankita Jodhani 11/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 22:31:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.703	3.463	39930512	721.5E6	17.175	18.006
27)	SA Decachlor...	7.835	8.918	76644040	400.7E6	39.046	42.608
Target Compounds							
2)	A alpha-BHC	3.206	3.927	14256130	259.0E6	4.083	4.883
3)	MA gamma-BHC...	3.537	4.261	13865501	215.0E6	4.375	5.058
4)	MA Heptachlor	3.869	4.828	13557078	146.7E6	4.178	4.934
5)	MB Aldrin	4.149	5.166	14153677	130.6E6	4.468	5.212
6)	B beta-BHC	3.839	4.476	6876500	82767775	4.526	4.879
7)	B delta-BHC	4.069	4.720	13659713	166.9E6	4.075	4.881
8)	B Heptachlo...	4.654	5.599	13115500	105.8E6	4.612	5.115
9)	A Endosulfan I	5.023	5.983	12247566	92163730	4.828	5.320
10)	B trans-Chl...	4.902	5.852	12928928	99219784	4.405	4.954
11)	B cis-Chlor...	4.965	5.927	13074643	98289631	4.580	5.043
12)	B 4,4'-DDE	5.154	6.101	22778357	175.5E6	8.368	9.828
13)	MA Dieldrin	5.289	6.260	24658805	189.4E6	8.950	10.631
14)	MA Endrin	5.566	6.492	19154402	137.3E6	7.904	9.386
15)	B Endosulfa...	5.865	6.721	22196021	157.3E6	9.438	11.012
16)	A 4,4'-DDD	5.713	6.626	20578260	153.6E6	9.664	11.379
17)	MA 4,4'-DDT	5.962	6.934	17687623	128.5E6	8.164	9.510
18)	B Endrin al...	6.046	6.853	19148952	128.9E6	9.725	10.753
19)	B Endosulfa...	6.270	7.085	20750484	130.4E6	9.066	9.908
20)	A Methoxychlor	6.544	7.412	47483906	273.3E6	40.904m	45.190m
21)	B Endrin ke...	6.780	7.575	26794779	162.9E6	10.046	11.370

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110222\
Data File : PD072777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2022 14:52
Operator : AR\AJ
Sample : PB148764BS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 22:31:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

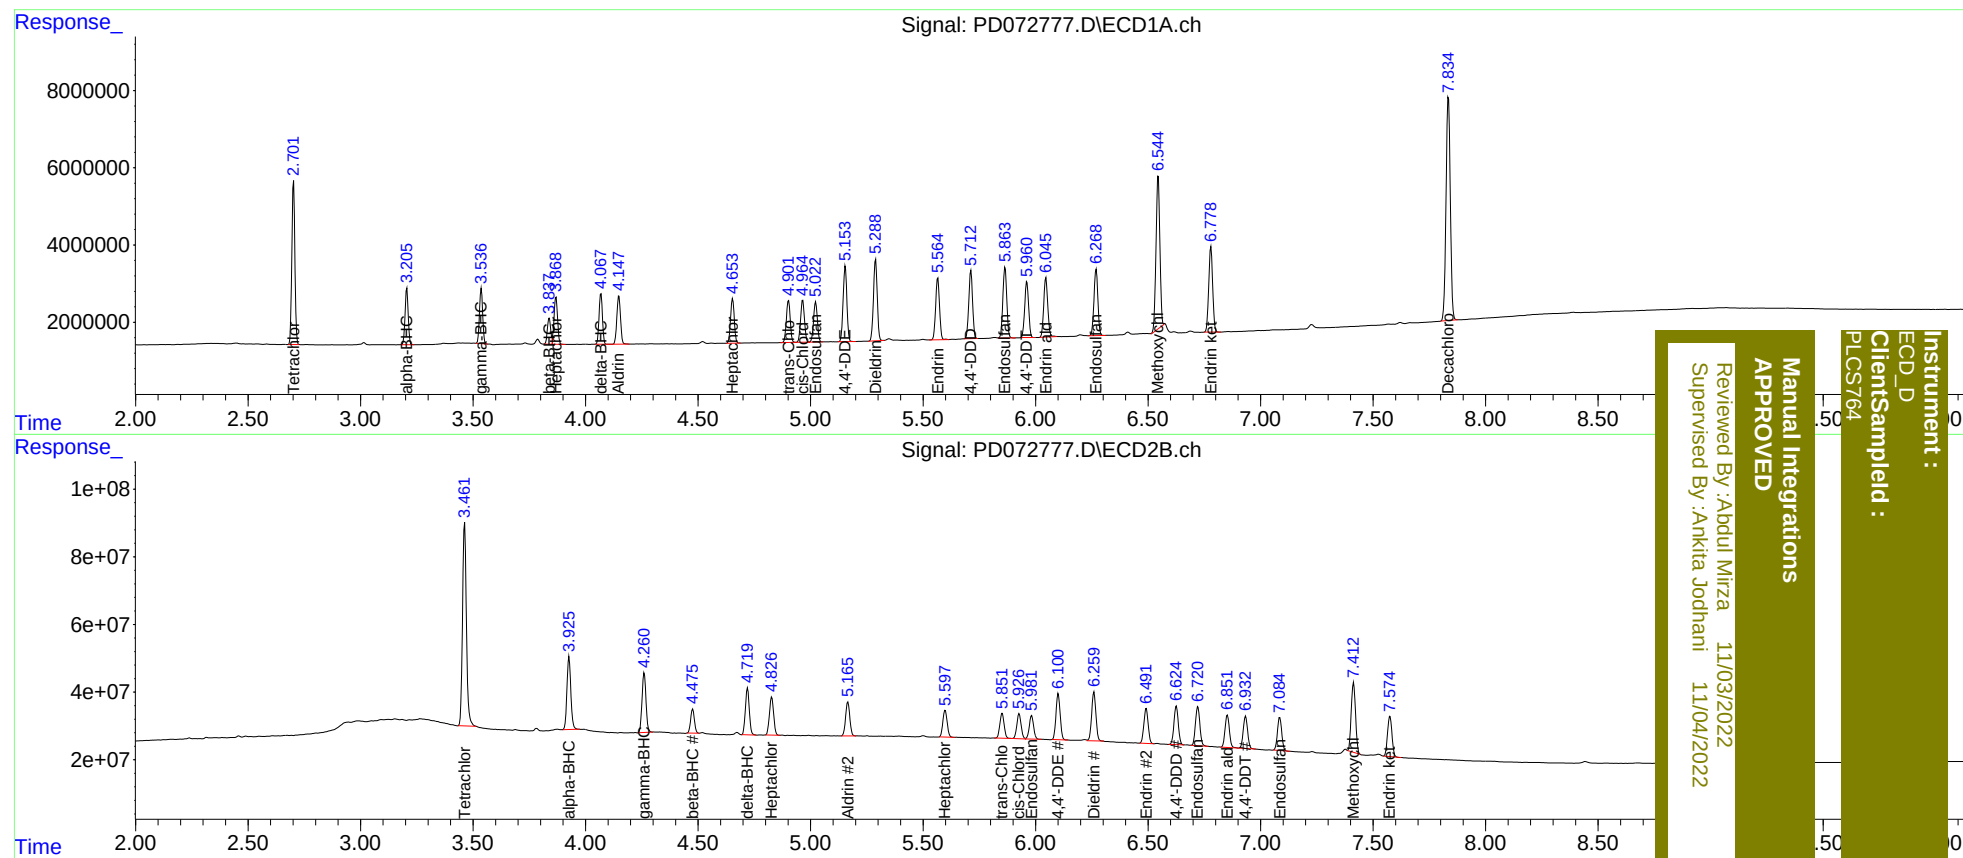

Instrument :
ECD_D
ClientSampled :
PLC5764

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/03/2022
Supervised By :Ankita Jodhani 11/04/2022