

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110222\
 Data File : PD072790.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2022 19:01
 Operator : AR\AJ
 Sample : N5353-15MSD
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBWW9MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/03/2022
 Supervised By : Ankita Jodhani 11/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 22:41:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.703	3.465	33017963	738.7E6	14.202	18.434 #
27)	SA Decachlor...	7.833	8.915	36435377	198.3E6	18.562	21.087
Target Compounds							
2)	A alpha-BHC	3.207	3.928	118.9E6	1574.5E6	34.063	29.681
3)	MA gamma-BHC...	3.537	4.262	116.8E6	1395.6E6	36.860	32.841
4)	MA Heptachlor	3.869	4.826	115.8E6	1102.0E6	35.701	37.063m
5)	MB Aldrin	4.148	5.167	131.4E6	851.4E6	41.472	33.972
6)	B beta-BHC	3.839	4.477	59503268	543.9E6	39.165	32.058
7)	B delta-BHC	4.073	4.721	35617658	167.3E6	10.626m	4.893 #
8)	B Heptachlo...	4.653	5.599	111.5E6	757.2E6	39.219	36.621
9)	A Endosulfan I	5.022	5.984	104.3E6	699.7E6	41.118	40.388
10)	B trans-Chl...	4.902	5.852	112.5E6	794.0E6	38.337	39.645
11)	B cis-Chlor...	4.965	5.928	107.7E6	739.8E6	37.736	37.958
12)	B 4,4'-DDE	5.153	6.101	223.0E6	1428.5E6	81.939	79.996
13)	MA Dieldrin	5.288	6.260	243.6E6	1542.2E6	88.428	86.548
14)	MA Endrin	5.565	6.492	231.7E6	1157.7E6	95.624	79.133
15)	B Endosulfa...	5.863	6.721	200.2E6	1266.0E6	85.124	88.623
16)	A 4,4'-DDD	5.712	6.625	180.7E6	1150.1E6	84.874	85.220
17)	MA 4,4'-DDT	5.960	6.933	181.6E6	1204.7E6	83.805	89.133
18)	B Endrin al...	6.044	6.852	148.0E6	937.4E6	75.165	78.228
19)	B Endosulfa...	6.268	7.085	128.1E6	789.2E6	55.944	59.961
20)	A Methoxychlor	6.544	7.412	497.3E6	2697.2E6	428.353	445.915
21)	B Endrin ke...	6.778	7.574	227.7E6	1269.2E6	85.379	88.604

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110222\
Data File : PD072790.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2022 19:01
Operator : AR\AJ
Sample : N5353-15MSD
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 22:41:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

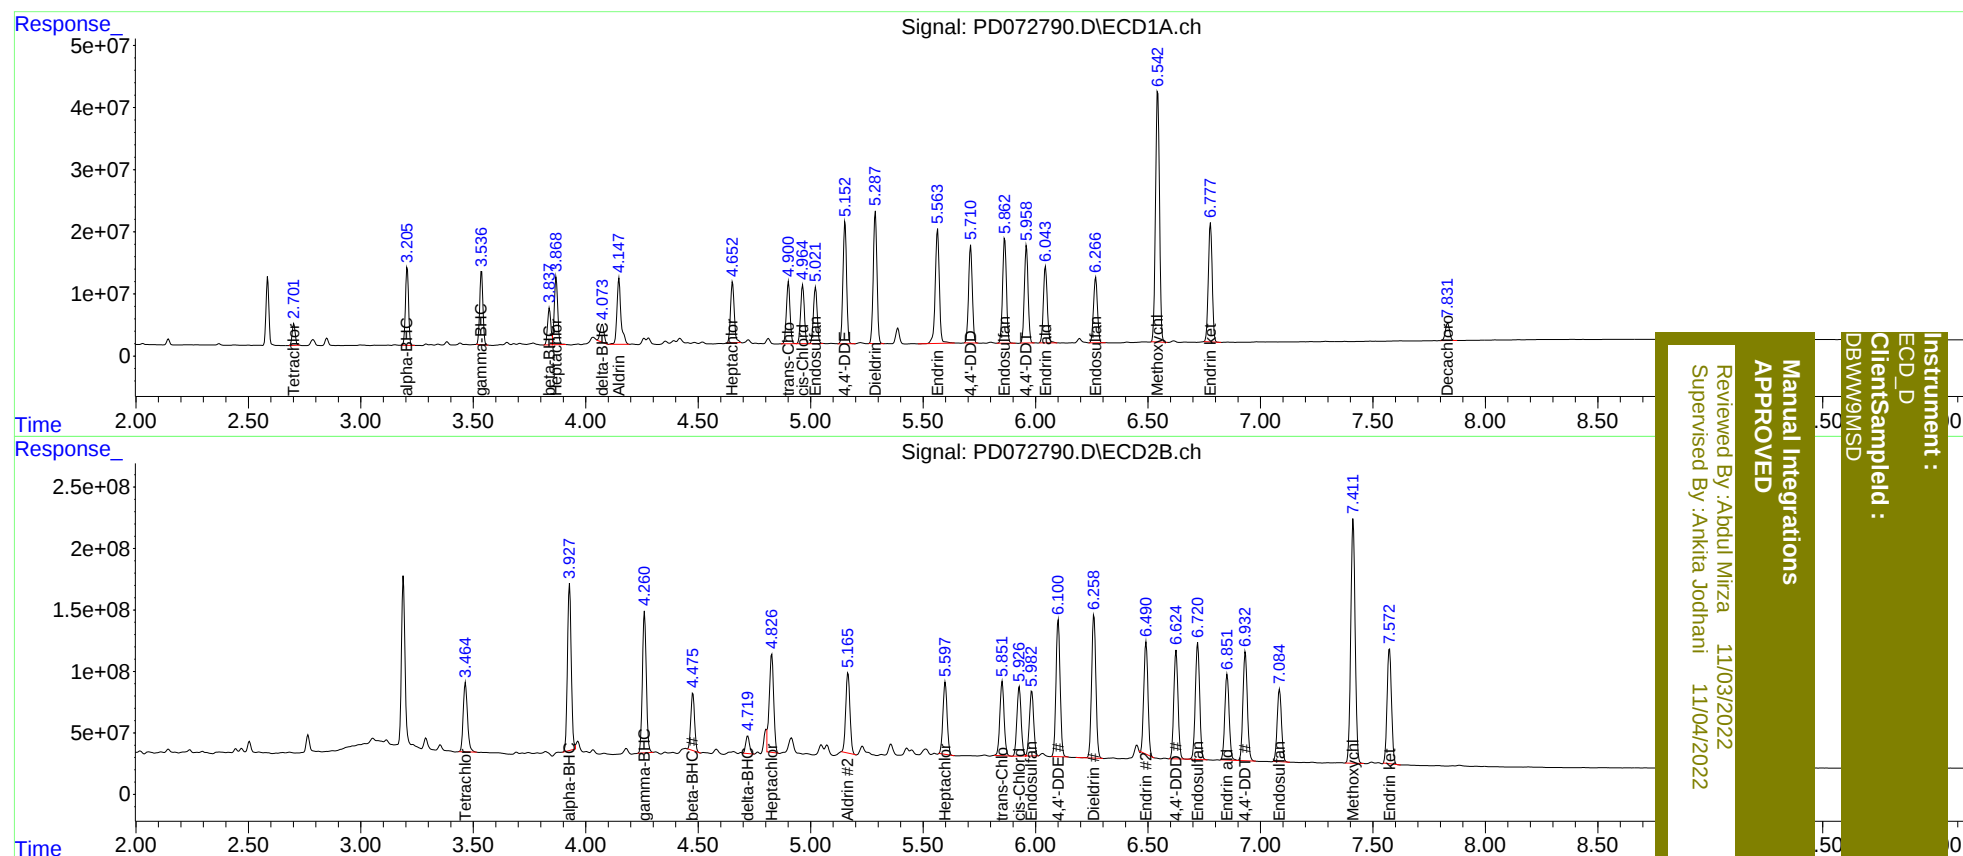

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/03/2022
Supervised By: Ankita Jodhani 11/04/2022

Instrument :
ECD_D
Client Sampled :
DBWM9MSD