

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110222\
 Data File : PD072769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2022 11:05
 Operator : AR\AJ
 Sample : N5321-10DL2 40X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBWM6DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/04/2022
 Supervised By : Ankita Jodhani 11/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 22:21:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
2) A	alpha-BHC	3.208	3.928	267.6E6	3512.1E6	76.625 66.207
3) MA	gamma-BHC...	3.538	4.261	46230092	623.5E6	14.586 14.671
6) B	beta-BHC	3.840	4.476	19960157	223.8E6	13.138 13.193
7) B	delta-BHC	4.070	4.721	53269942	558.0E6	15.892 16.322
13) MA	Dieldrin	5.289	6.261	15642950	128.8E6	5.677m 7.227 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110222\
Data File : PD072769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2022 11:05
Operator : AR\AJ
Sample : N5321-10DL2 40X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 22:21:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

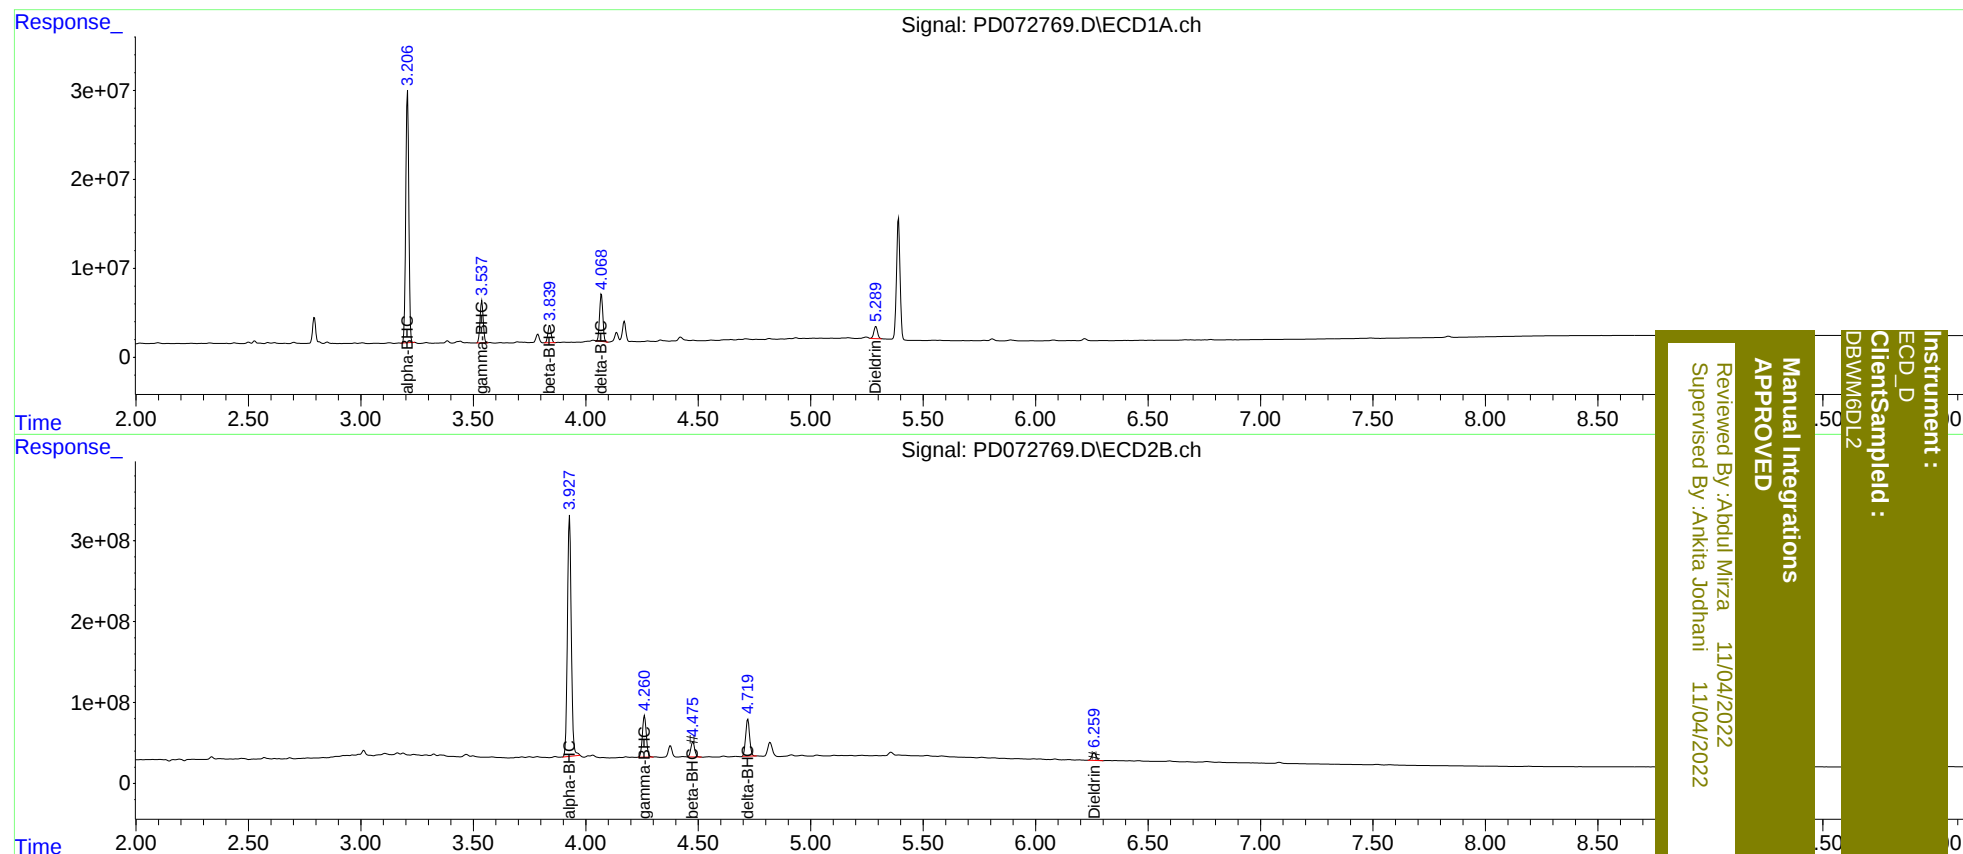

Instrument :
ECD_D
ClientSampled :
DBWM6DL2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/04/2022
Supervised By :Ankita Jodhani 11/04/2022