

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110222\
 Data File : PD072789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2022 18:48
 Operator : AR\AJ
 Sample : N5353-14MS
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBWW9MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/03/2022
 Supervised By : Ankita Jodhani 11/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 22:41:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.703	3.466	32979666	740.3E6	14.185	18.474 #
27)	SA Decachlor...	7.833	8.917	36597110	200.8E6	18.644	21.352
Target Compounds							
2)	A alpha-BHC	3.206	3.929	119.4E6	1566.9E6	34.199	29.538
3)	MA gamma-BHC...	3.537	4.262	117.7E6	1394.6E6	37.124	32.817
4)	MA Heptachlor	3.869	4.826	115.7E6	1102.3E6	35.667	37.074m
5)	MB Aldrin	4.148	5.167	132.7E6	856.7E6	41.891	34.181
6)	B beta-BHC	3.838	4.477	59786944	536.5E6	39.351	31.624
7)	B delta-BHC	4.072	4.720	35318085	168.4E6	10.536m	4.925m#
8)	B Heptachlo...	4.653	5.599	111.5E6	788.4E6	39.205	38.129
9)	A Endosulfan I	5.022	5.984	104.4E6	696.6E6	41.168	40.208
10)	B trans-Chl...	4.902	5.853	112.5E6	790.7E6	38.337	39.482
11)	B cis-Chlor...	4.965	5.928	108.4E6	736.5E6	37.976	37.787
12)	B 4,4'-DDE	5.154	6.102	224.3E6	1418.1E6	82.391	79.417
13)	MA Dieldrin	5.289	6.260	244.6E6	1545.3E6	88.788	86.721
14)	MA Endrin	5.565	6.492	231.1E6	1184.2E6	95.341	80.950
15)	B Endosulfa...	5.863	6.721	201.3E6	1262.9E6	85.594	88.404
16)	A 4,4'-DDD	5.712	6.626	182.2E6	1150.8E6	85.576	85.271
17)	MA 4,4'-DDT	5.960	6.934	180.8E6	1199.0E6	83.473	88.706
18)	B Endrin al...	6.045	6.853	148.3E6	943.3E6	75.333	78.722
19)	B Endosulfa...	6.268	7.086	128.7E6	795.8E6	56.220	60.462
20)	A Methoxychlor	6.544	7.413	497.2E6	2686.6E6	428.273	444.155
21)	B Endrin ke...	6.778	7.575	229.8E6	1283.7E6	86.158	89.615

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110222\
Data File : PD072789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2022 18:48
Operator : AR\AJ
Sample : N5353-14MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 22:41:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

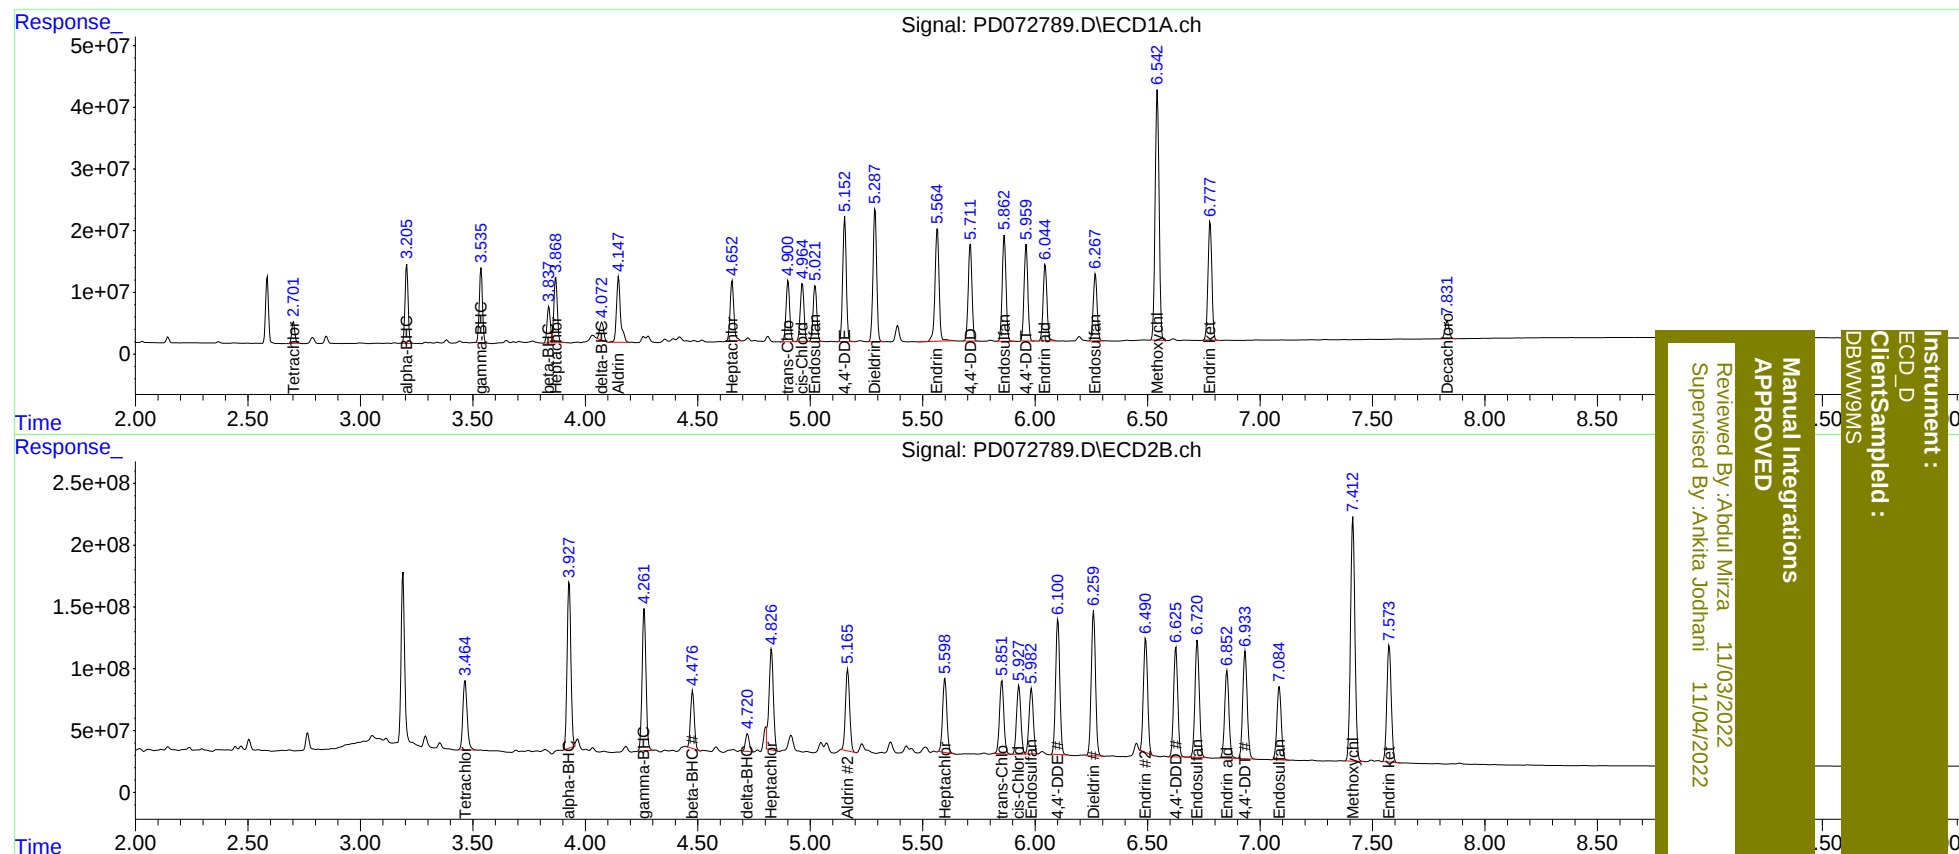

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/03/2022
Supervised By: Ankita Jodhani 11/04/2022

Instrument :
ECD_D
Client Sampled :
DBWM9MS