

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110222\
 Data File : PD072791.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2022 19:15
 Operator : AR\AJ
 Sample : N5353-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBWX1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/04/2022
 Supervised By : Ankita Jodhani 11/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 22:42:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.702	3.464	33175293	591.5E6	14.269	14.762
27)	SA Decachlor...	7.833	8.915	45849906	248.7E6	23.358	26.442
Target Compounds							
2)	A alpha-BHC	3.204	3.926	4570026	74705237	1.309m	1.408m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110222\
Data File : PD072791.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2022 19:15
Operator : AR\AJ
Sample : N5353-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 22:42:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

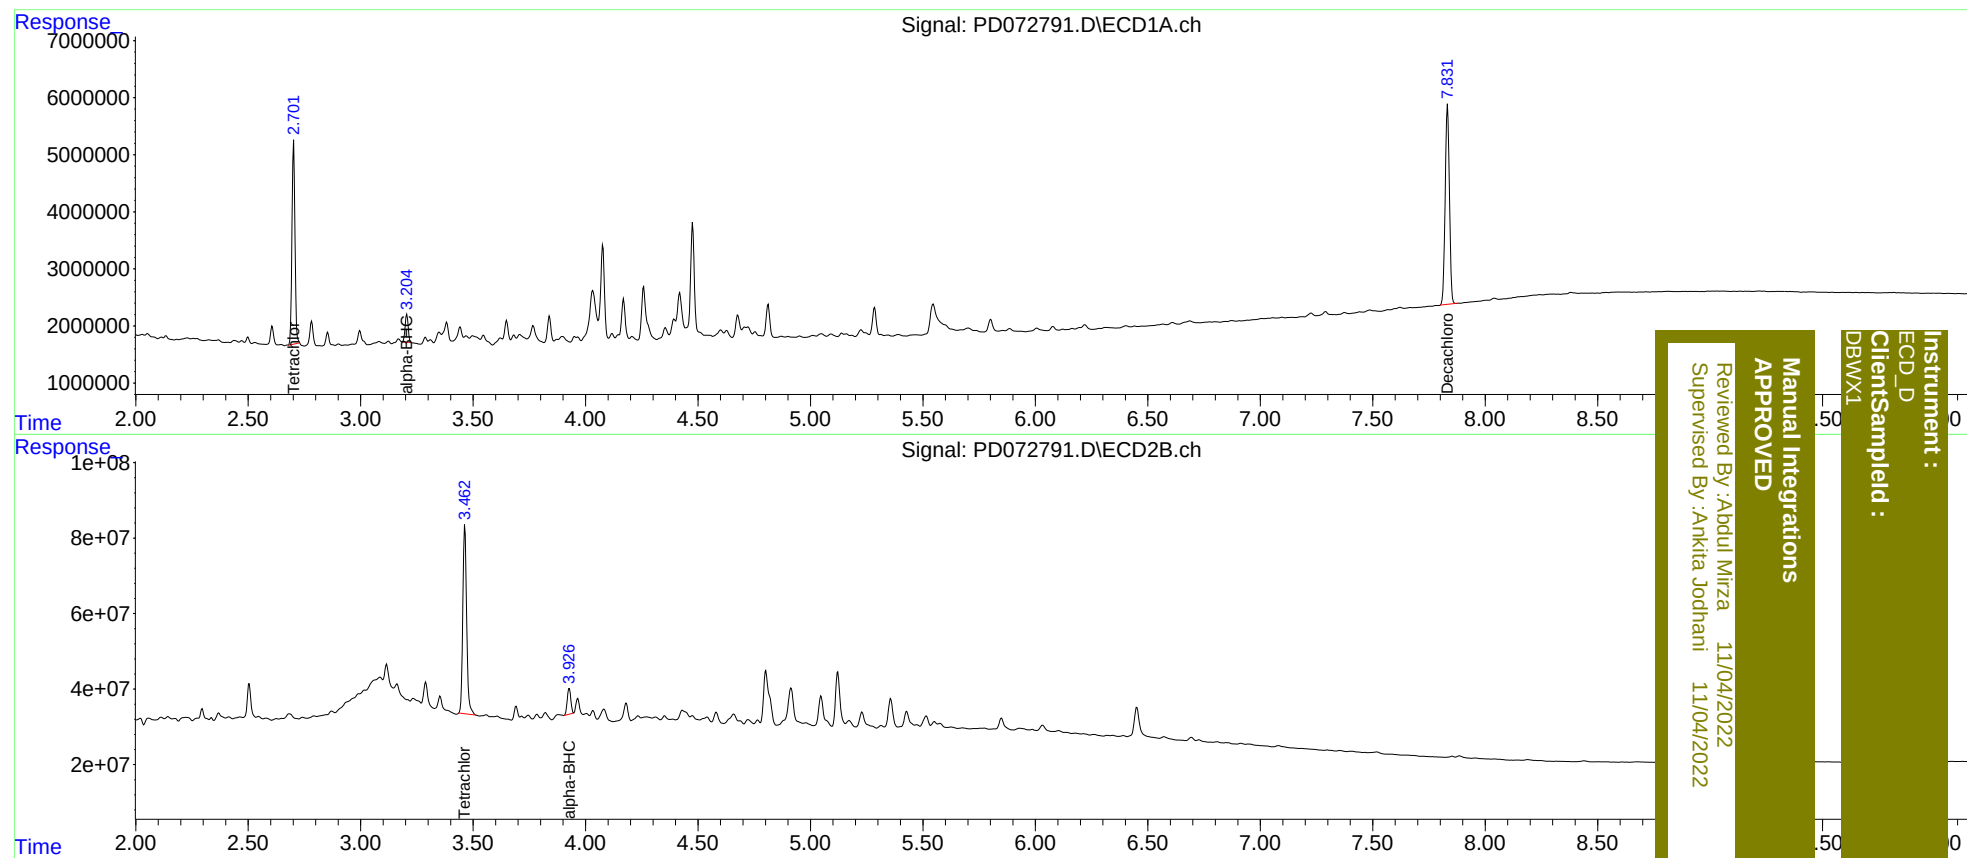

Reviewed By: Abdul Mirza 11/04/2022
Supervised By: Ankita Jodhani 11/04/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DBWX1