

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD110318\  
 Data File : PD050170.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 02 Nov 2018 13:24  
 Operator : AJ\SJ  
 Sample : PSTDCCC050  
 Misc : FOR MIREX  
 ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 03 01:34:27 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\Mirex-PD110218.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Nov 02 05:33:40 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm



|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|----------|----------|--------|--------|
| -----                       |                 |       |       |          |          |        |        |
| System Monitoring Compounds |                 |       |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 4.232 | 4.061 | 33357505 | 1437.0E6 | 51.470 | 51.704 |
| 28)                         | SA Decachlor... | 9.019 | 9.171 | 31460610 | 882.6E6  | 52.019 | 51.001 |
| Target Compounds            |                 |       |       |          |          |        |        |
| 22)                         | Mirex           | 8.162 | 8.272 | 29149623 | 762.0E6  | 52.452 | 51.912 |
| -----                       |                 |       |       |          |          |        |        |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD110318\  
Data File : PD050170.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 02 Nov 2018 13:24  
Operator : AJ\SJ  
Sample : PSTDCCC050  
Misc : FOR MIREX  
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 03 01:34:27 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\Mirex-PD110218.M  
Quant Title : GC Extractables  
QLast Update : Fri Nov 02 05:33:40 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

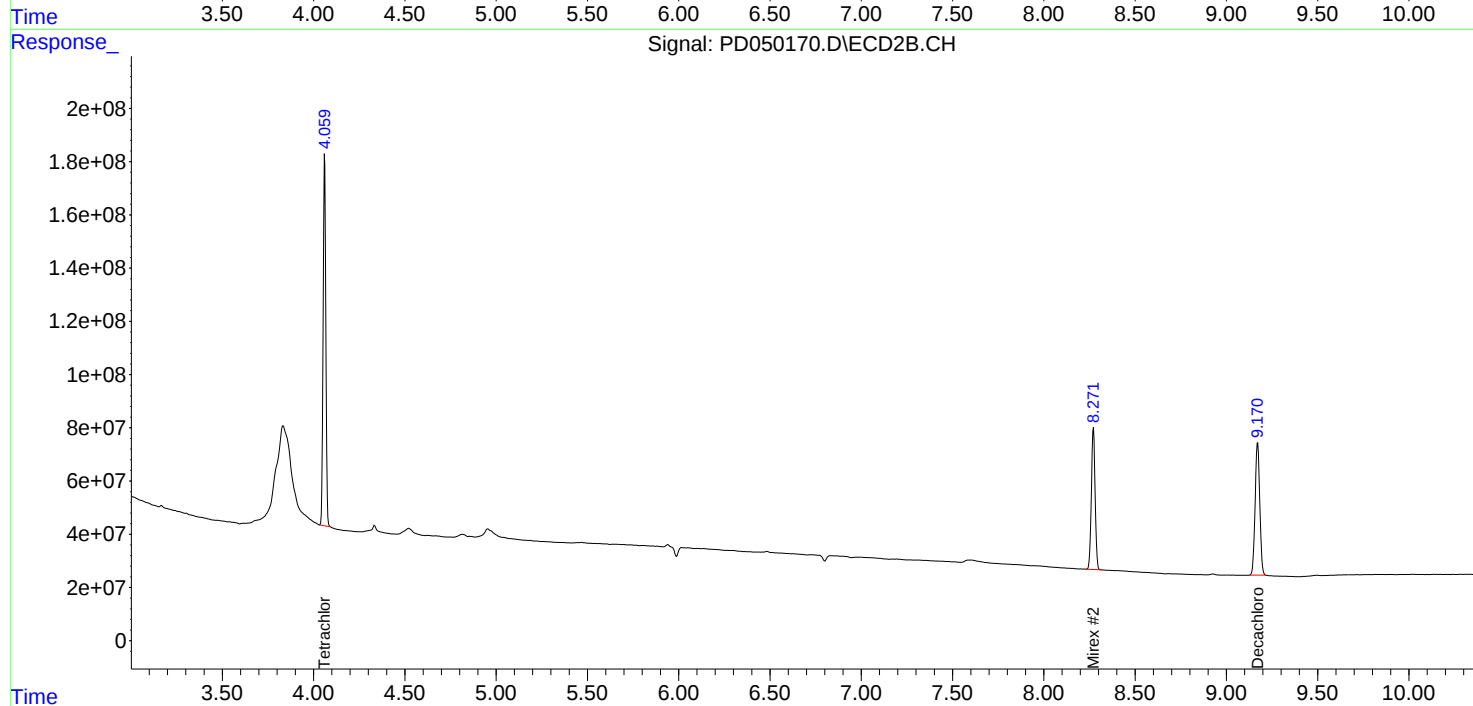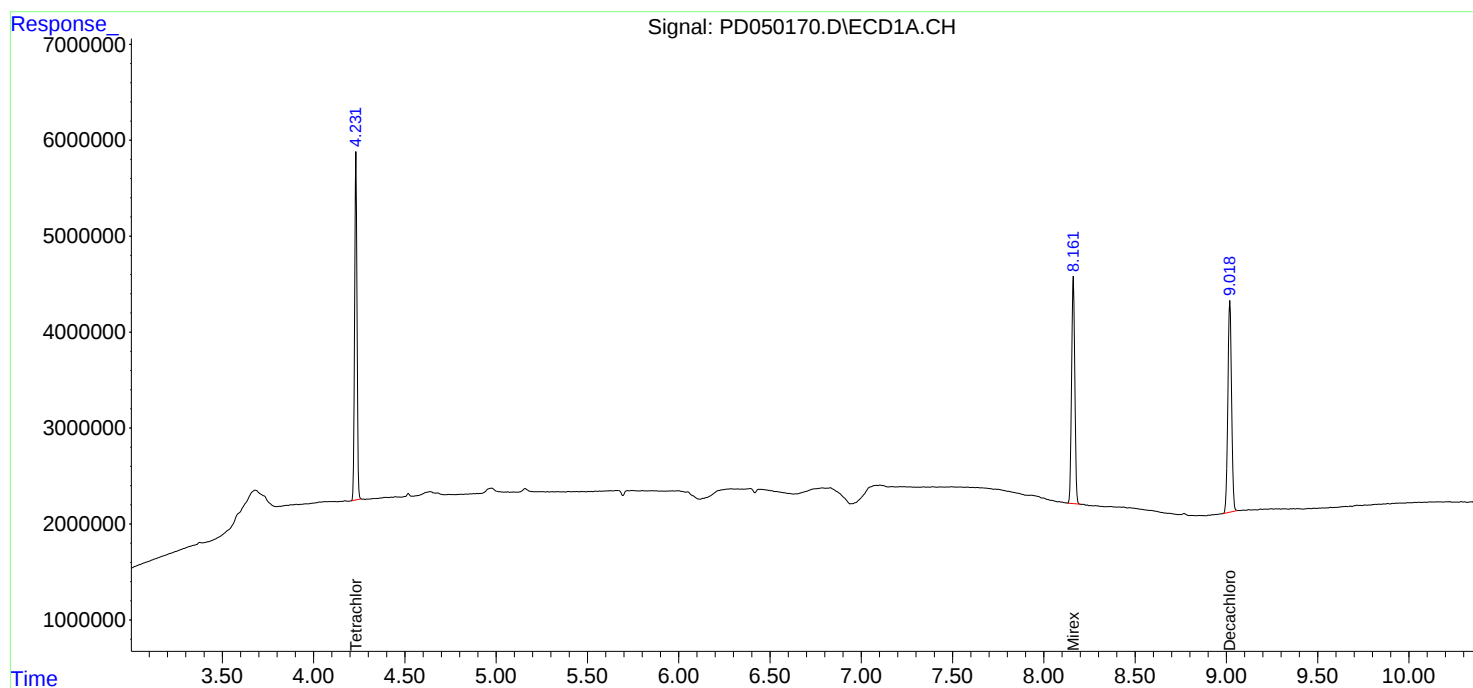

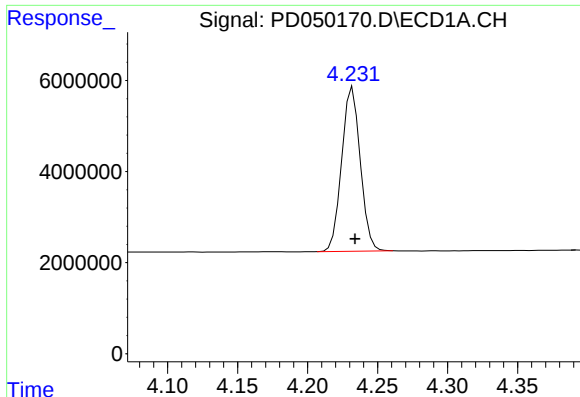


#1 Tetrachloro-m-xylene

R.T.: 4.232 min  
Delta R.T.: -0.002 min  
Response: 33357505  
Conc: 51.47 ng/ml

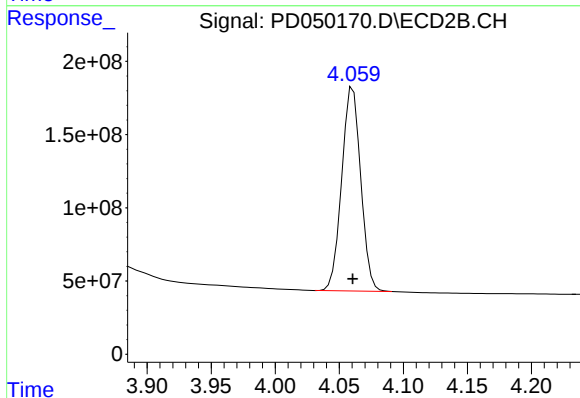


#1 Tetrachloro-m-xylene

R.T.: 4.061 min  
Delta R.T.: 0.000 min  
Response: 1436961491  
Conc: 51.70 ng/ml

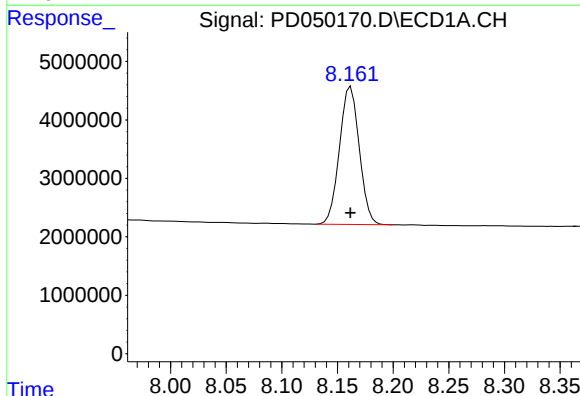


#22 Mirex

R.T.: 8.162 min  
Delta R.T.: 0.000 min  
Response: 29149623  
Conc: 52.45 ng/ml

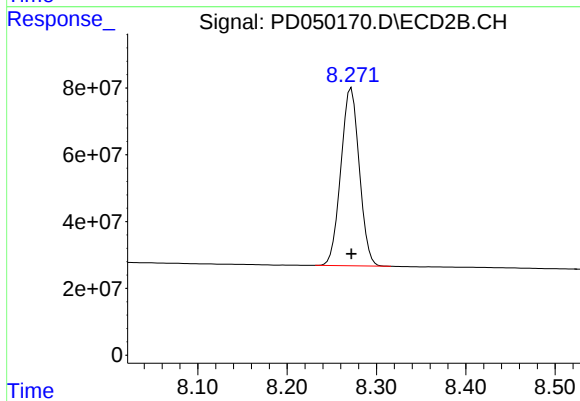


#22 Mirex

R.T.: 8.272 min  
Delta R.T.: 0.000 min  
Response: 762031745  
Conc: 51.91 ng/ml

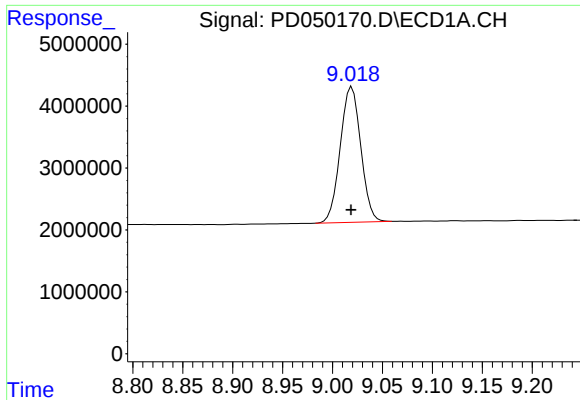

#28 Decachlorobiphenyl

R.T.: 9.019 min  
Delta R.T.: 0.000 min  
Response: 31460610  
Conc: 52.02 ng/ml

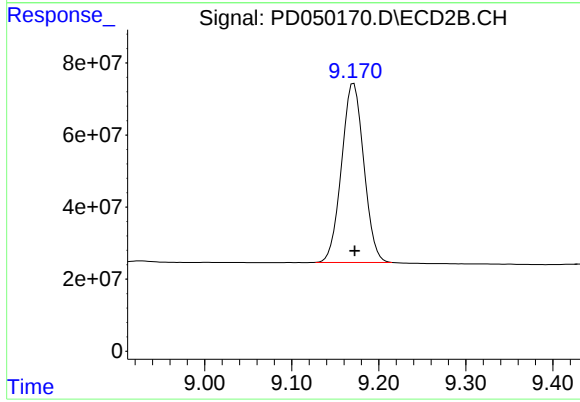

#28 Decachlorobiphenyl

R.T.: 9.171 min  
Delta R.T.: -0.001 min  
Response: 882580650  
Conc: 51.00 ng/ml