

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110318\
Data File : PD050173.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2018 14:30
Operator : AJ\SJ
Sample : MIREX-MDL-S-05
Misc : FOR MIREX
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:34:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.061	11055416	517.2E6	17.058	18.608
28)	SA Decachlor...	9.019	9.173	10739870	335.0E6	17.758	19.360
Target Compounds							
22)	Mirex	8.161	8.272	438516	14527742	0.789	0.990 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110318\
Data File : PD050173.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2018 14:30
Operator : AJ\SJ
Sample : MIREX-MDL-S-05
Misc : FOR MIREX
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:34:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

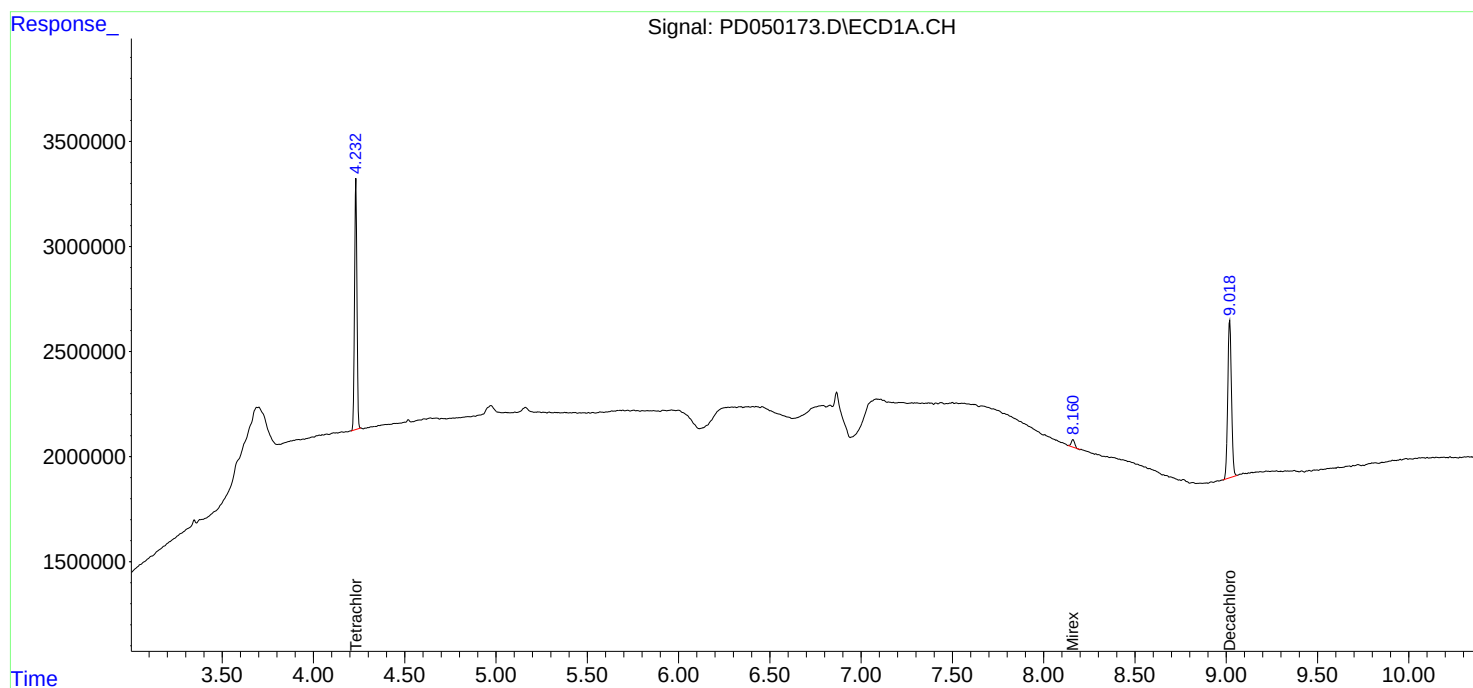

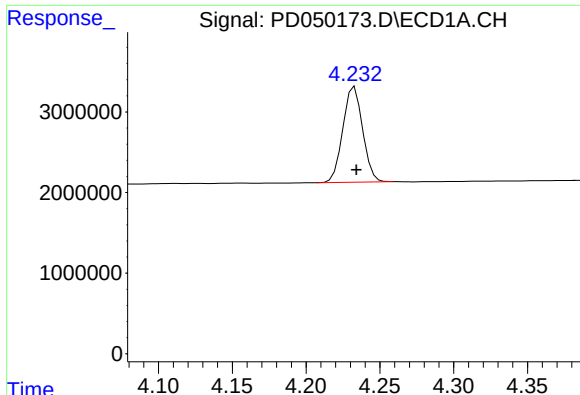


#1 Tetrachloro-m-xylene

R.T.: 4.233 min
Delta R.T.: -0.001 min
Response: 11055416
Conc: 17.06 ng/ml

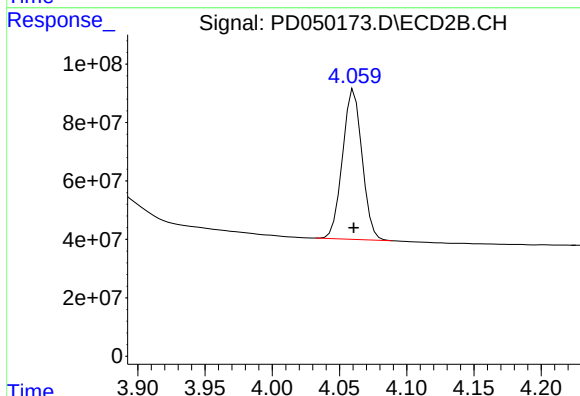


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 517161609
Conc: 18.61 ng/ml

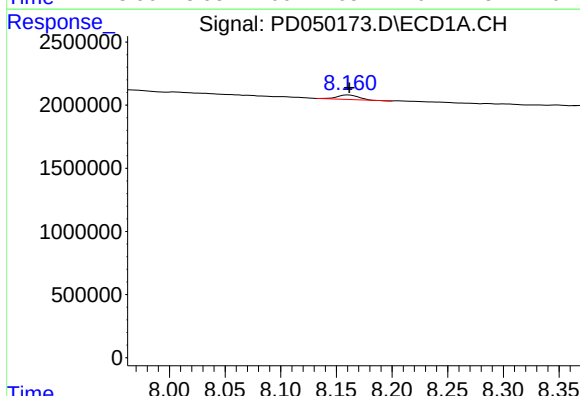


#22 Mirex

R.T.: 8.161 min
Delta R.T.: 0.000 min
Response: 438516
Conc: 0.79 ng/ml

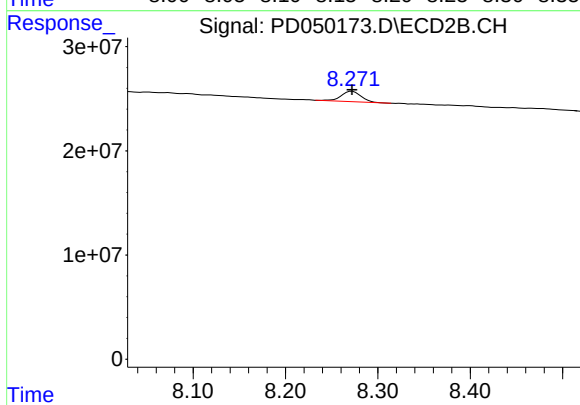


#22 Mirex

R.T.: 8.272 min
Delta R.T.: 0.000 min
Response: 14527742
Conc: 0.99 ng/ml

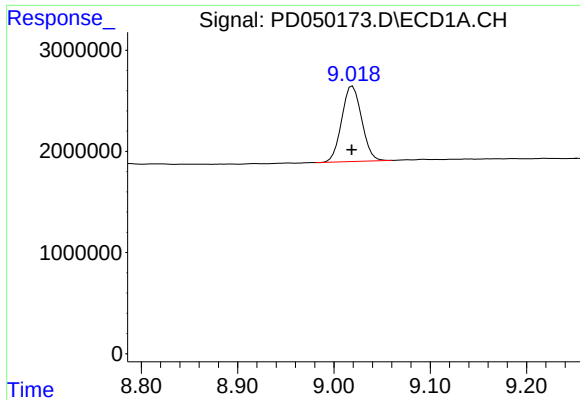

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 10739870
Conc: 17.76 ng/ml

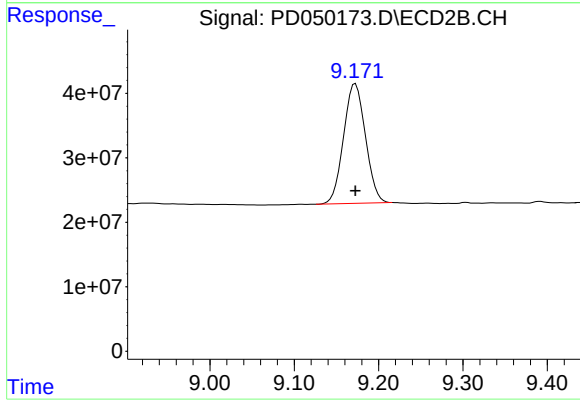

#28 Decachlorobiphenyl

R.T.: 9.173 min
Delta R.T.: 0.000 min
Response: 335026328
Conc: 19.36 ng/ml