

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110318\
Data File : PD050171.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2018 14:02
Operator : AJ\SJ
Sample : MIREX-MDL-BL-S-02
Misc : FOR MIREX
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:34:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.239	4.061	11277663	507.9E6	17.401	18.276
28)	SA Decachlor...	9.033	9.181	10575706	324.3E6	17.487	18.740



Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110318\
Data File : PD050171.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2018 14:02
Operator : AJ\SJ
Sample : MIREX-MDL-BL-S-02
Misc : FOR MIREX
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:34:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

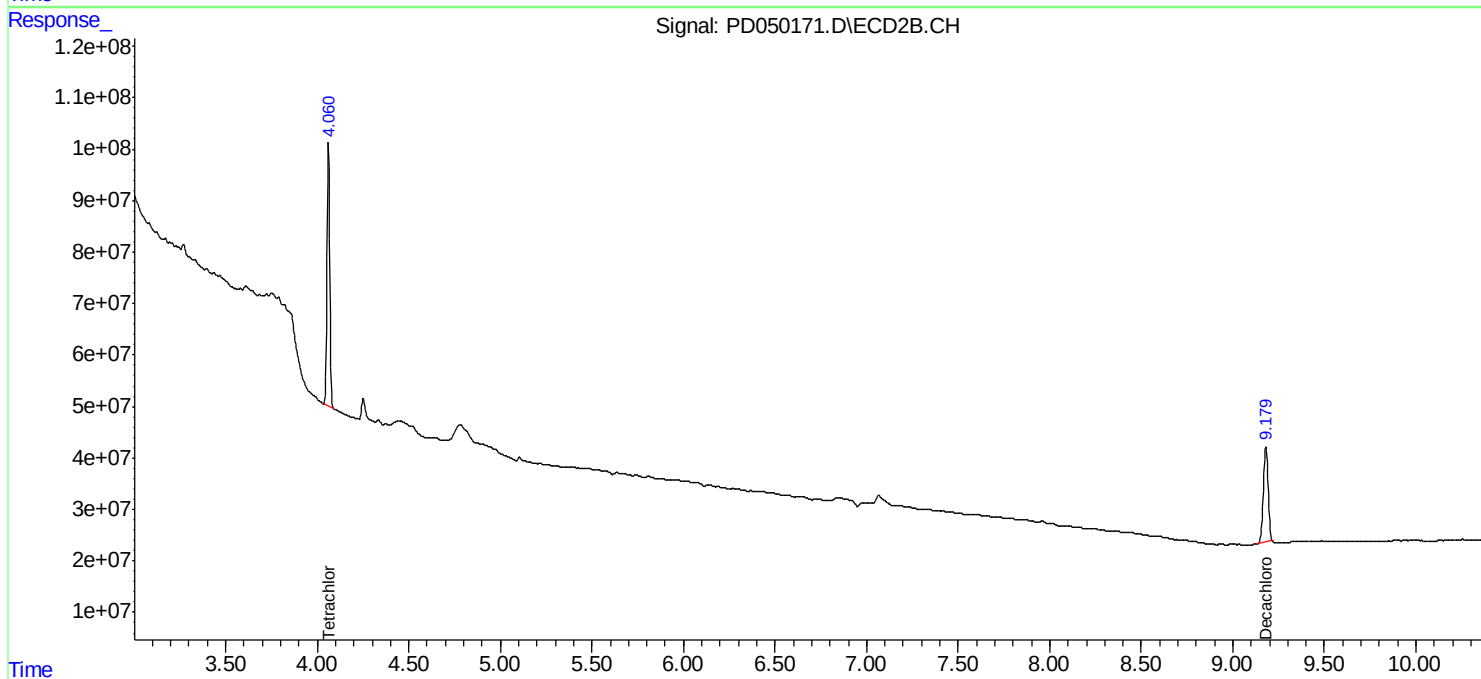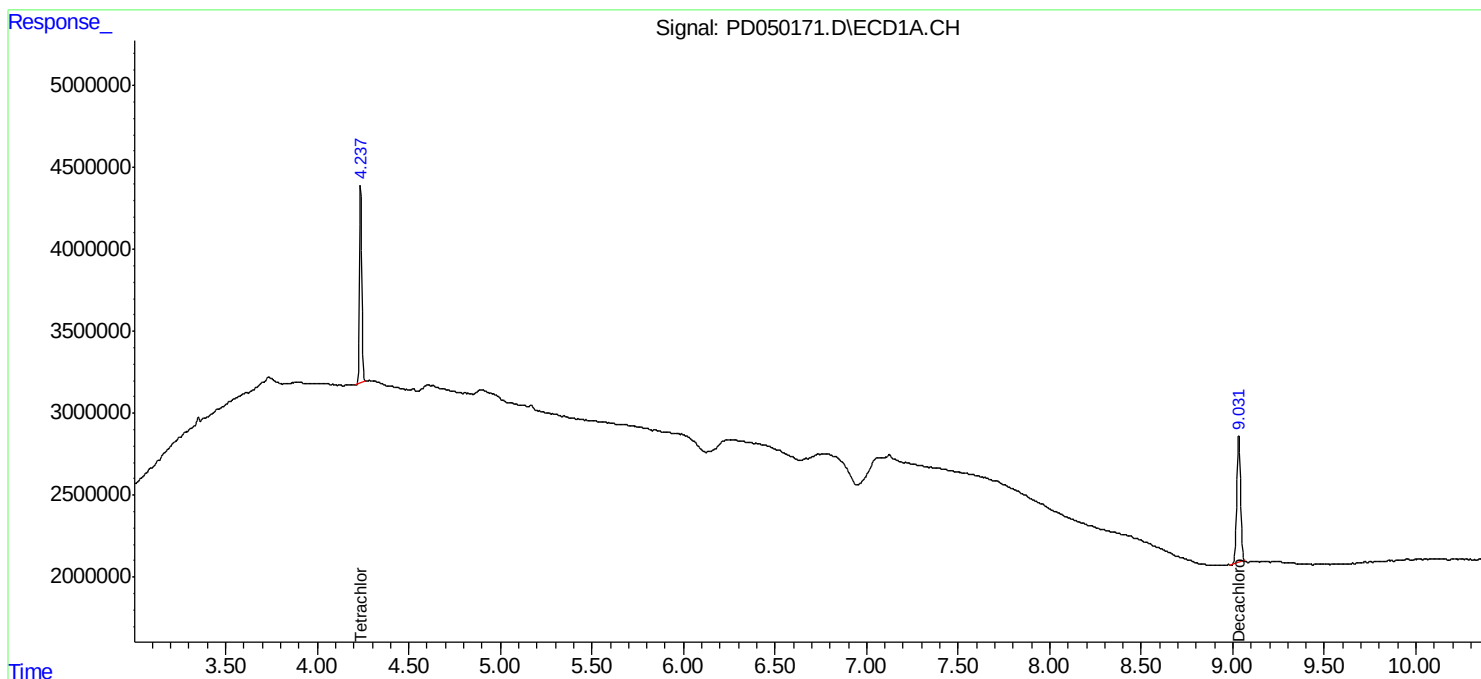

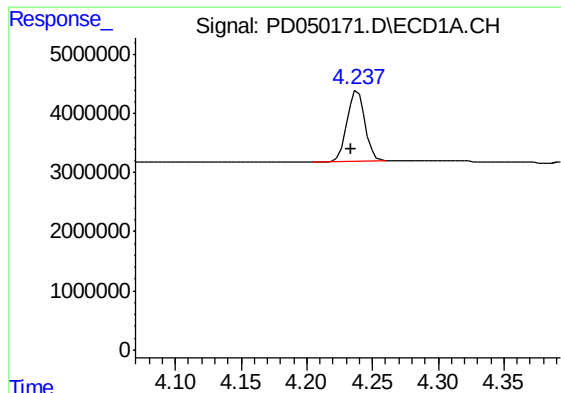


#1 Tetrachloro-m-xylene

R.T.: 4.239 min
Delta R.T.: 0.005 min
Response: 11277663
Conc: 17.40 ng/ml

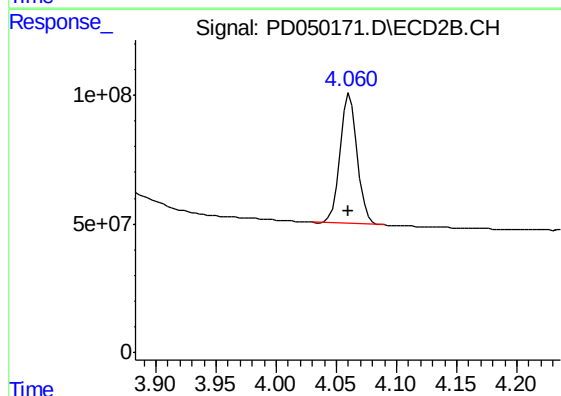


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 507930476
Conc: 18.28 ng/ml

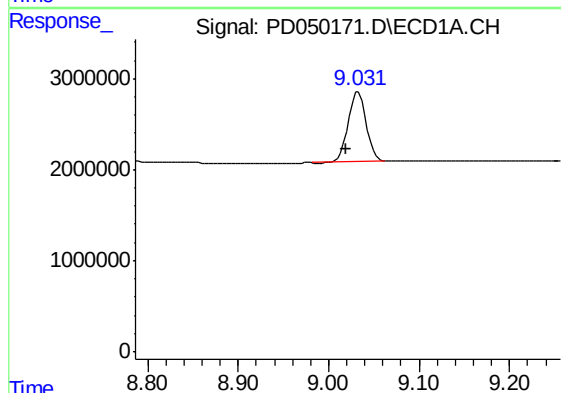

#28 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.014 min
Response: 10575706
Conc: 17.49 ng/ml

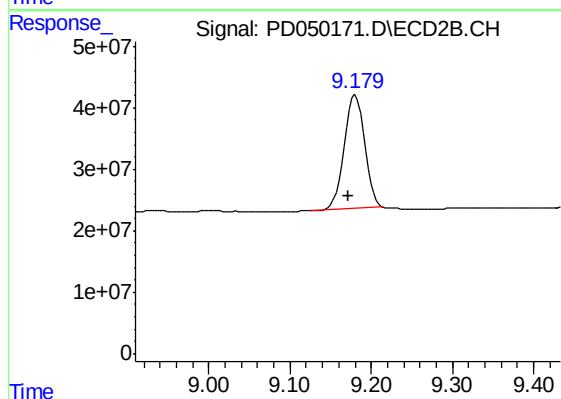

#28 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: 0.008 min
Response: 324289827
Conc: 18.74 ng/ml