

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110318\
 Data File : PD050172.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2018 14:16
 Operator : AJ\SJ
 Sample : MIREX-MDL-S-04
 Misc : FOR MIREX
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:34:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.061	11022704	520.3E6	17.008	18.721
28)	SA Decachlor...	9.021	9.173	10877291	332.5E6	17.985	19.216
Target Compounds							
22)	Mirex	8.163	8.273	429088	14886510	0.772	1.014 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110318\
Data File : PD050172.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2018 14:16
Operator : AJ\SJ
Sample : MIREX-MDL-S-04
Misc : FOR MIREX
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:34:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

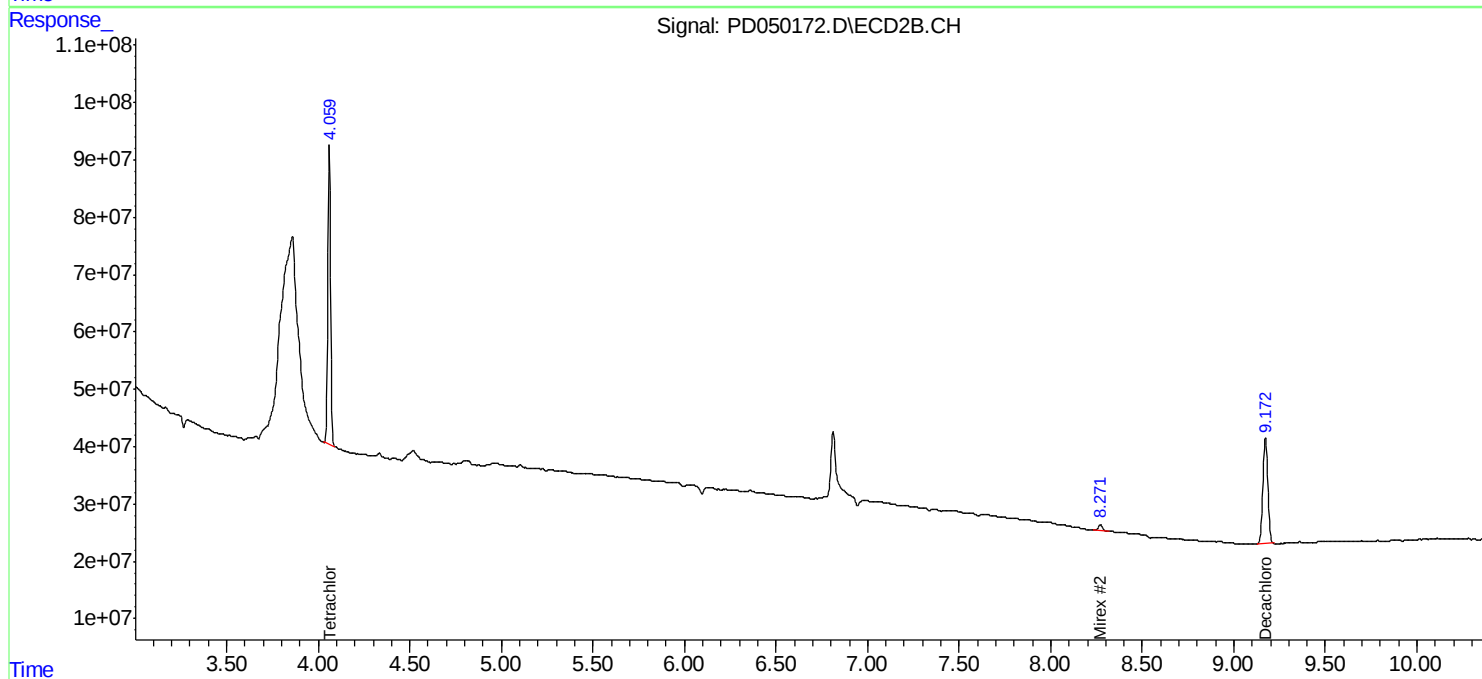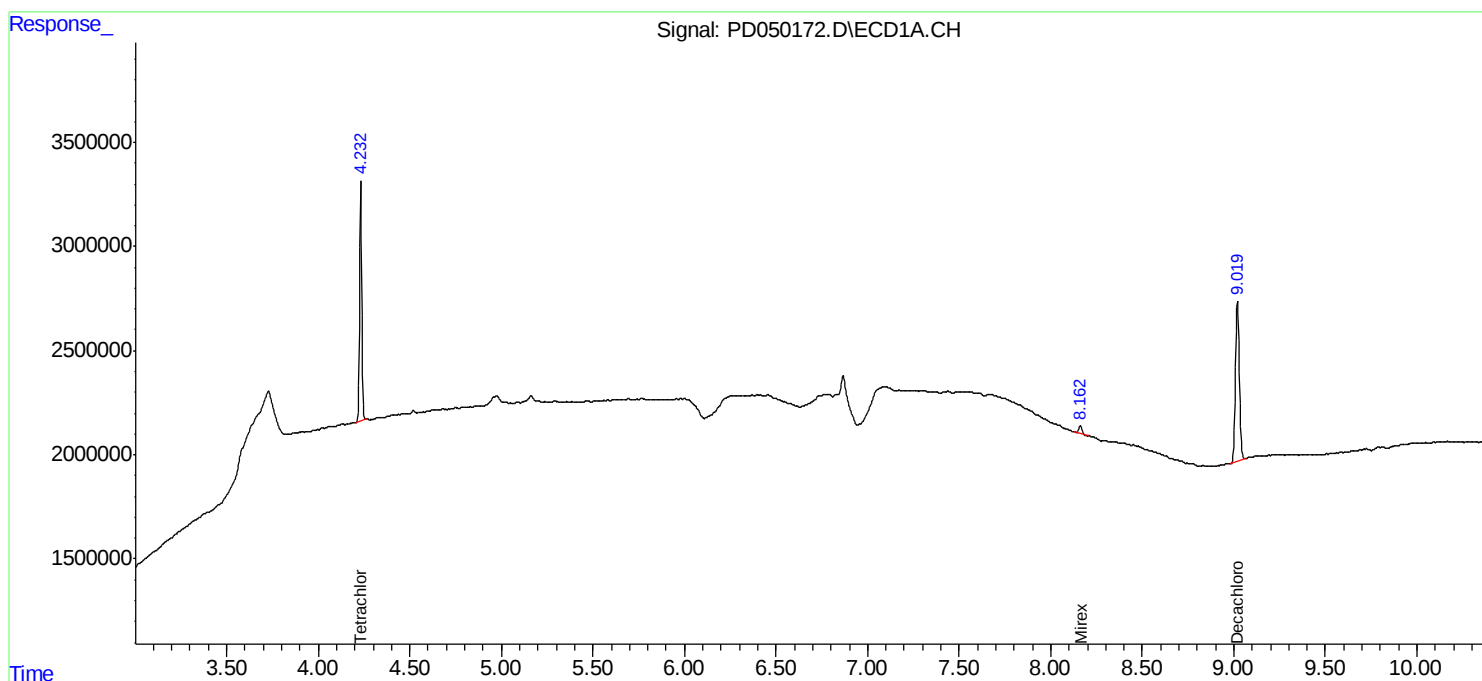

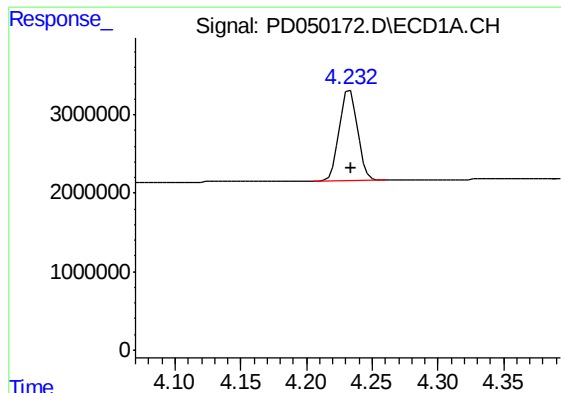


#1 Tetrachloro-m-xylene

R.T.: 4.233 min
Delta R.T.: 0.000 min
Response: 11022704
Conc: 17.01 ng/ml

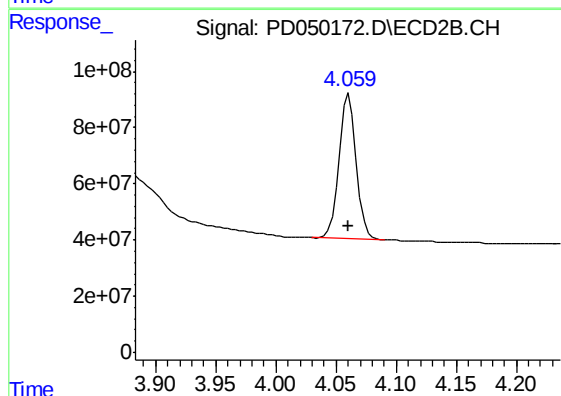


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 520283452
Conc: 18.72 ng/ml

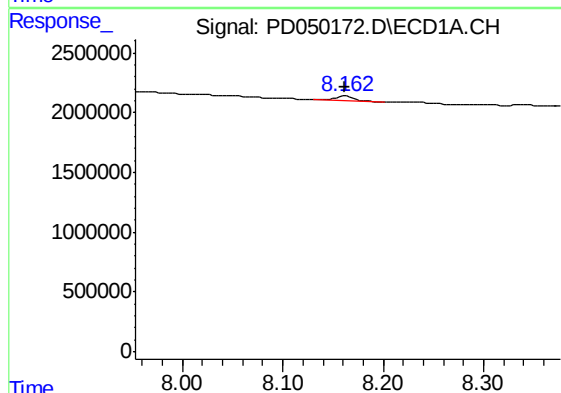


#22 Mirex

R.T.: 8.163 min
Delta R.T.: 0.001 min
Response: 429088
Conc: 0.77 ng/ml

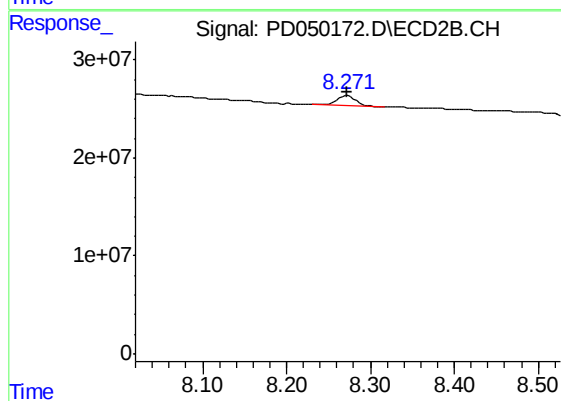


#22 Mirex

R.T.: 8.273 min
Delta R.T.: 0.000 min
Response: 14886510
Conc: 1.01 ng/ml

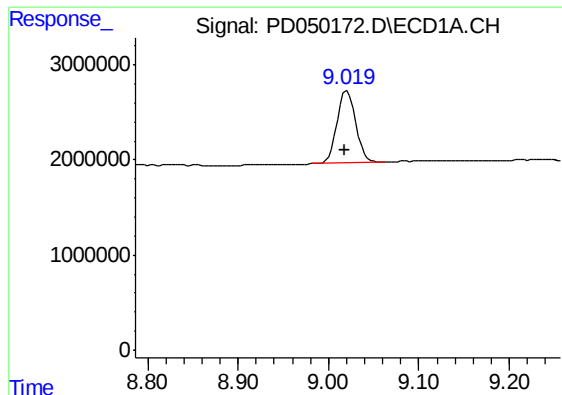

#28 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.002 min
Response: 10877291
Conc: 17.99 ng/ml

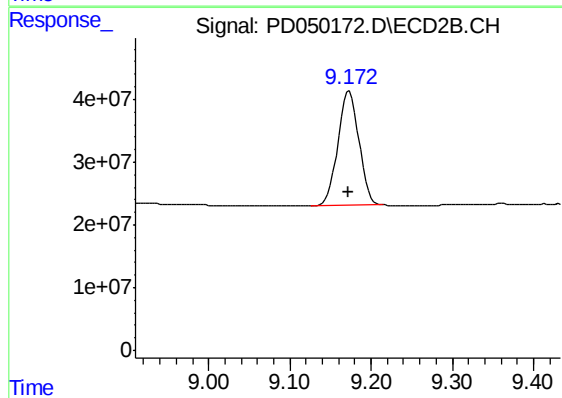

#28 Decachlorobiphenyl

R.T.: 9.173 min
Delta R.T.: 0.000 min
Response: 332537410
Conc: 19.22 ng/ml