

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110318\
 Data File : PD050174.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2018 14:44
 Operator : AJ\SJ
 Sample : MIREX-MDL-BL-W-02
 Misc : FOR MIREX
 ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:35:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.061	11262819	523.2E6	17.378	18.825
28)	SA Decachlor...	9.021	9.173	11133562	341.5E6	18.409	19.736



Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110318\
Data File : PD050174.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2018 14:44
Operator : AJ\SJ
Sample : MIREX-MDL-BL-W-02
Misc : FOR MIREX
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:35:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

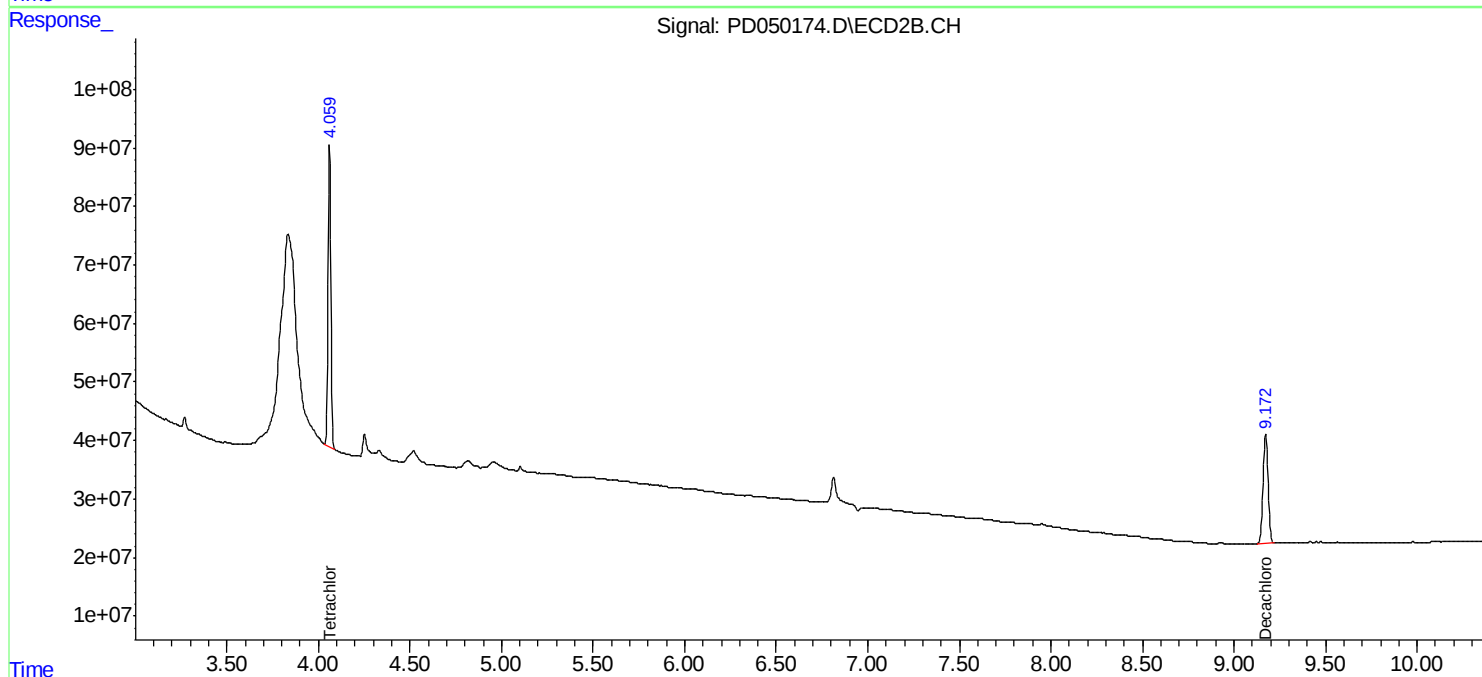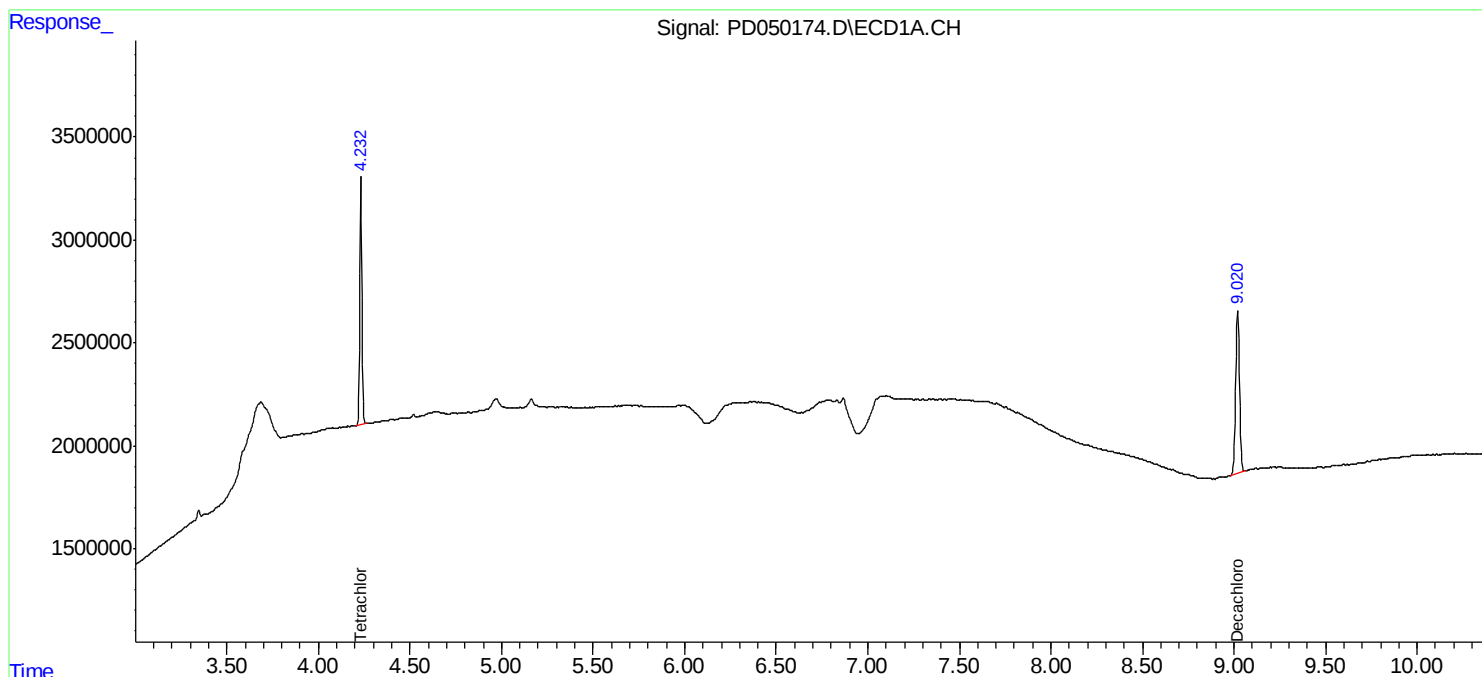

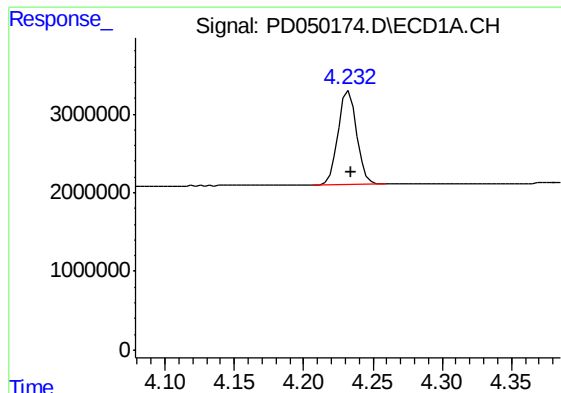


#1 Tetrachloro-m-xylene

R.T.: 4.233 min
Delta R.T.: -0.001 min
Response: 11262819
Conc: 17.38 ng/ml

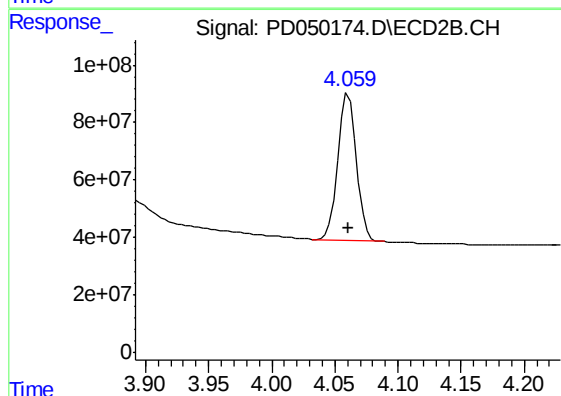


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 523173393
Conc: 18.82 ng/ml

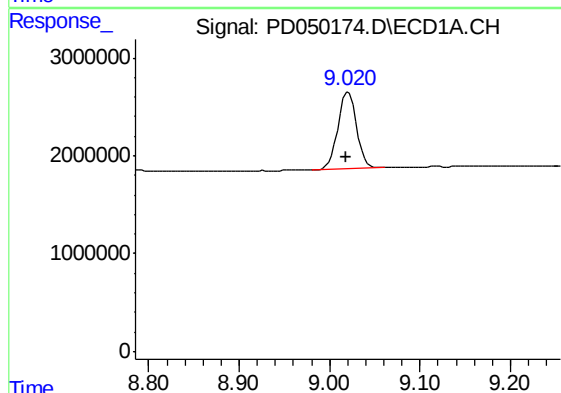

#28 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.002 min
Response: 11133562
Conc: 18.41 ng/ml

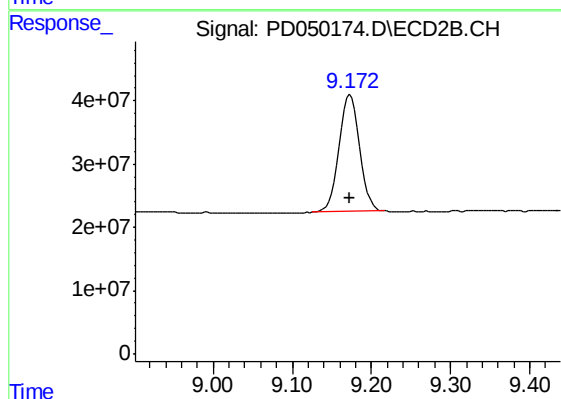

#28 Decachlorobiphenyl

R.T.: 9.173 min
Delta R.T.: 0.000 min
Response: 341538532
Conc: 19.74 ng/ml