

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110318\
 Data File : PD050175.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2018 14:58
 Operator : AJ\SJ
 Sample : MIREX-MDL-W-04
 Misc : FOR MIREX
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 01:35:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 02 05:33:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.061	11254016	518.2E6	17.365	18.645
28)	SA Decachlor...	9.019	9.173	11060839	340.1E6	18.289	19.653
Target Compounds							
22)	Mirex	8.162	8.272	364640	14565518	0.656	0.992 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110318\
Data File : PD050175.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2018 14:58
Operator : AJ\SJ
Sample : MIREX-MDL-W-04
Misc : FOR MIREX
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 01:35:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\Mirex-PD110218.M
Quant Title : GC Extractables
QLast Update : Fri Nov 02 05:33:40 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

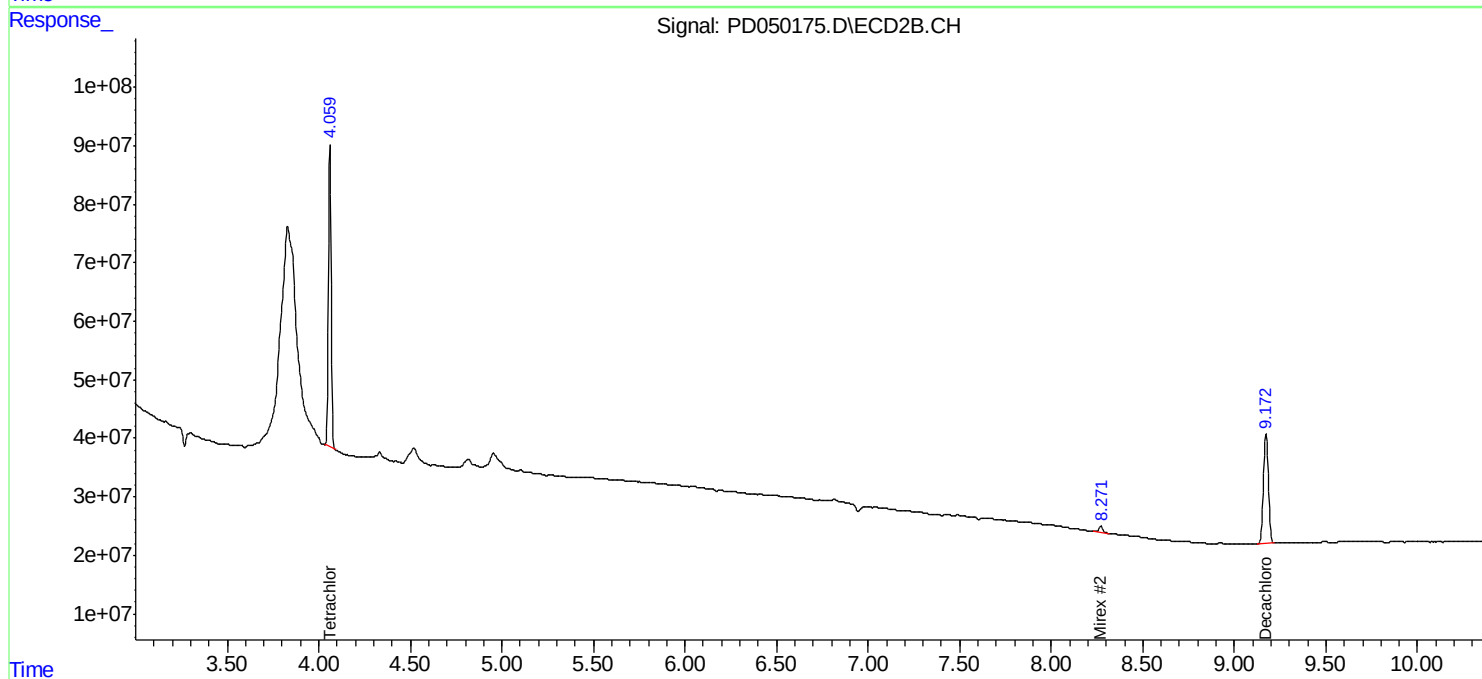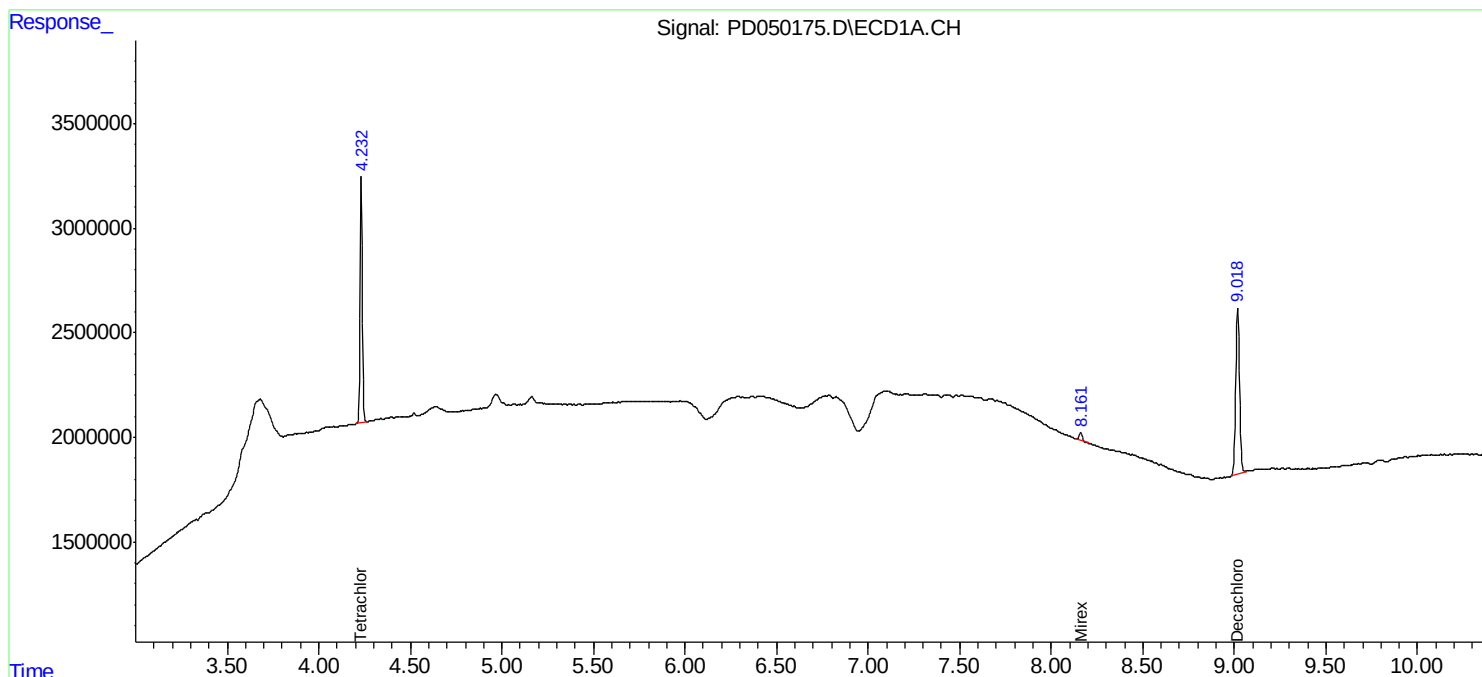

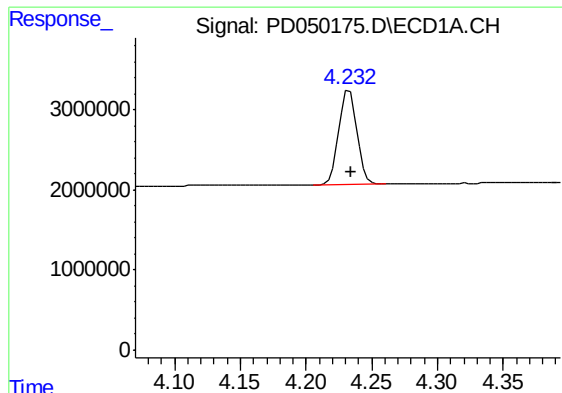


#1 Tetrachloro-m-xylene

R.T.: 4.233 min
Delta R.T.: -0.001 min
Response: 11254016
Conc: 17.36 ng/ml

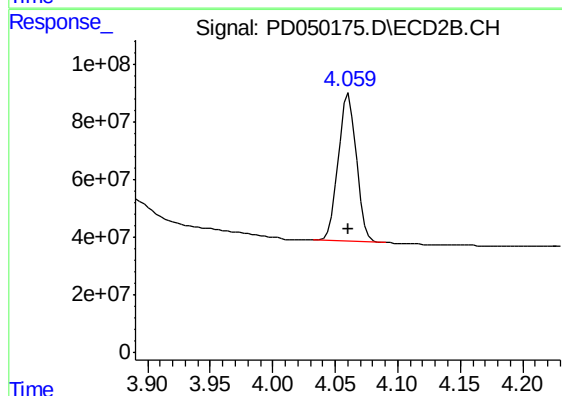


#1 Tetrachloro-m-xylene

R.T.: 4.061 min
Delta R.T.: 0.000 min
Response: 518185842
Conc: 18.65 ng/ml

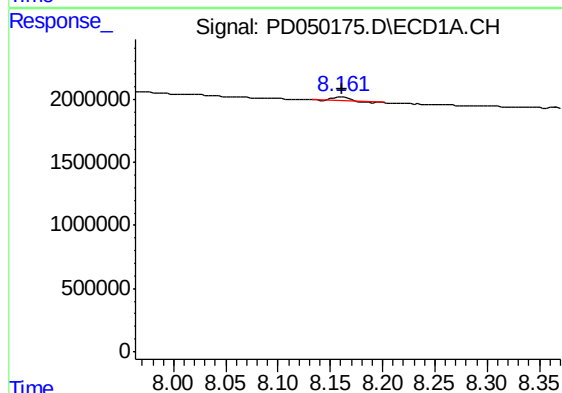


#22 Mirex

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 364640
Conc: 0.66 ng/ml

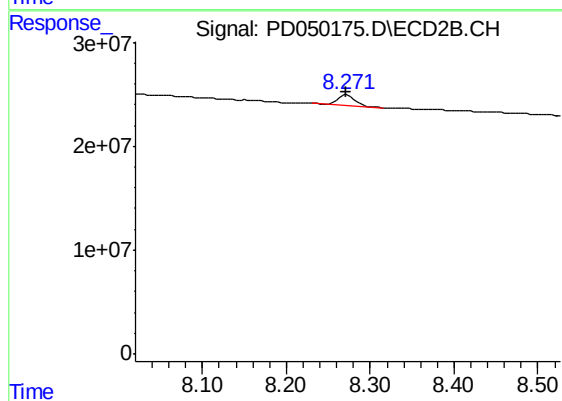


#22 Mirex

R.T.: 8.272 min
Delta R.T.: 0.000 min
Response: 14565518
Conc: 0.99 ng/ml

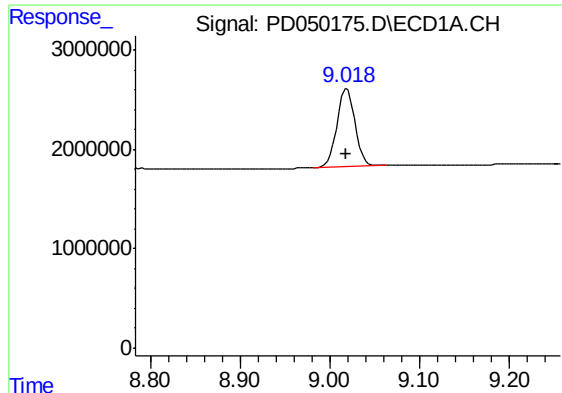

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 11060839
Conc: 18.29 ng/ml

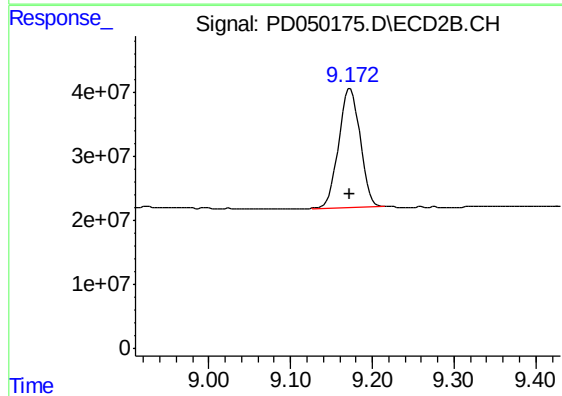

#28 Decachlorobiphenyl

R.T.: 9.173 min
Delta R.T.: 0.000 min
Response: 340091473
Conc: 19.65 ng/ml