

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110319\
 Data File : PD055814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 19:35
 Operator : SG\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3003

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 07:10:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:09:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.962	15084606	21002594	20.000	20.000
27)	SA Decachlor...	7.964	8.997	33325018	46371474	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.716	4.349	21044761	28620655	20.000	20.000
3)	MA gamma-BHC...	3.991	4.631	20382889	28277365	20.000	20.000
4)	MA Heptachlor	4.277	5.137	19055753	29365629	20.000	20.000
9)	A Endosulfan I	5.283	6.179	17147527	26470584	20.000	20.000
13)	MA Dieldrin	5.523	6.435	38331912	57726593	40.000	40.000
14)	MA Endrin	5.776	6.652	32693081	46984036	40.000	40.000
16)	A 4,4'-DDD	5.910	6.774	28875214	45844599	40.000	40.000
17)	MA 4,4'-DDT	6.146	7.072	27027299	44749438	40.000	40.000
20)	A Methoxychlor	6.695	7.529	77778603	128.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110319\
Data File : PD055814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 19:35
Operator : SG\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA3003

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 07:10:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:09:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

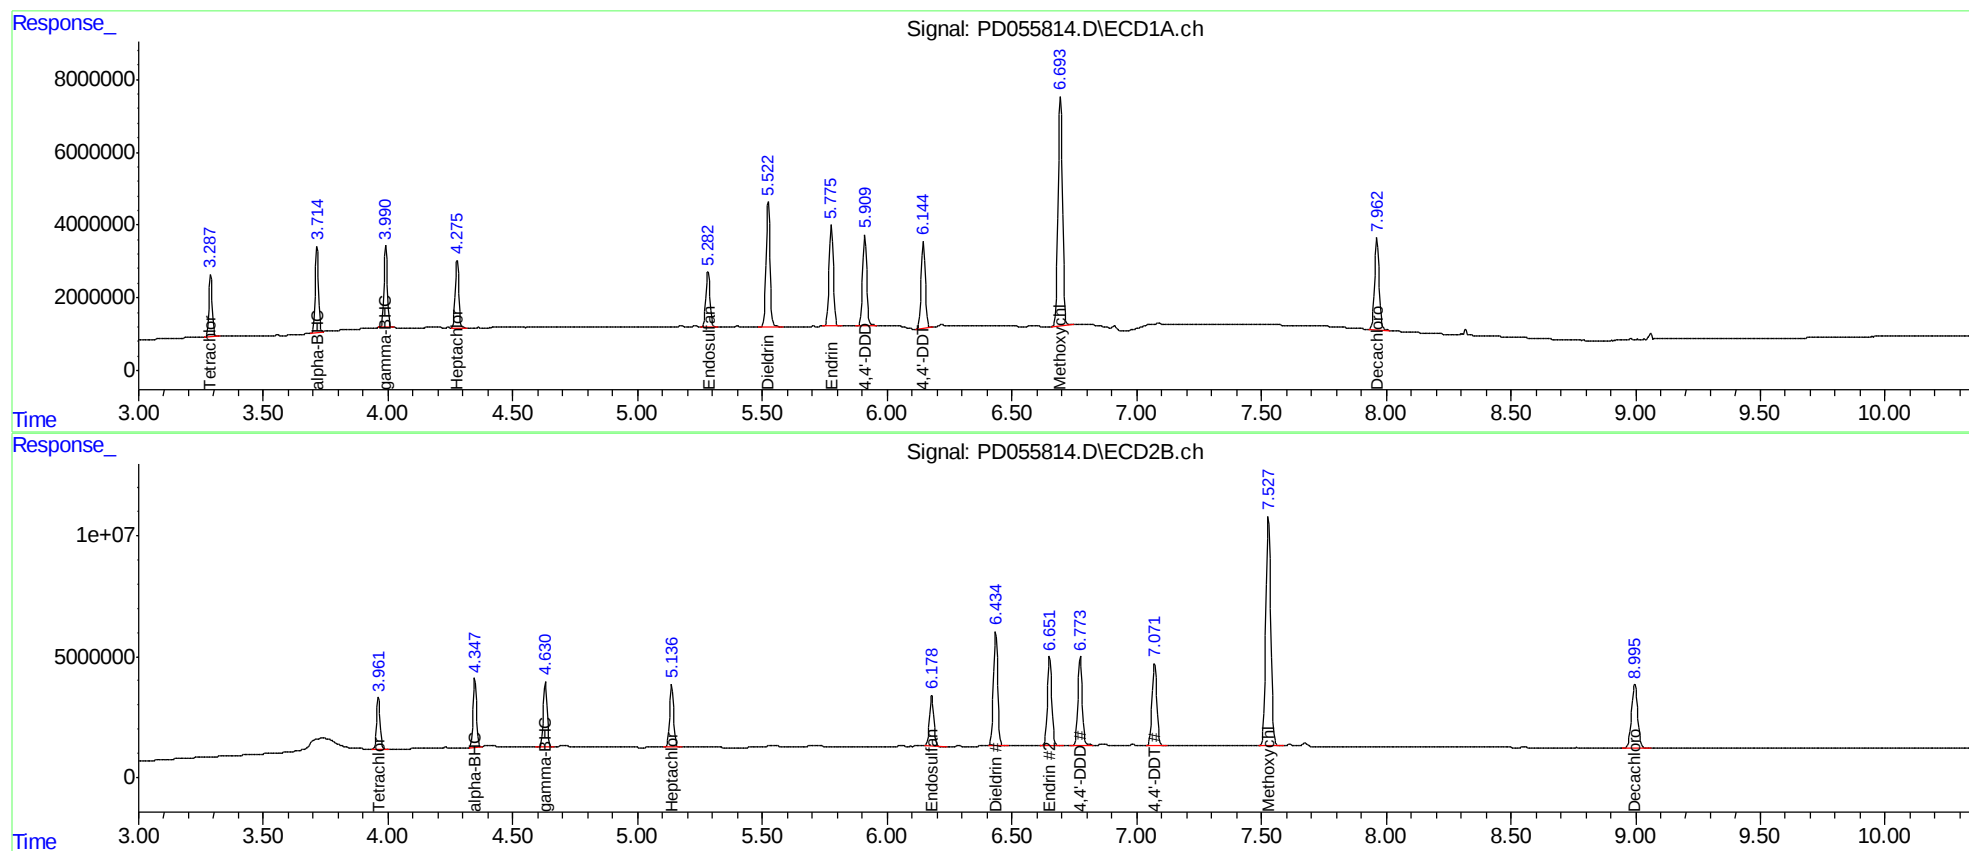


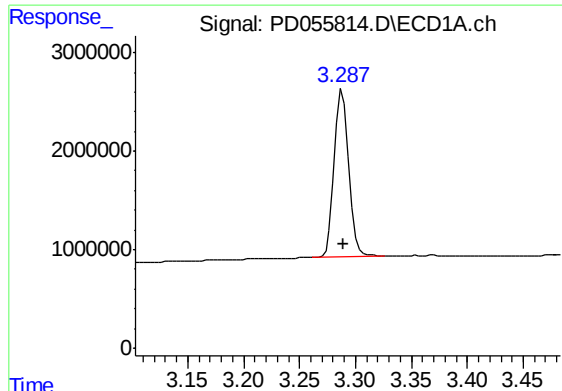

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 15084606
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3003

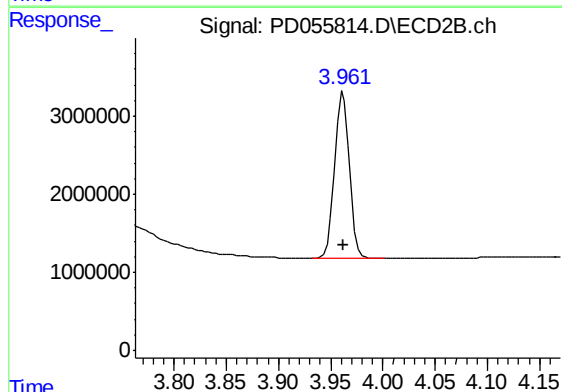


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 21002594
Conc: 20.00 ng/ml

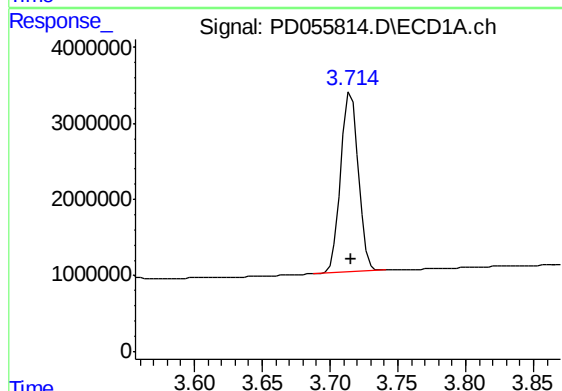


#2 alpha-BHC

R.T.: 3.716 min
Delta R.T.: 0.000 min
Response: 21044761
Conc: 20.00 ng/ml

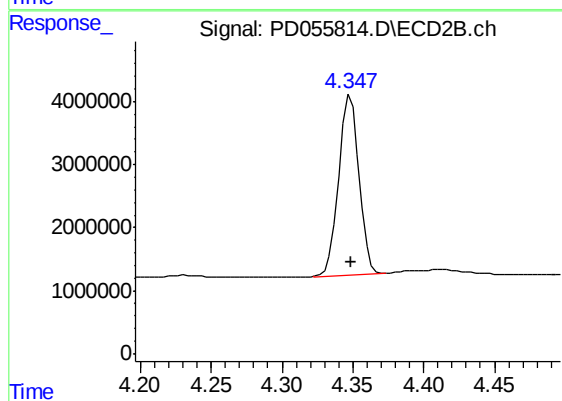

#2 alpha-BHC


R.T.: 4.349 min
Delta R.T.: 0.000 min
Response: 28620655
Conc: 20.00 ng/ml

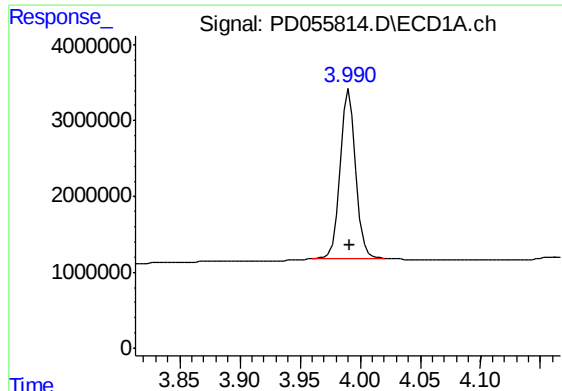

#3 gamma-BHC (Lindane)


R.T.: 3.991 min
Delta R.T.: 0.000 min
Response: 20382889
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3003

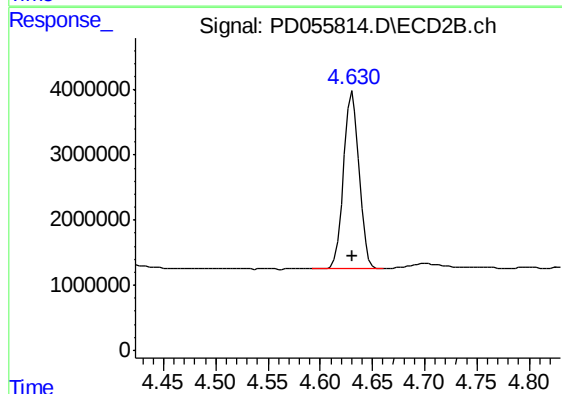


#3 gamma-BHC (Lindane)

R.T.: 4.631 min
Delta R.T.: 0.000 min
Response: 28277365
Conc: 20.00 ng/ml

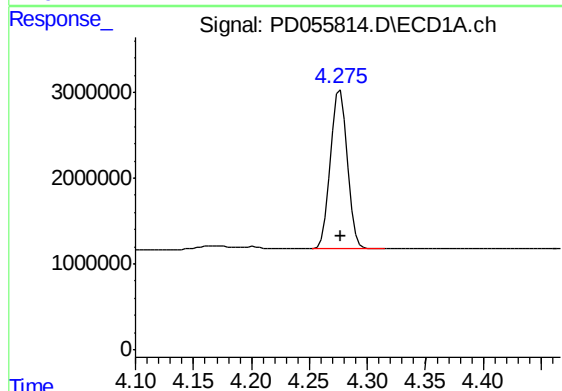


#4 Heptachlor

R.T.: 4.277 min
Delta R.T.: 0.000 min
Response: 19055753
Conc: 20.00 ng/ml

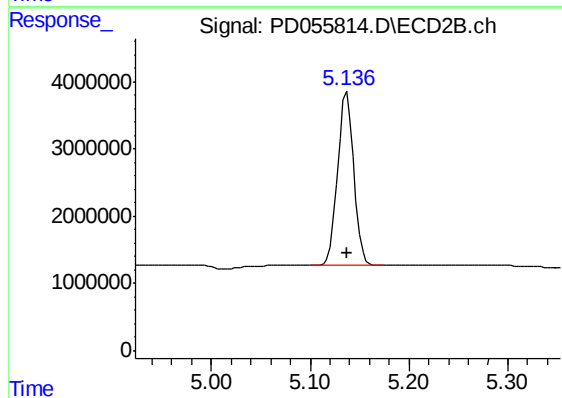

#4 Heptachlor


R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 29365629
Conc: 20.00 ng/ml

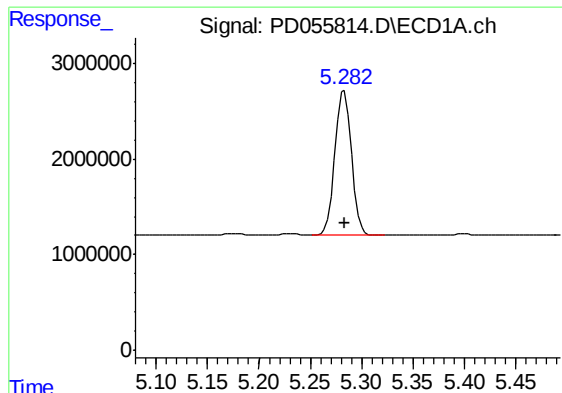

#9 Endosulfan I


R.T.: 5.283 min
Delta R.T.: 0.000 min
Response: 17147527
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3003

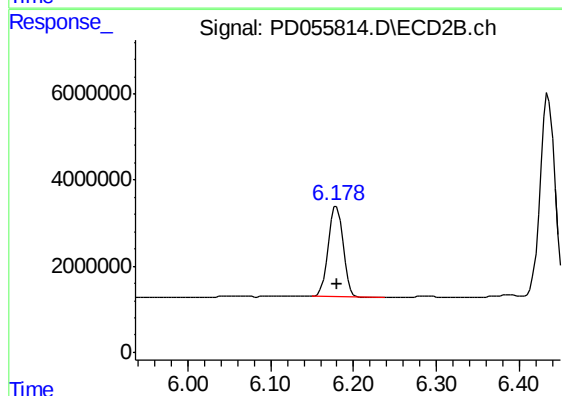


#9 Endosulfan I

R.T.: 6.179 min
Delta R.T.: 0.000 min
Response: 26470584
Conc: 20.00 ng/ml

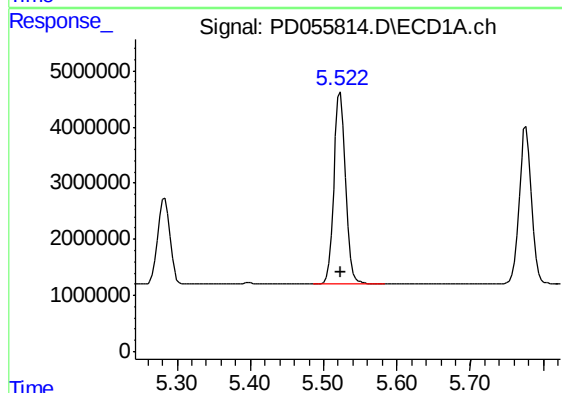


#13 Dieldrin

R.T.: 5.523 min
Delta R.T.: 0.000 min
Response: 38331912
Conc: 40.00 ng/ml

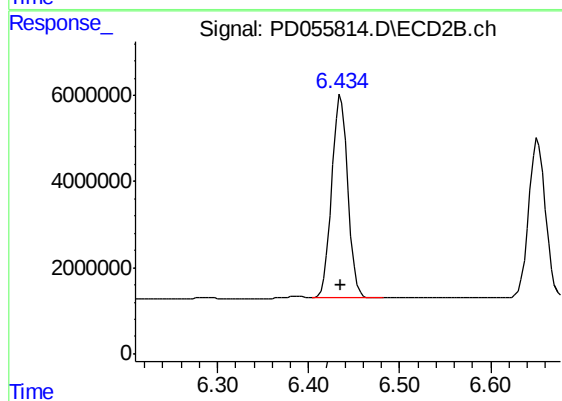

#13 Dieldrin


R.T.: 6.435 min
Delta R.T.: 0.000 min
Response: 57726593
Conc: 40.00 ng/ml

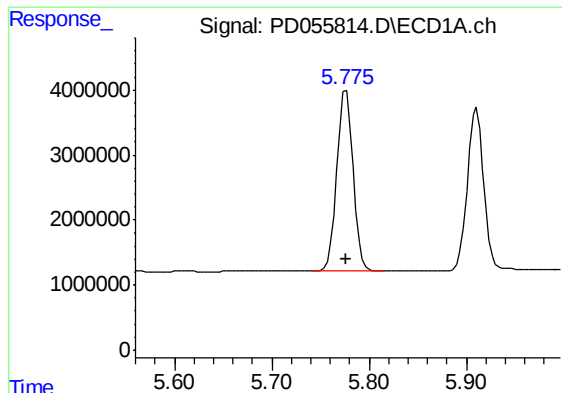

#14 Endrin


R.T.: 5.776 min
Delta R.T.: 0.000 min
Response: 32693081
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3003

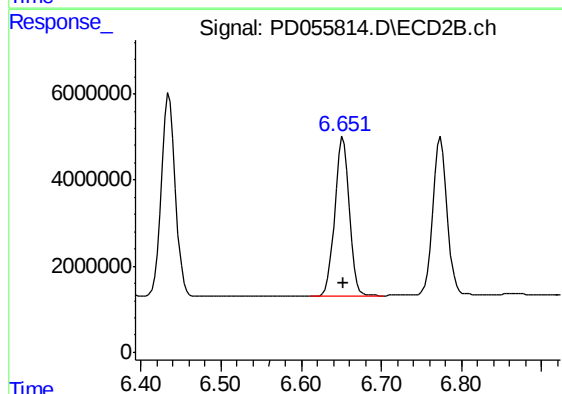


#14 Endrin

R.T.: 6.652 min
Delta R.T.: 0.000 min
Response: 46984036
Conc: 40.00 ng/ml

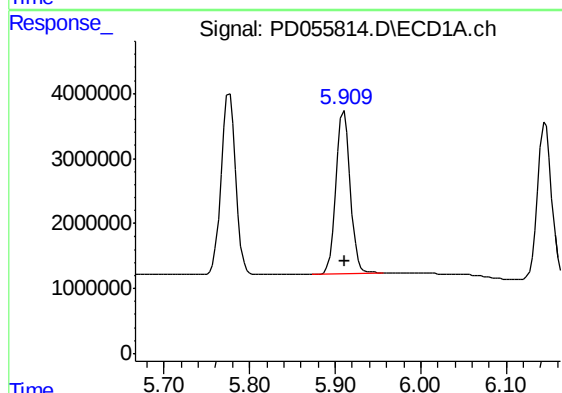


#16 4,4'-DDD

R.T.: 5.910 min
Delta R.T.: 0.000 min
Response: 28875214
Conc: 40.00 ng/ml

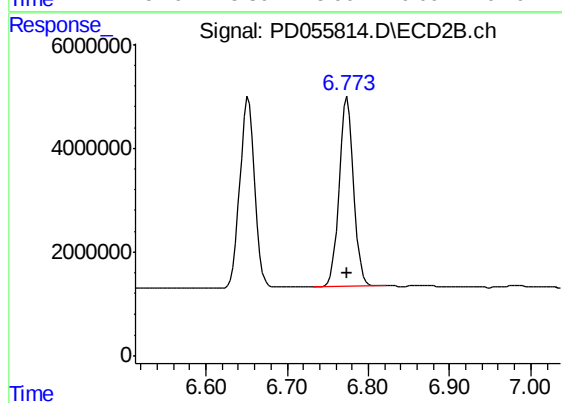

#16 4,4'-DDD


R.T.: 6.774 min
Delta R.T.: 0.000 min
Response: 45844599
Conc: 40.00 ng/ml

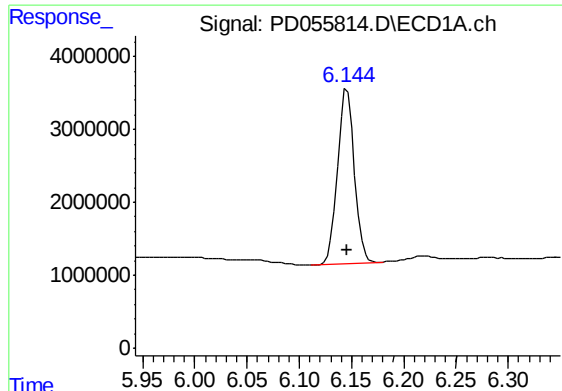

#17 4,4'-DDT


R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 27027299
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3003

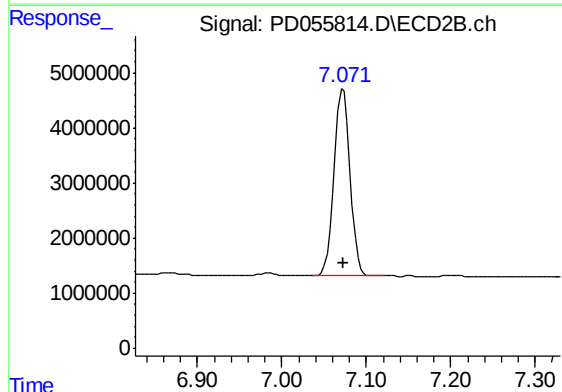


#17 4,4'-DDT

R.T.: 7.072 min
Delta R.T.: 0.000 min
Response: 44749438
Conc: 40.00 ng/ml

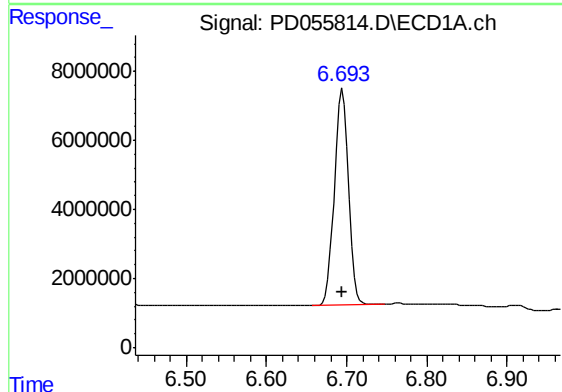


#20 Methoxychlor

R.T.: 6.695 min
Delta R.T.: 0.000 min
Response: 77778603
Conc: 200.00 ng/ml

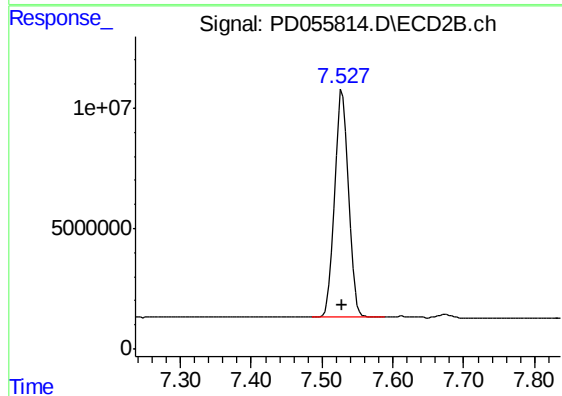

#20 Methoxychlor


R.T.: 7.529 min
Delta R.T.: 0.000 min
Response: 128749050
Conc: 200.00 ng/ml

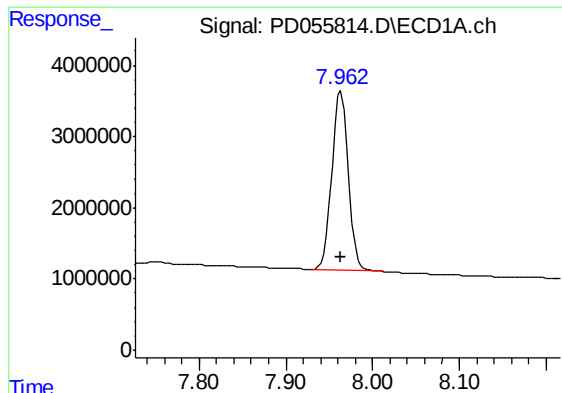

#27 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 33325018
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3003

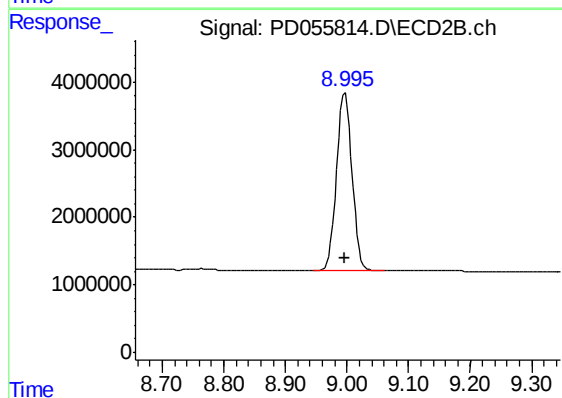

#27 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 46371474
Conc: 40.00 ng/ml