

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110319\
 Data File : PD055816.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 20:03
 Operator : SG\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4003

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 07:10:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:09:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.962	29394726	40641033	38.973	38.701
27)	SA Decachlor...	7.963	8.997	61990331	84431051	74.407	72.830
Target Compounds							
2)	A alpha-BHC	3.716	4.349	43086197	58467926	40.947	40.857
3)	MA gamma-BHC...	3.991	4.631	40469825	56683107	39.710	40.091
4)	MA Heptachlor	4.276	5.137	37726638	57198548	39.596	38.956
9)	A Endosulfan I	5.283	6.180	33231069	50986996	38.759	38.524
13)	MA Dieldrin	5.523	6.436	76175739	113.3E6	79.491	78.518
14)	MA Endrin	5.776	6.653	64476576	92127706	78.887	78.433
16)	A 4,4'-DDD	5.910	6.775	57324123	89995952	79.409	78.523
17)	MA 4,4'-DDT	6.146	7.073	55921222	90058559	82.763	80.500
20)	A Methoxychlor	6.694	7.529	147.8E6	242.1E6	380.130	376.101


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110319\
Data File : PD055816.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 20:03
Operator : SG\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA4003

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 07:10:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:09:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

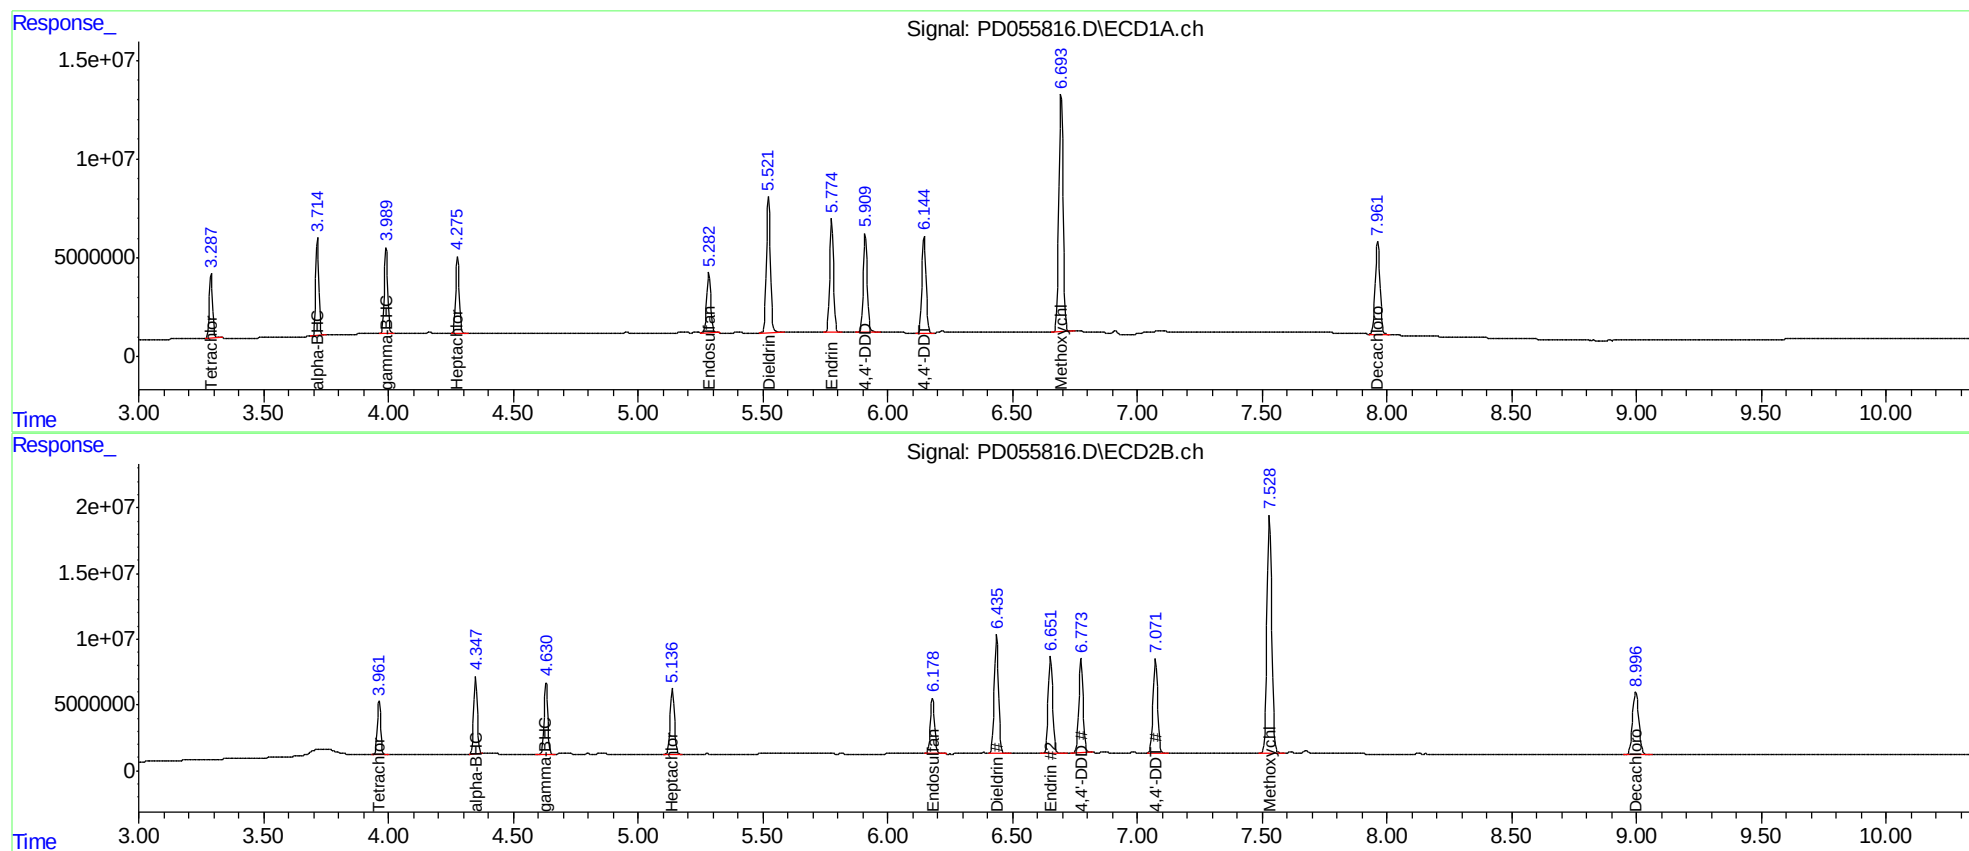


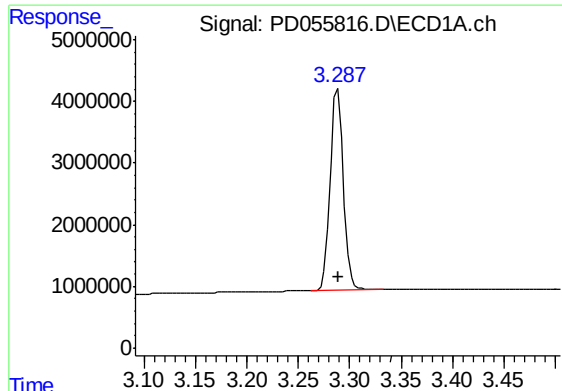

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 29394726
Conc: 38.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4003

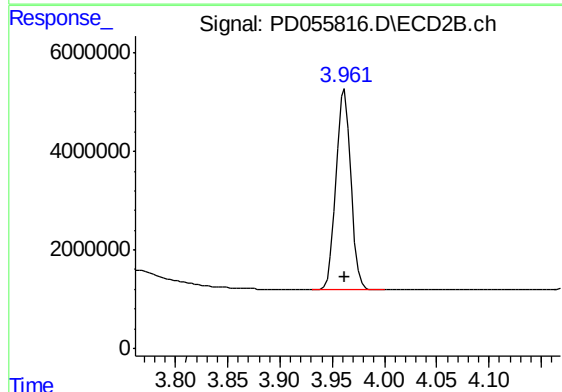


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 40641033
Conc: 38.70 ng/ml

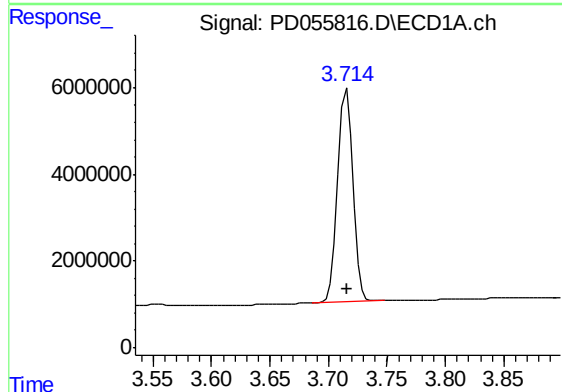


#2 alpha-BHC

R.T.: 3.716 min
Delta R.T.: 0.000 min
Response: 43086197
Conc: 40.95 ng/ml

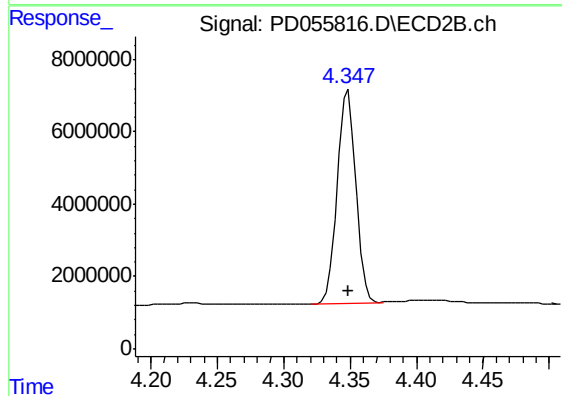

#2 alpha-BHC


R.T.: 4.349 min
Delta R.T.: 0.000 min
Response: 58467926
Conc: 40.86 ng/ml

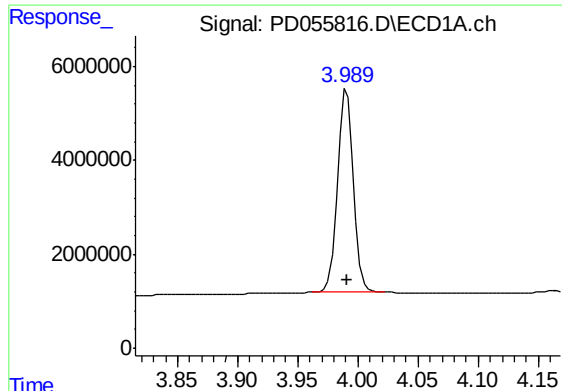

#3 gamma-BHC (Lindane)


R.T.: 3.991 min
Delta R.T.: 0.000 min
Response: 40469825
Conc: 39.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4003

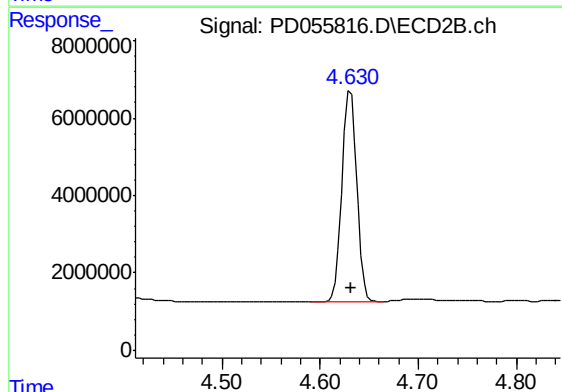


#3 gamma-BHC (Lindane)

R.T.: 4.631 min
Delta R.T.: 0.000 min
Response: 56683107
Conc: 40.09 ng/ml

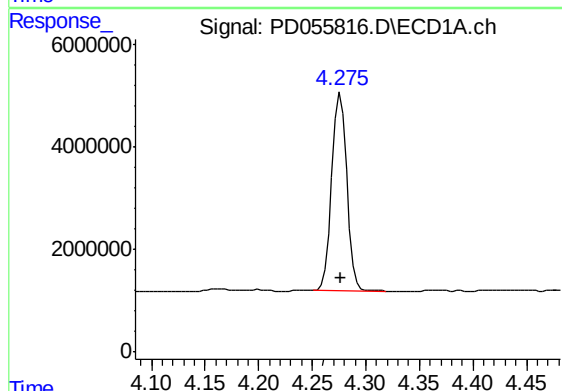


#4 Heptachlor

R.T.: 4.276 min
Delta R.T.: 0.000 min
Response: 37726638
Conc: 39.60 ng/ml

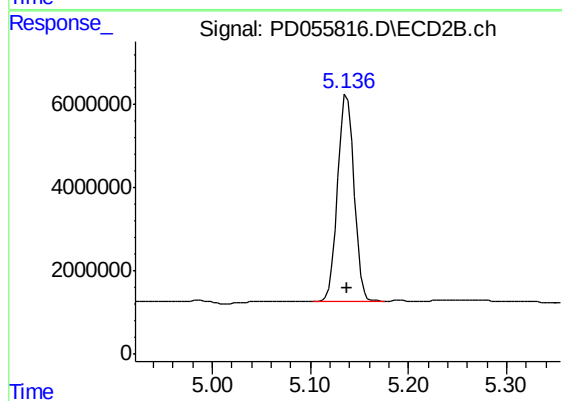

#4 Heptachlor


R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 57198548
Conc: 38.96 ng/ml

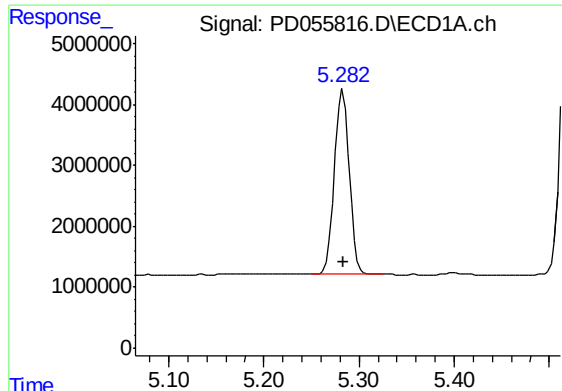

#9 Endosulfan I


R.T.: 5.283 min
Delta R.T.: 0.000 min
Response: 33231069
Conc: 38.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4003

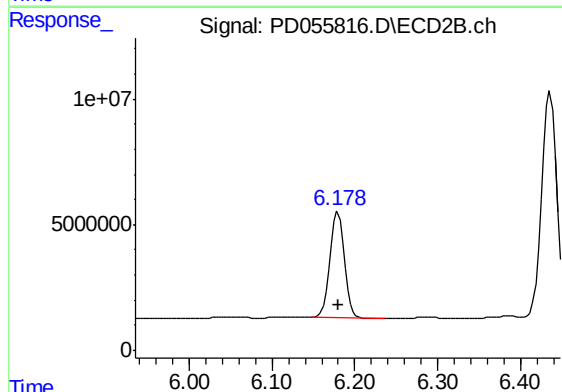


#9 Endosulfan I

R.T.: 6.180 min
Delta R.T.: 0.000 min
Response: 50986996
Conc: 38.52 ng/ml

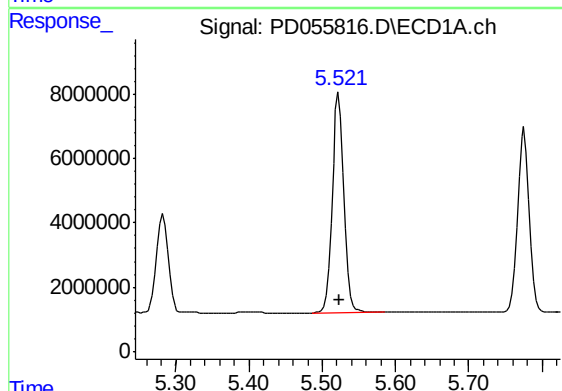


#13 Dieldrin

R.T.: 5.523 min
Delta R.T.: 0.000 min
Response: 76175739
Conc: 79.49 ng/ml

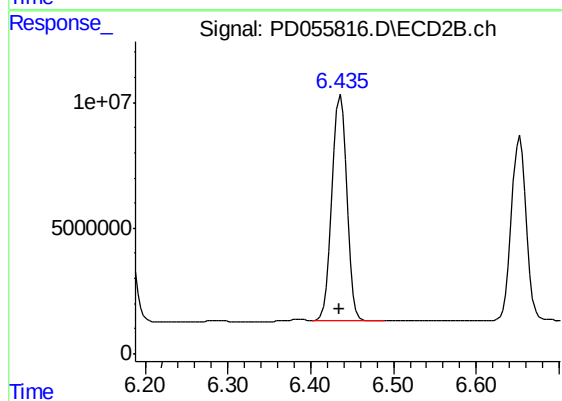

#13 Dieldrin


R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 113313763
Conc: 78.52 ng/ml

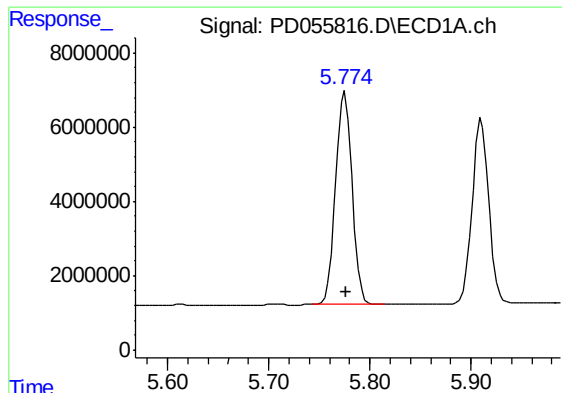

#14 Endrin


R.T.: 5.776 min
Delta R.T.: 0.000 min
Response: 64476576
Conc: 78.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4003

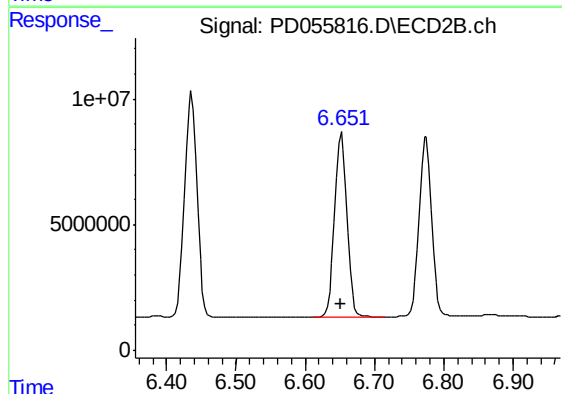


#14 Endrin

R.T.: 6.653 min
Delta R.T.: 0.000 min
Response: 92127706
Conc: 78.43 ng/ml

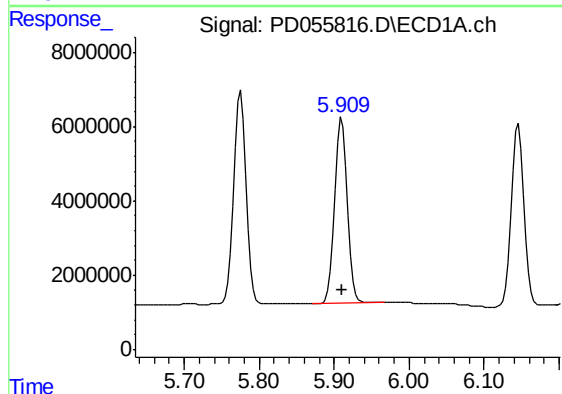


#16 4,4'-DDD

R.T.: 5.910 min
Delta R.T.: 0.000 min
Response: 57324123
Conc: 79.41 ng/ml

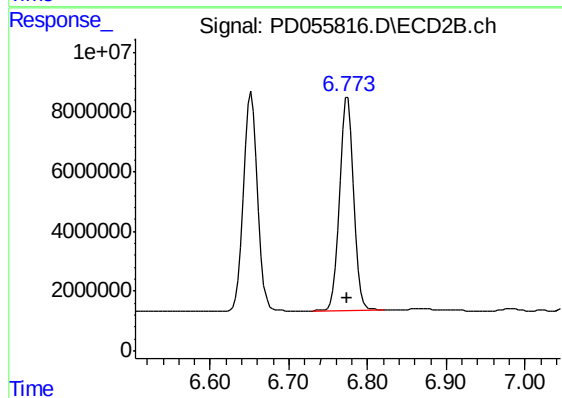

#16 4,4'-DDD


R.T.: 6.775 min
Delta R.T.: 0.000 min
Response: 89995952
Conc: 78.52 ng/ml

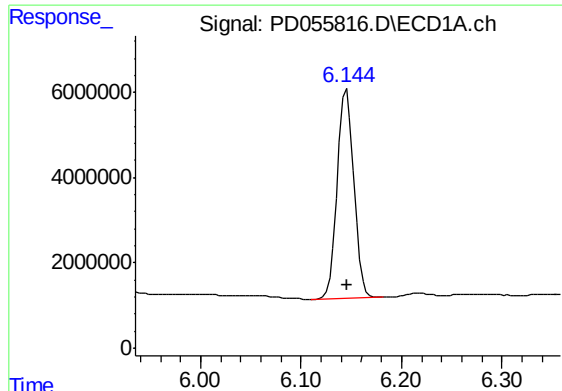

#17 4,4'-DDT


R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 55921222
Conc: 82.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4003

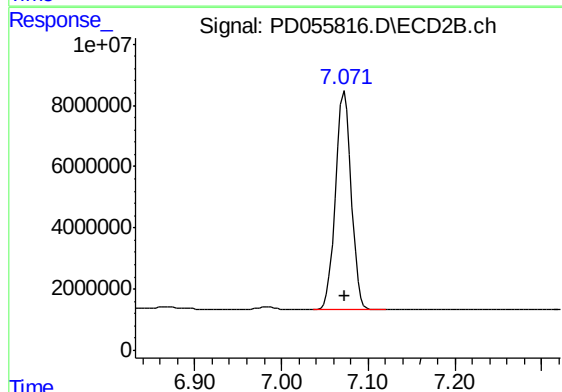


#17 4,4'-DDT

R.T.: 7.073 min
Delta R.T.: 0.000 min
Response: 90058559
Conc: 80.50 ng/ml

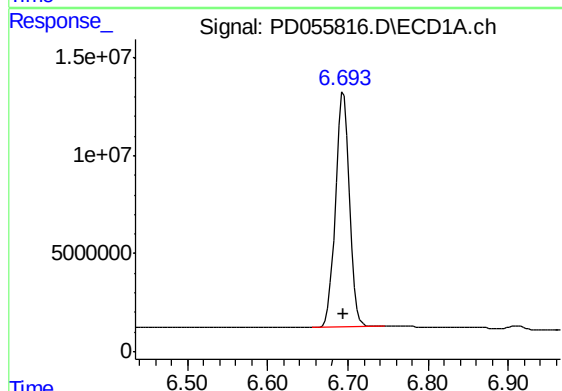


#20 Methoxychlor

R.T.: 6.694 min
Delta R.T.: 0.000 min
Response: 147830016
Conc: 380.13 ng/ml

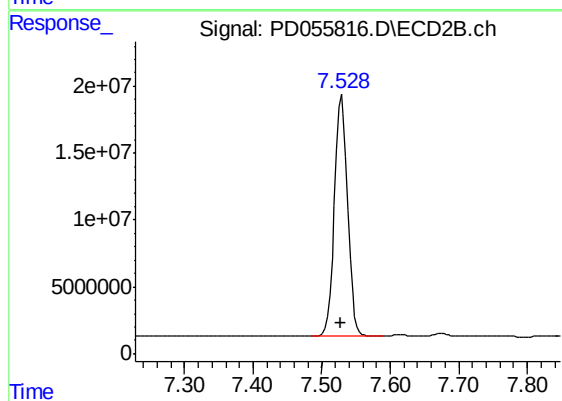

#20 Methoxychlor


R.T.: 7.529 min
Delta R.T.: 0.000 min
Response: 242113424
Conc: 376.10 ng/ml

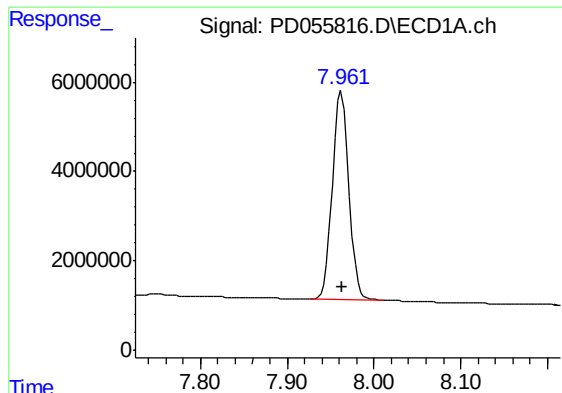

#27 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: -0.001 min
Response: 61990331
Conc: 74.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4003

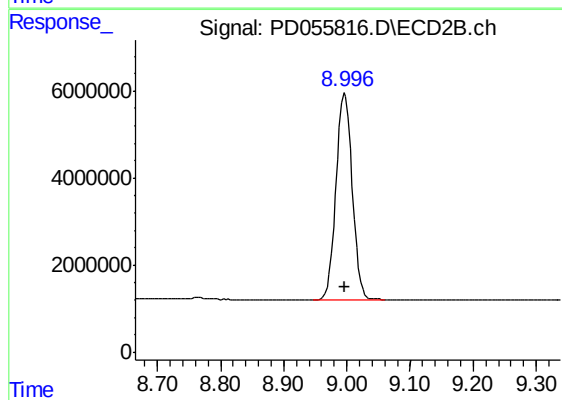

#27 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: 0.000 min
Response: 84431051
Conc: 72.83 ng/ml