

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110319\
 Data File : PD055803.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 17:01
 Operator : SG\AJ
 Sample : RESC10
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC010

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 07:26:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.962	14732480	20543882	19.571	19.604
27)	SA Decachlor...	7.964	8.998	33060282	46081477	40.559	40.580
Target Compounds							
2)	A alpha-BHC	3.716	4.348	9871610	13288725	9.375	9.325
3)	MA gamma-BHC...	3.991	4.631	9821152	13413812	9.602	9.521
4)	MA Heptachlor	4.277	5.138	9339462	14207766	9.864	9.769
5)	MB Aldrin	4.516	5.441	9125187	13558565	9.849	9.882
6)	B beta-BHC	4.241	4.800	4678271	7209624	10.343	10.305
7)	B delta-BHC	4.436	5.016	9835895	10584200	9.637	8.029
8)	B Heptachlo...	4.953	5.825	8999186	12775286	10.079	9.466
9)	A Endosulfan I	5.284	6.180	8494805	12917202	10.137	9.921
10)	B trans-Chl...	5.175	6.059	9126686	14362934	10.065	10.069
11)	B cis-Chlor...	5.232	6.131	8921220	13990755	10.075	9.969
12)	B 4,4'-DDE	5.400	6.287	17153464	26460563	19.730	19.637
13)	MA Dieldrin	5.523	6.436	18212902	27573242	19.363	19.506
14)	MA Endrin	5.777	6.653	15848893	22777018	19.756	19.784
15)	B Endosulfa...	6.050	6.861	17092112	25899457	20.285	20.000
16)	A 4,4'-DDD	5.911	6.775	13908028	21852641	19.692	19.570
17)	MA 4,4'-DDT	6.147	7.073	12122172	21198172	18.706	19.495
18)	B Endrin al...	6.219	6.985	15046394	22440809	21.062	20.667
19)	B Endosulfa...	6.429	7.207	16048029	24773291	20.453	20.548
20)	A Methoxychlor	6.695	7.530	38158108	64414485	102.012	103.346
21)	B Endrin ke...	6.914	7.675	18952653	27891465	21.398	21.146

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110319\
Data File : PD055803.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 17:01
Operator : SG\AJ
Sample : RESC10
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 07:26:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

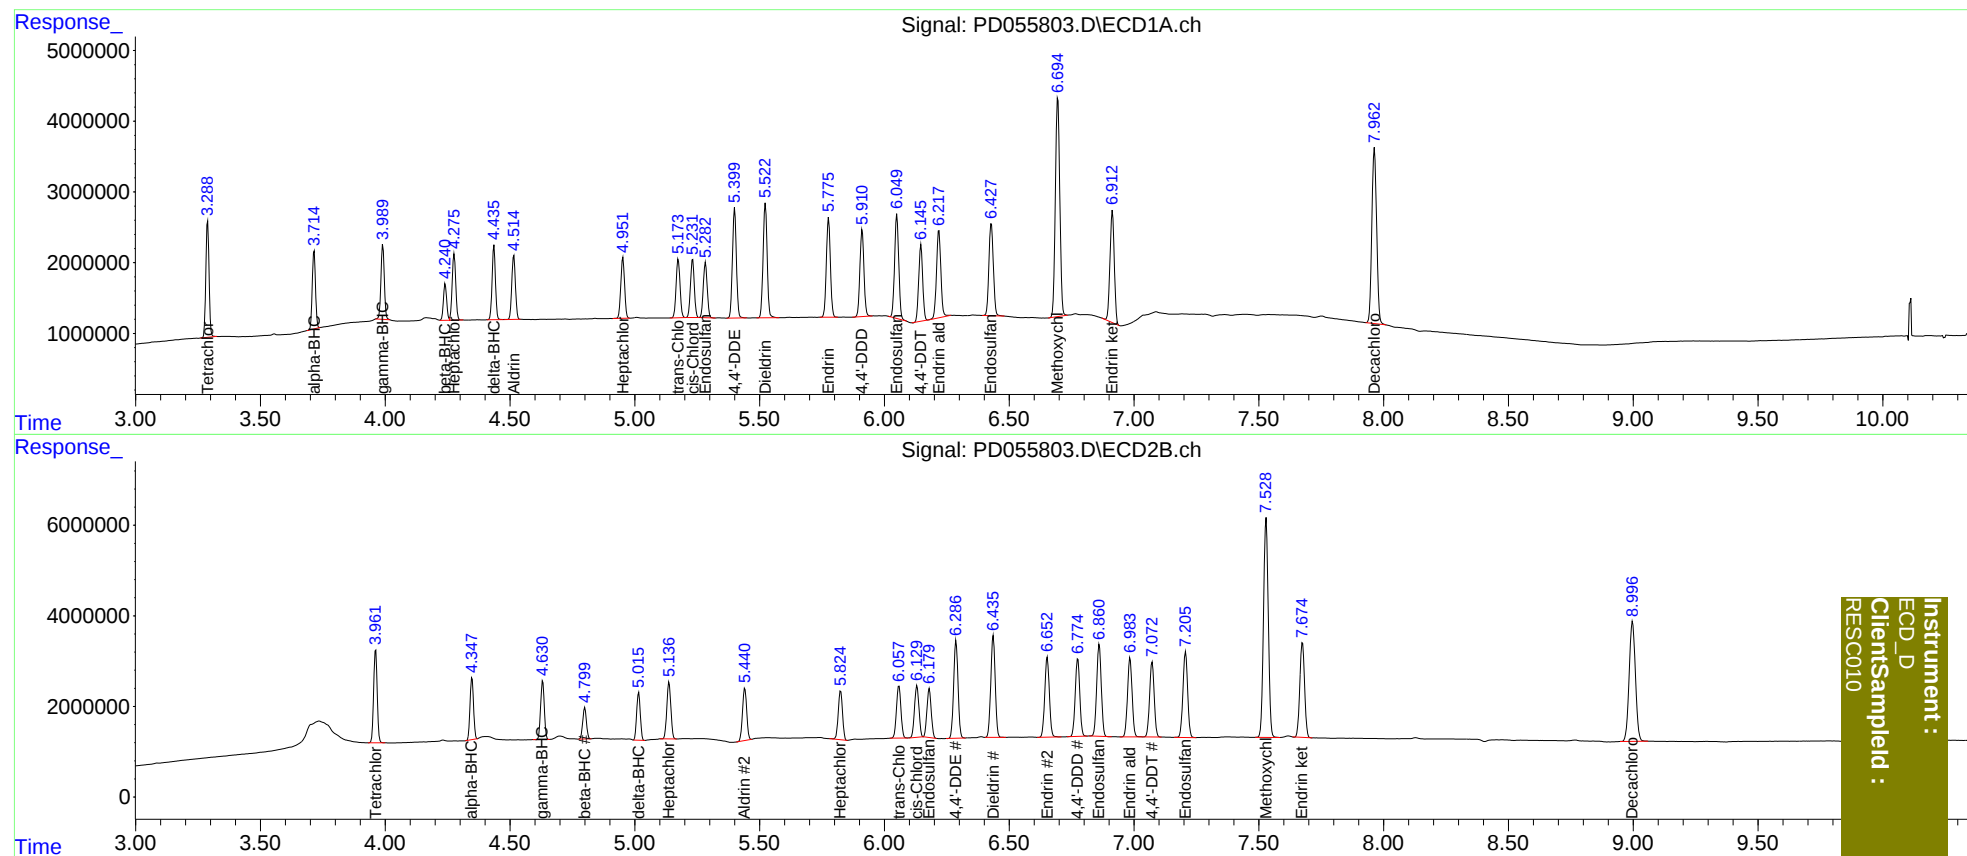

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110319\
Data File : PD055803.D
Acq On : 01 Nov 2019 17:01
Operator : SG\AJ
Sample : RESC10
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC010

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Title : GC Extractables
Last Update : Sat Nov 02 07:20:38 2019
Integrator: ChemStation

RT#1	RT#2	Resolution
3.289	3.716	100.00%
3.716	3.991	100.00%
3.991	4.241	100.00%
4.241	4.277	96.36%
4.277	4.436	100.00%
4.436	4.516	100.00%
4.516	4.953	100.00%
4.953	5.175	100.00%
5.175	5.232	100.00%
5.232	5.284	100.00%
5.284	5.400	100.00%
5.400	5.523	100.00%
5.523	5.777	100.00%
5.777	5.911	100.00%
5.911	6.050	100.00%
6.050	6.147	100.00%
6.147	6.219	100.00%
6.219	6.429	100.00%
6.429	6.695	100.00%
6.695	6.914	100.00%
6.914	7.964	100.00%

Signal #2



3.962	4.348	100.00%
4.348	4.631	100.00%
4.631	4.800	100.00%
4.800	5.016	100.00%
5.016	5.138	100.00%
5.138	5.441	100.00%
5.441	5.825	100.00%
5.825	6.059	100.00%
6.059	6.131	100.00%
6.131	6.180	100.00%
6.180	6.287	100.00%
6.287	6.436	100.00%
6.436	6.653	100.00%
6.653	6.775	100.00%
6.775	6.861	100.00%
6.861	6.985	100.00%
6.985	7.073	100.00%
7.073	7.207	100.00%
7.207	7.530	100.00%
7.530	7.675	100.00%
7.675	8.998	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110319\
Data File : PD055803.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 17:01
Operator : SG\AJ
Sample : RESC10
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC010

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 07:26:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

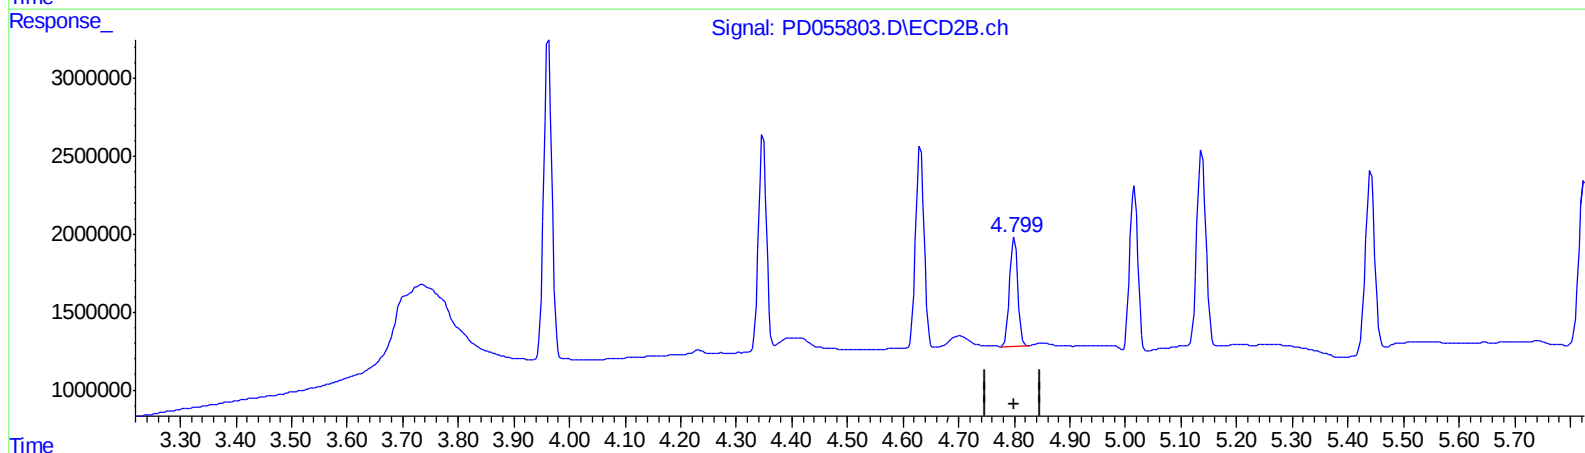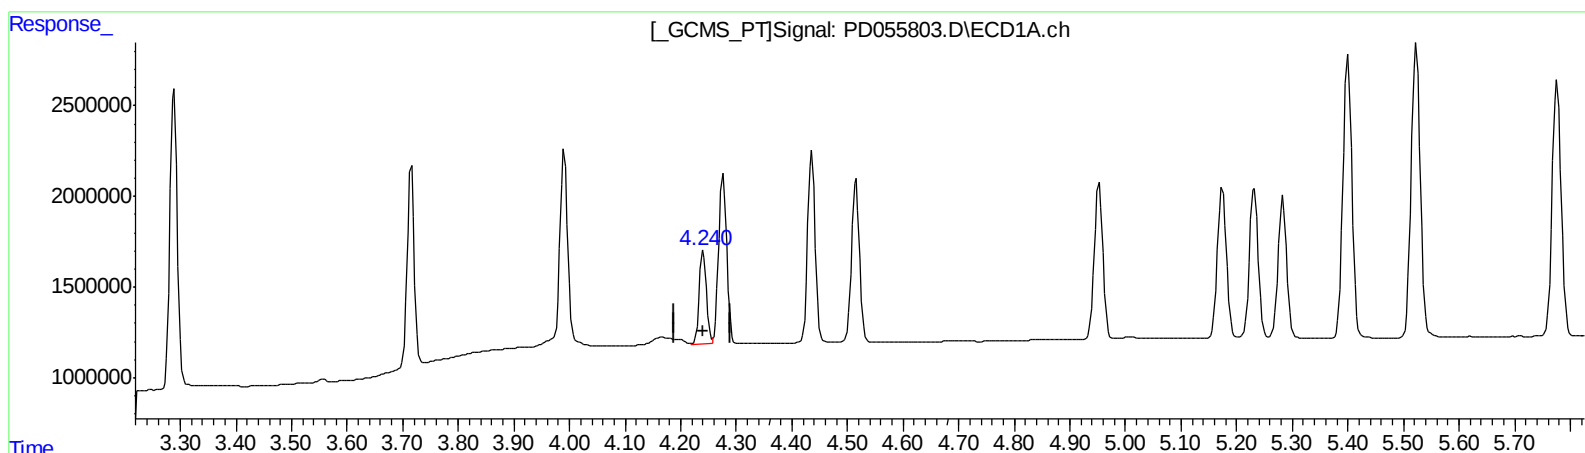

QEdit

(6) beta-BHC (B)

4.241min 10.343 ng/ml

response 4678271

(6) beta-BHC #2 (B)

4.800min 10.305 ng/ml

response 7209624