

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
 Data File : PD060035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 08:22
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 04:07:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds


9) A	Endosulfan I	0.000	6.194f	0	1404580	N.D.	0.438
10) B	trans-Chl...	5.439	6.143	6352784	12449294	5.981	3.623 #
11) B	cis-Chlor...	0.000	6.194	0	1404580	N.D.	0.409
17) MA	4,4'-DDT	0.000	7.152	0	1205551	N.D.	0.443
19) B	Endosulfa...	6.691f	0.000	1635744	0	1.872	N.D. #
20) A	Methoxychlor	7.038	0.000	19887367	0	46.731	N.D. #
24)	Toxaphene-3	0.000	7.152	0	1205551	N.D.	43.469
25)	Toxaphene-4	0.000	7.152	0	1205551	N.D.	15.896

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 08:22
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 04:07:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

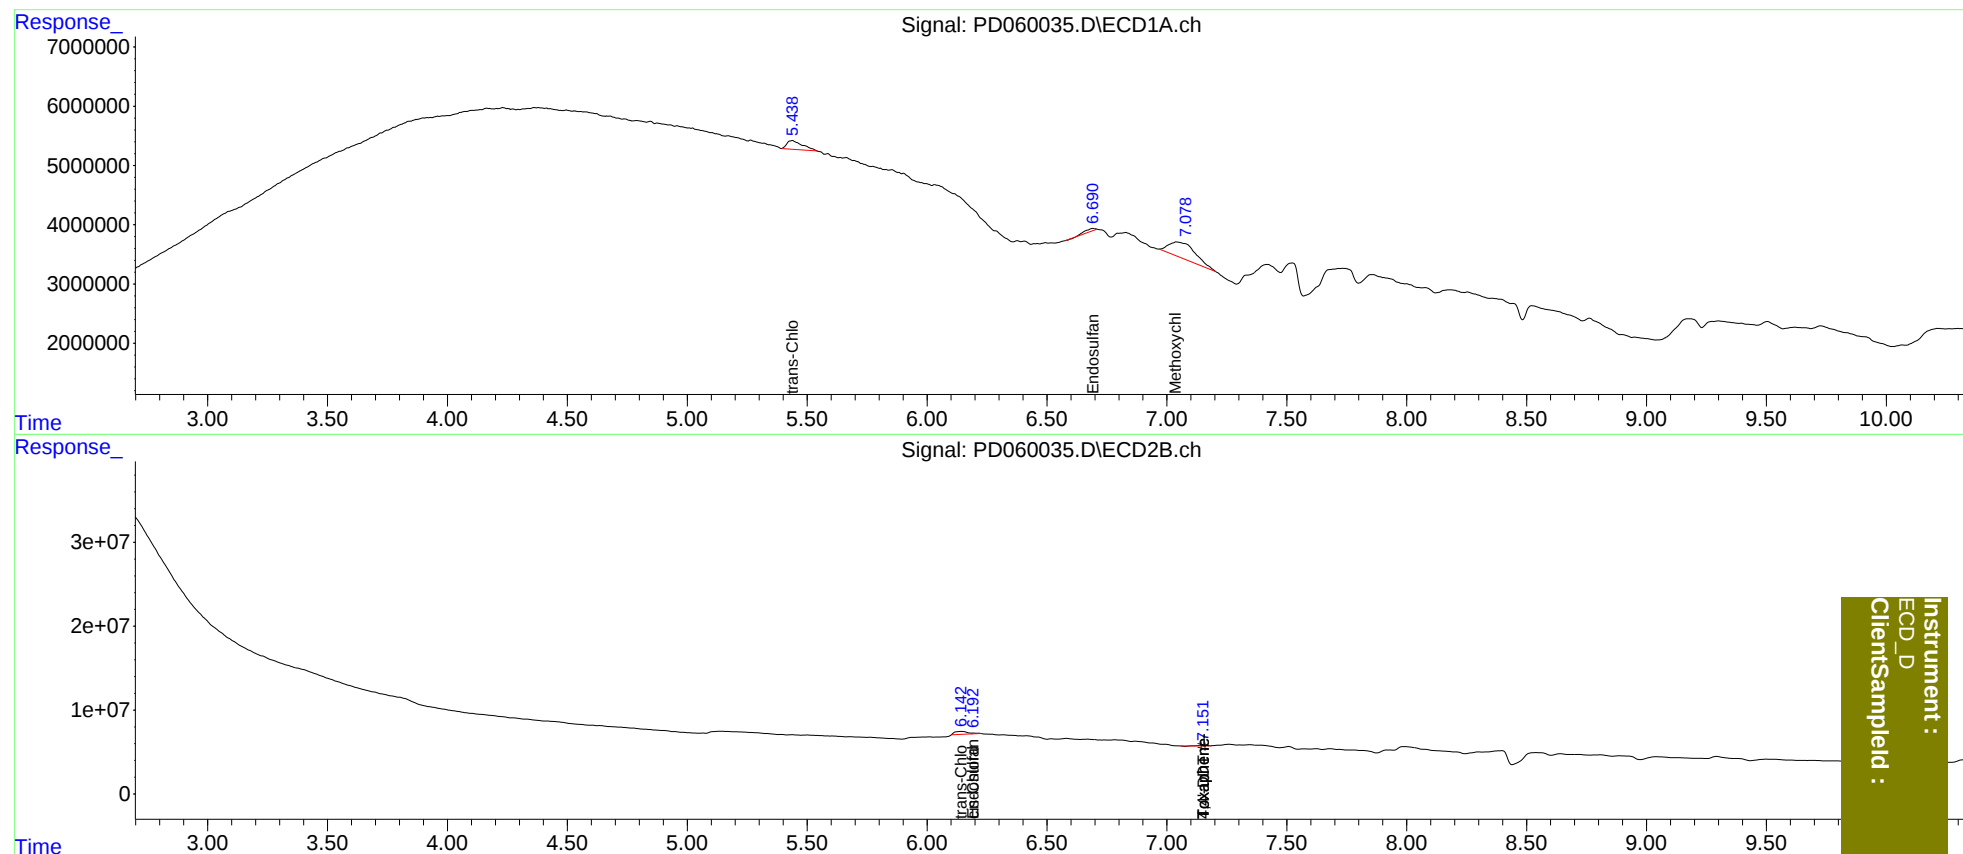


Instrument :
ECD_D
ClientSampled :

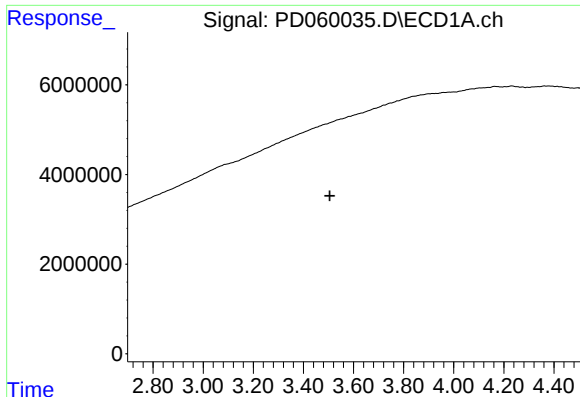

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

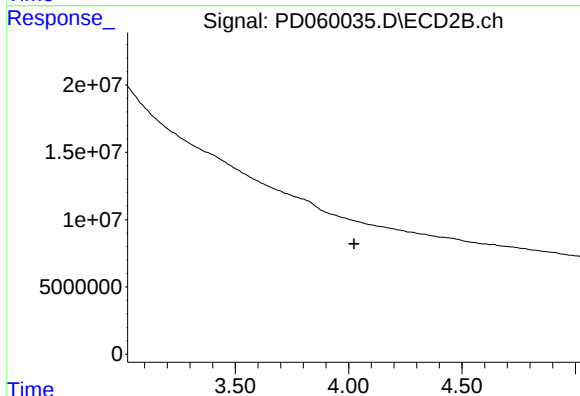


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.024 min
Response: 0
Conc: N.D.

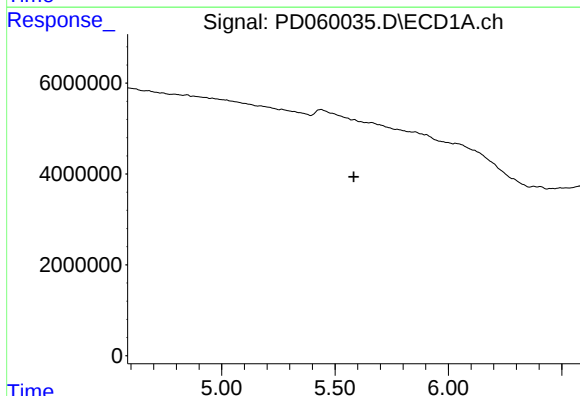


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.582 min
Response: 0
Conc: N.D.

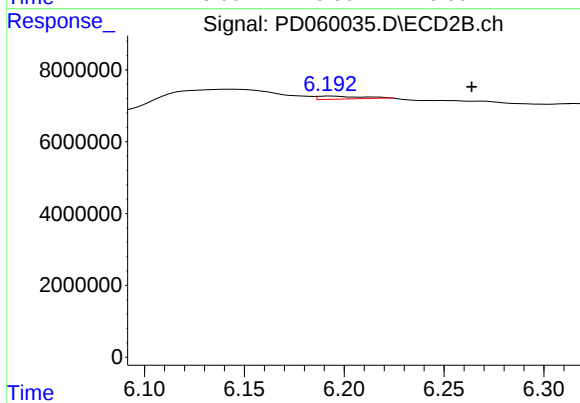

#9 Endosulfan I


R.T.: 6.194 min
Delta R.T.: -0.070 min
Response: 1404580
Conc: 0.44 ng/ml

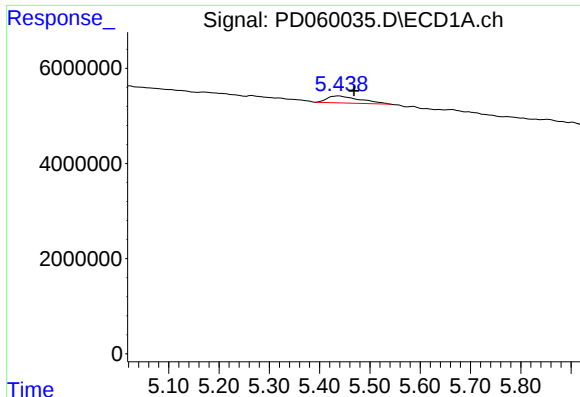

#10 trans-Chlordane


R.T.: 5.439 min
Delta R.T.: -0.030 min
Response: 6352784
Conc: 5.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

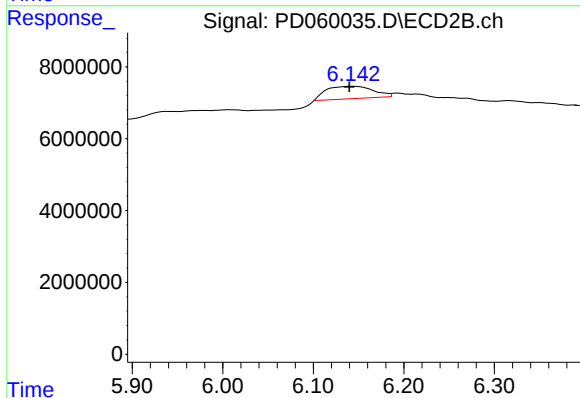


#10 trans-Chlordane

R.T.: 6.143 min
Delta R.T.: 0.004 min
Response: 12449294
Conc: 3.62 ng/ml

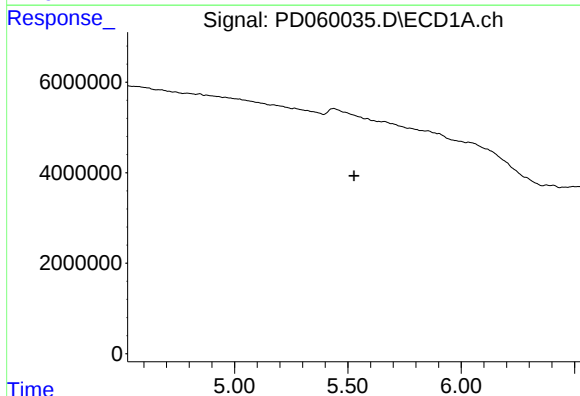


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.528 min
Response: 0
Conc: N.D.

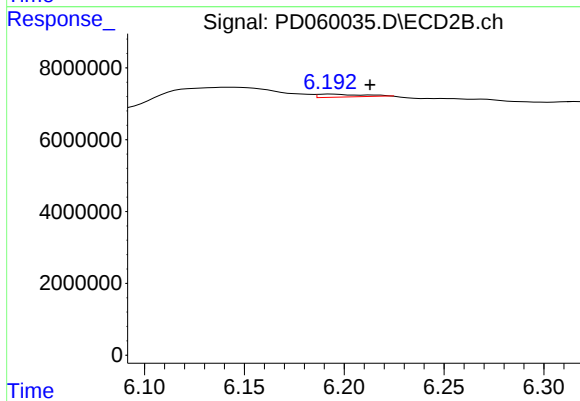

#11 cis-Chlordane


R.T.: 6.194 min
Delta R.T.: -0.019 min
Response: 1404580
Conc: 0.41 ng/ml

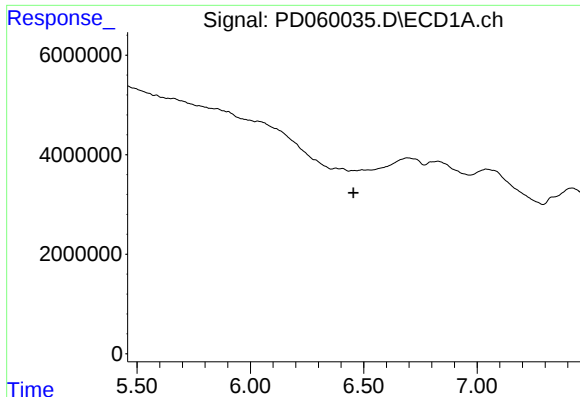

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

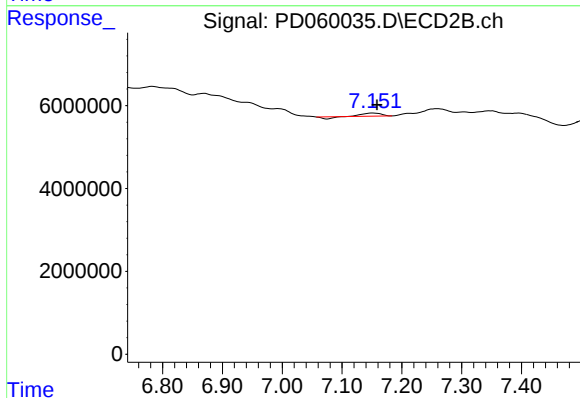


#17 4,4'-DDT

R.T.: 7.152 min
Delta R.T.: -0.006 min
Response: 1205551
Conc: 0.44 ng/ml

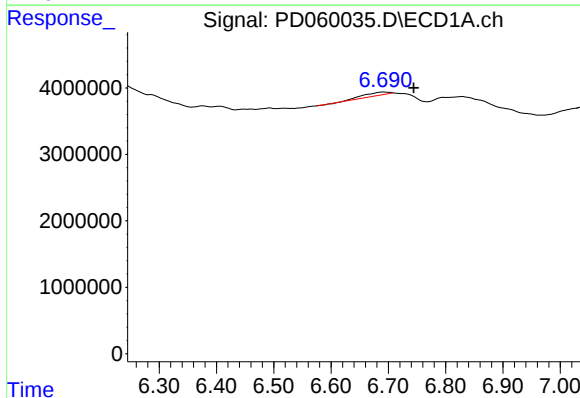


#19 Endosulfan Sulfate

R.T.: 6.691 min
Delta R.T.: -0.053 min
Response: 1635744
Conc: 1.87 ng/ml

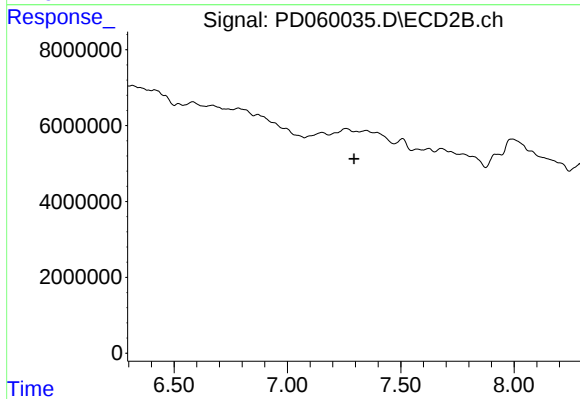

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.294 min
Response: 0
Conc: N.D.

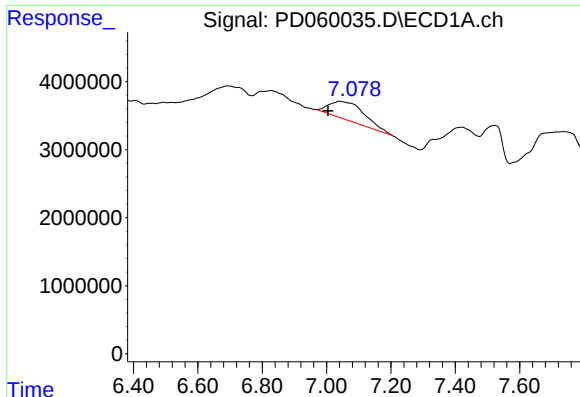

#20 Methoxychlor


R.T.: 7.038 min
Delta R.T.: 0.034 min
Response: 19887367
Conc: 46.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

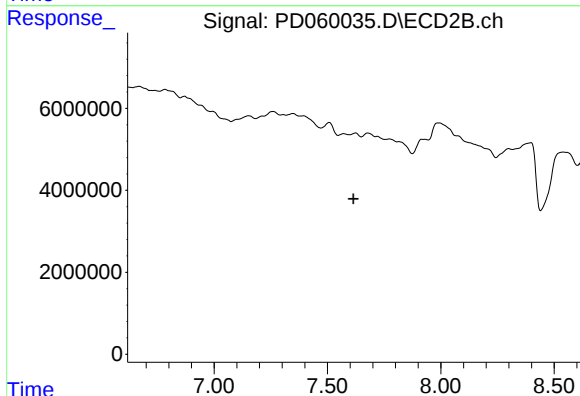


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.615 min
Response: 0
Conc: N.D.

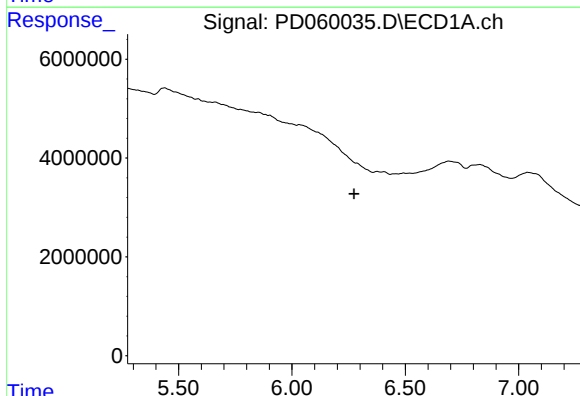


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 6.275 min
Response: 0
Conc: N.D.

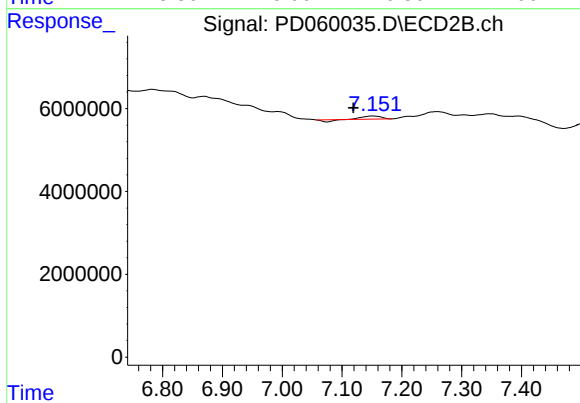

#24 Toxaphene-3


R.T.: 7.152 min
Delta R.T.: 0.033 min
Response: 1205551
Conc: 43.47 ng/ml

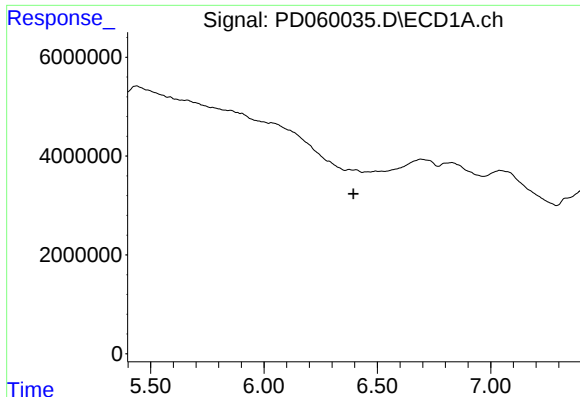

#25 Toxaphene-4


R.T.: 0.000 min
Exp R.T.: 6.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

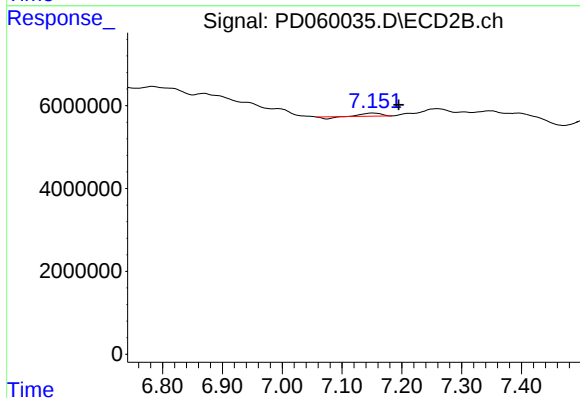


#25 Toxaphene-4

R.T.: 7.152 min
Delta R.T.: -0.043 min
Response: 1205551
Conc: 15.90 ng/ml

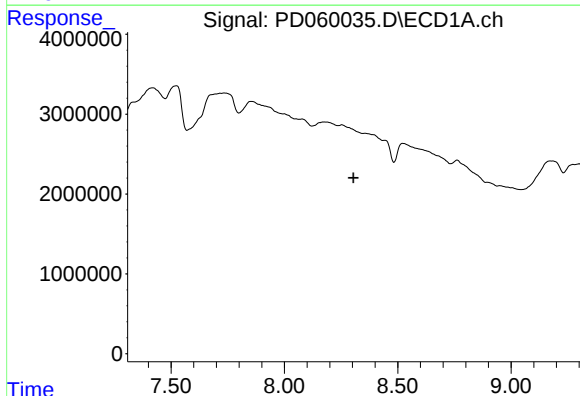

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.305 min
Response: 0
Conc: N.D.

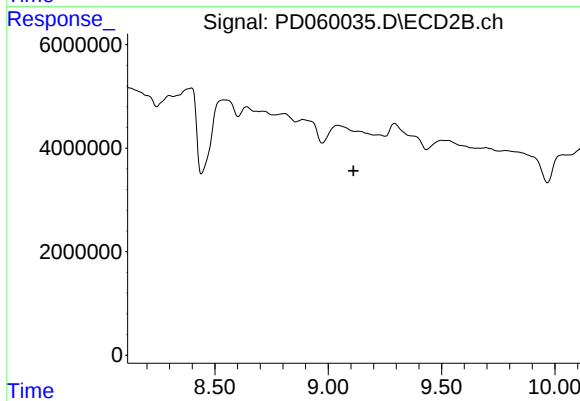

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.112 min
Response: 0
Conc: N.D.