

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
 Data File : PD060046.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 12:55
 Operator : DD\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 03:53:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 03:53:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.506	4.024	4692001	15035564	5.432	4.960
27)	SA Decachlor...	8.305	9.112	9397159	26367043	11.122	10.480
Target Compounds							
2)	A alpha-BHC	3.947	4.415	6950804	22078140	5.411	4.922
3)	MA gamma-BHC...	4.234	4.701	6700398	19770350	5.468	4.802
4)	MA Heptachlor	4.541	5.213	6447108	20502416	5.435	5.080
9)	A Endosulfan I	5.582	6.264	5640557	16320356	5.492	5.021
13)	MA Dieldrin	5.828	6.521	11913670	34634611	10.931	9.749
14)	MA Endrin	6.087	6.740	9910725	27831486	10.916	9.770
16)	A 4,4'-DDD	6.212	6.859	9978402	26295142	11.333	9.626
17)	MA 4,4'-DDT	6.455	7.159	9557374	26518047	10.510	9.591
20)	A Methoxychlor	7.005	7.615	23420659	74591186	54.383	51.887


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060046.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 12:55
Operator : DD\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 03:53:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 03:53:19 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

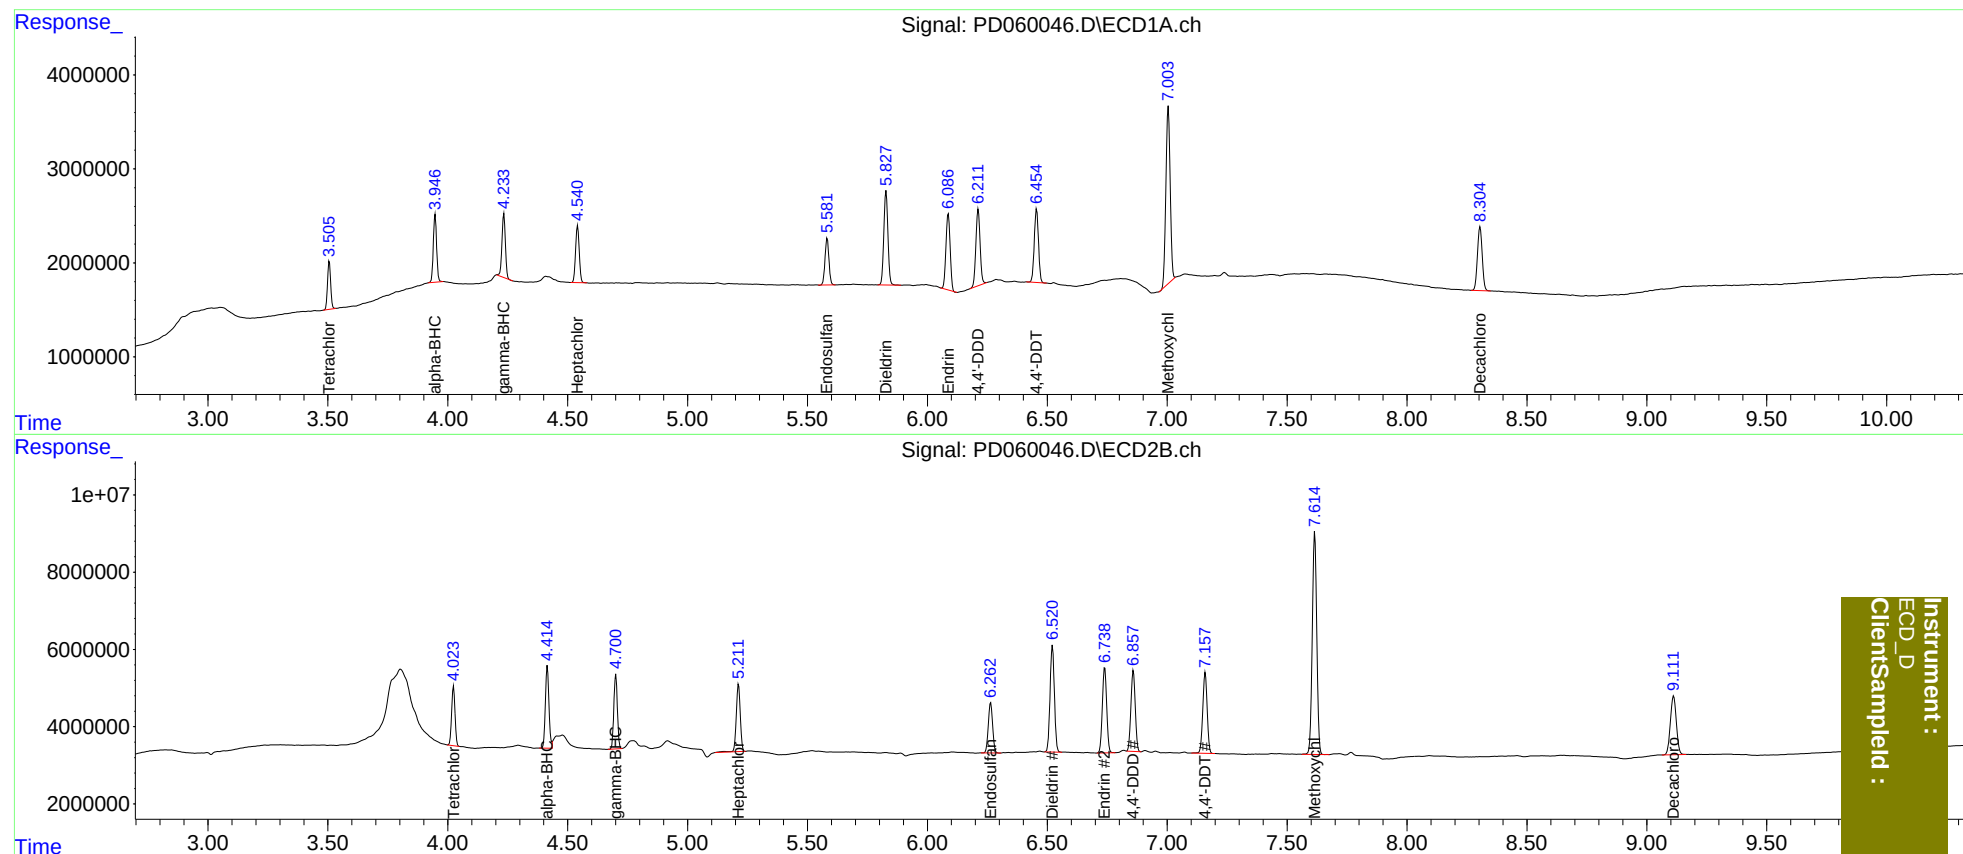


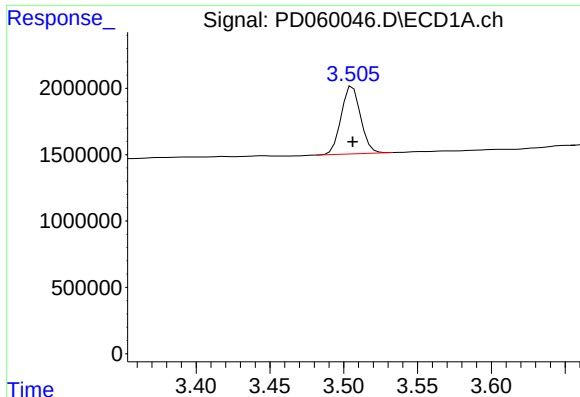

#1 Tetrachloro-m-xylene


R.T.: 3.506 min
Delta R.T.: 0.000 min
Response: 4692001
Conc: 5.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

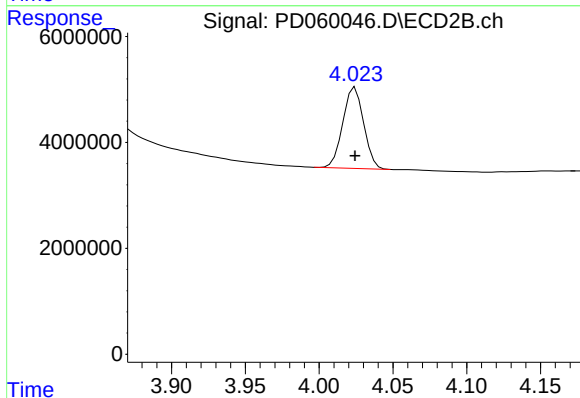


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 15035564
Conc: 4.96 ng/ml

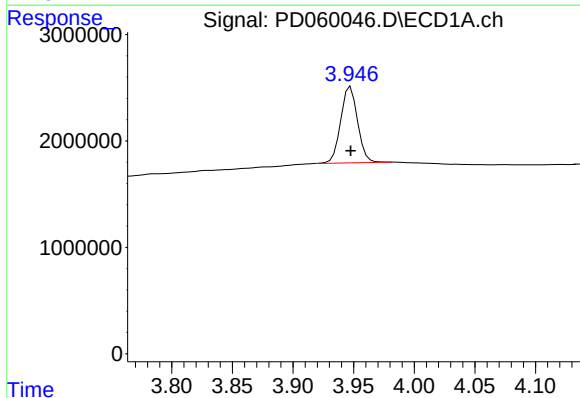


#2 alpha-BHC

R.T.: 3.947 min
Delta R.T.: 0.000 min
Response: 6950804
Conc: 5.41 ng/ml

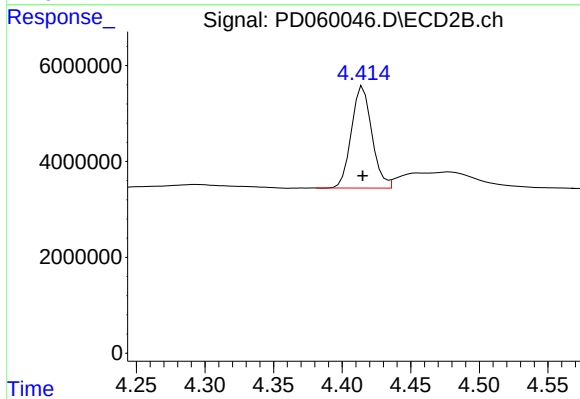

#2 alpha-BHC


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 22078140
Conc: 4.92 ng/ml

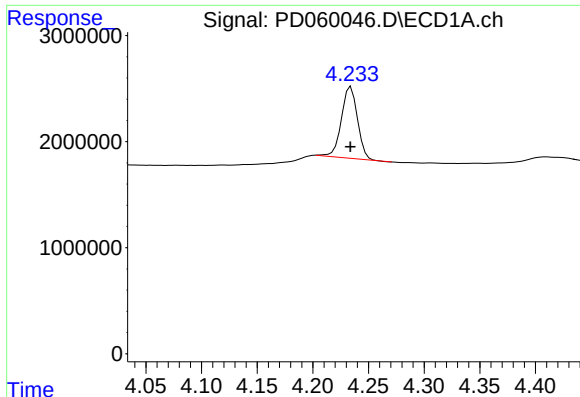

#3 gamma-BHC (Lindane)


R.T.: 4.234 min
Delta R.T.: 0.000 min
Response: 6700398
Conc: 5.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

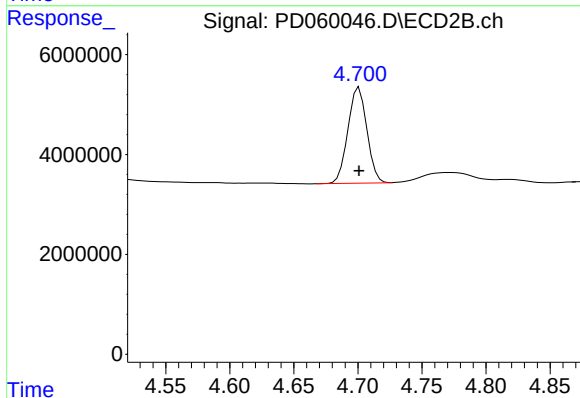


#3 gamma-BHC (Lindane)

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 19770350
Conc: 4.80 ng/ml

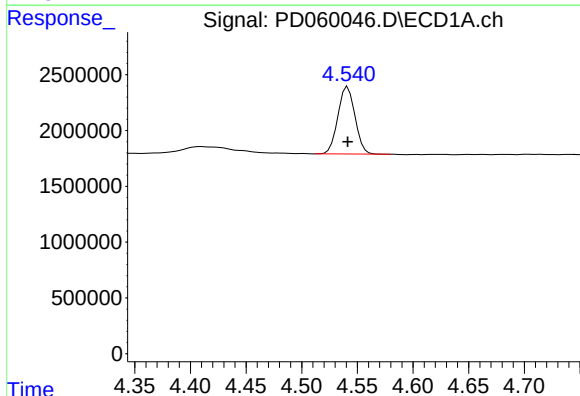


#4 Heptachlor

R.T.: 4.541 min
Delta R.T.: 0.000 min
Response: 6447108
Conc: 5.44 ng/ml

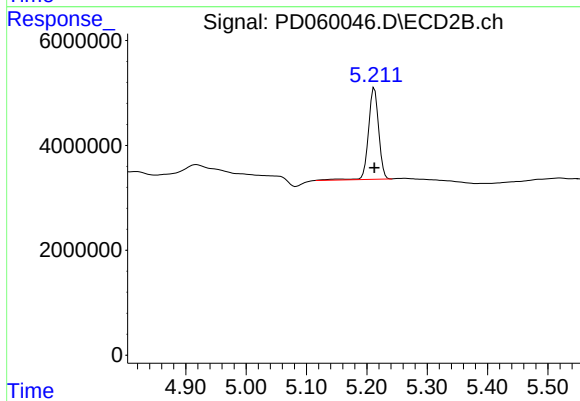

#4 Heptachlor


R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 20502416
Conc: 5.08 ng/ml

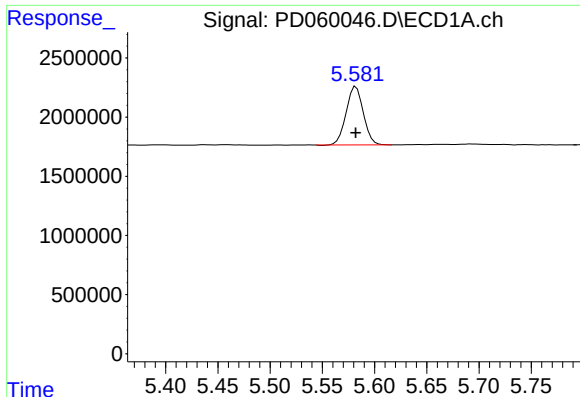

#9 Endosulfan I


R.T.: 5.582 min
Delta R.T.: 0.000 min
Response: 5640557
Conc: 5.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

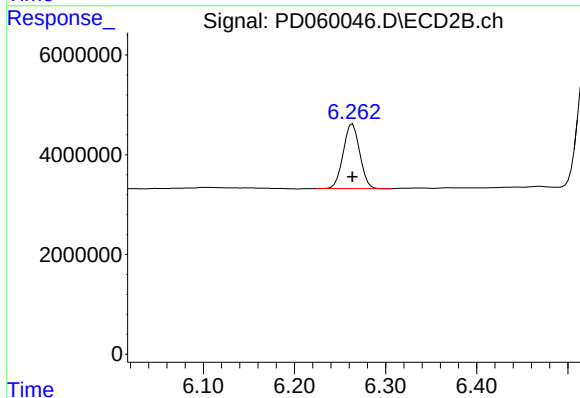


#9 Endosulfan I

R.T.: 6.264 min
Delta R.T.: 0.000 min
Response: 16320356
Conc: 5.02 ng/ml

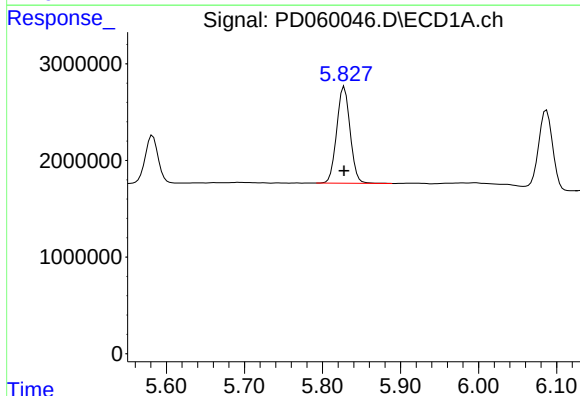


#13 Dieldrin

R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 11913670
Conc: 10.93 ng/ml

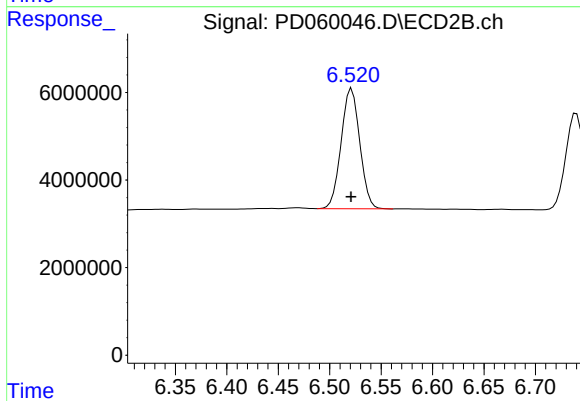

#13 Dieldrin


R.T.: 6.521 min
Delta R.T.: 0.000 min
Response: 34634611
Conc: 9.75 ng/ml

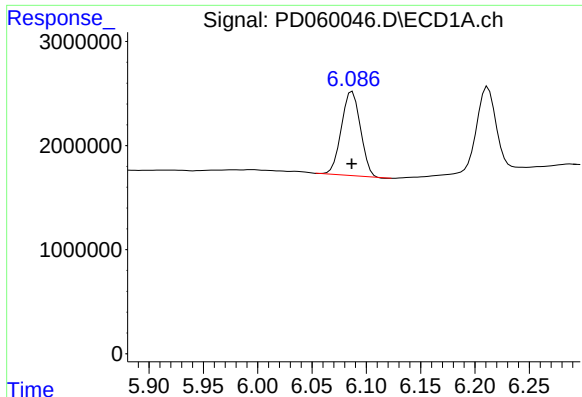

#14 Endrin


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 9910725
Conc: 10.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

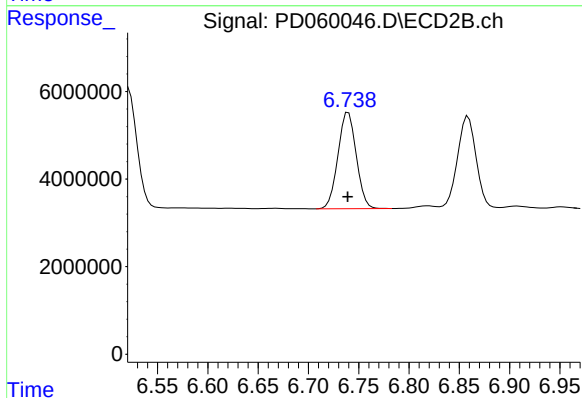


#14 Endrin

R.T.: 6.740 min
Delta R.T.: 0.000 min
Response: 27831486
Conc: 9.77 ng/ml

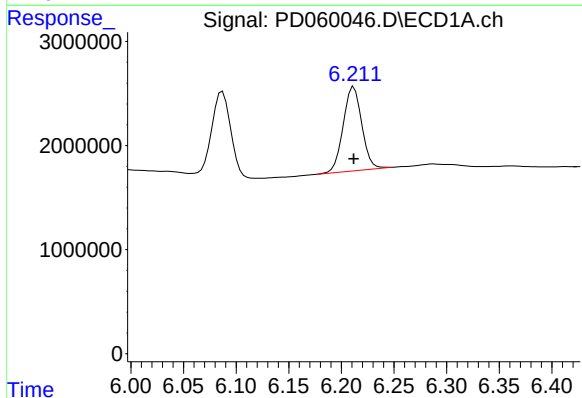


#16 4,4'-DDD

R.T.: 6.212 min
Delta R.T.: 0.000 min
Response: 9978402
Conc: 11.33 ng/ml

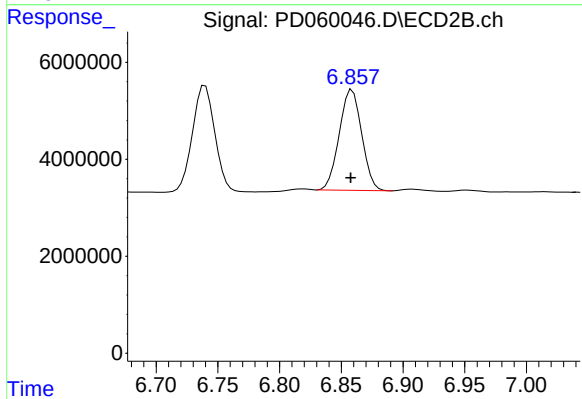

#16 4,4'-DDD


R.T.: 6.859 min
Delta R.T.: 0.001 min
Response: 26295142
Conc: 9.63 ng/ml

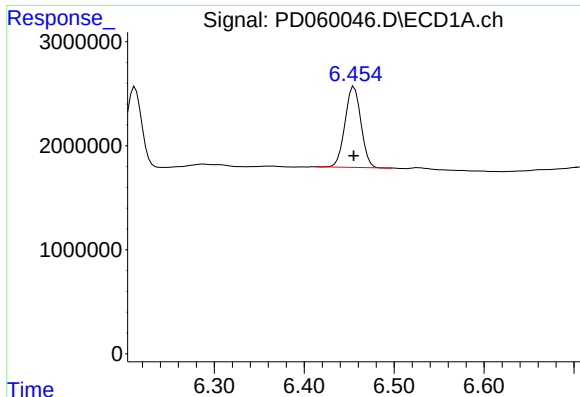

#17 4,4'-DDT


R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 9557374
Conc: 10.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

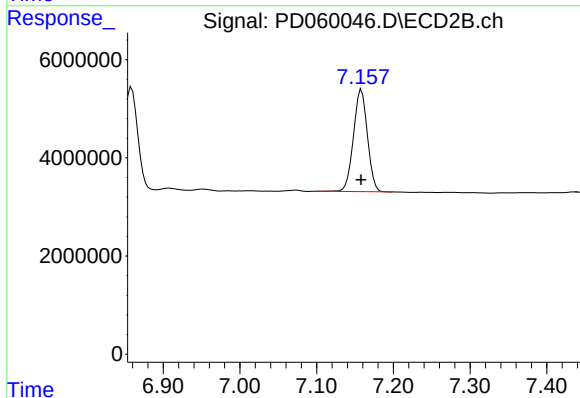


#17 4,4'-DDT

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 26518047
Conc: 9.59 ng/ml

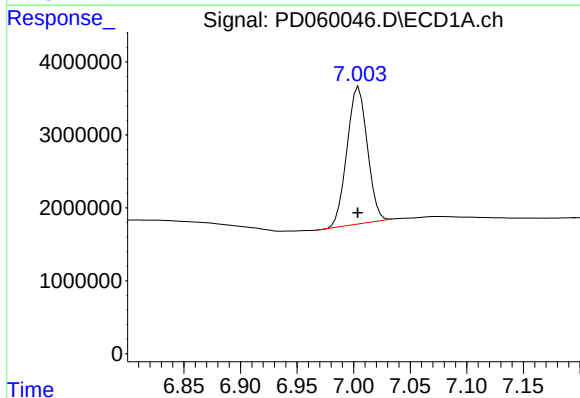


#20 Methoxychlor

R.T.: 7.005 min
Delta R.T.: 0.000 min
Response: 23420659
Conc: 54.38 ng/ml

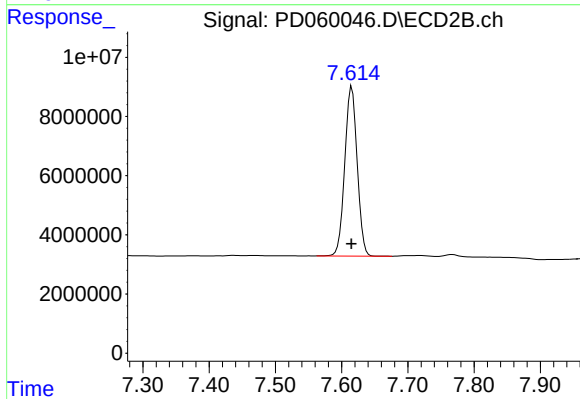

#20 Methoxychlor


R.T.: 7.615 min
Delta R.T.: 0.000 min
Response: 74591186
Conc: 51.89 ng/ml

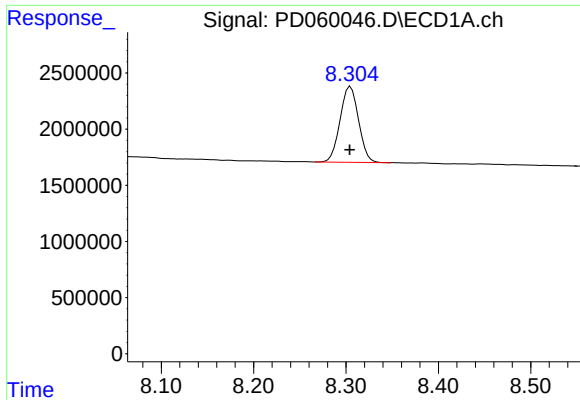

#27 Decachlorobiphenyl

R.T.: 8.305 min
Delta R.T.: 0.000 min
Response: 9397159
Conc: 11.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

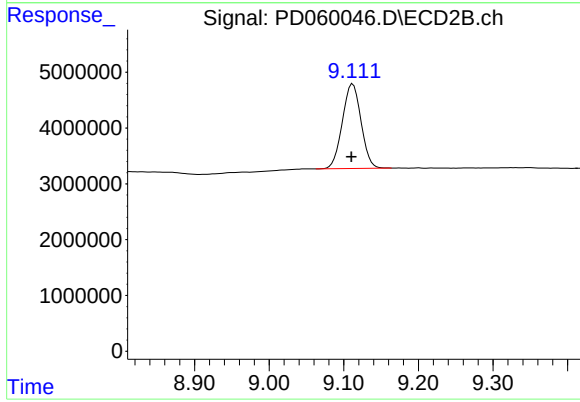

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.002 min
Response: 26367043
Conc: 10.48 ng/ml