

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
 Data File : PD060050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 13:52
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 03:54:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 03:53:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.506	4.024	17275441	60629275	20.000	20.000
27)	SA Decachlor...	8.304	9.110	33795735	100.6E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.948	4.415	25690684	89712830	20.000	20.000
3)	MA gamma-BHC...	4.234	4.701	24508086	82349301	20.000	20.000
4)	MA Heptachlor	4.541	5.213	23724338	80722312	20.000	20.000
9)	A Endosulfan I	5.582	6.264	20539623	65008883	20.000	20.000
13)	MA Dieldrin	5.828	6.521	43597481	142.1E6	40.000	40.000
14)	MA Endrin	6.087	6.739	36316990	113.9E6	40.000	40.000
16)	A 4,4'-DDD	6.212	6.858	35218724	109.3E6	40.000	40.000
17)	MA 4,4'-DDT	6.455	7.158	36375685	110.6E6	40.000	40.000
20)	A Methoxychlor	7.004	7.615	86132787	287.5E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 13:52
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 03:54:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 03:53:19 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

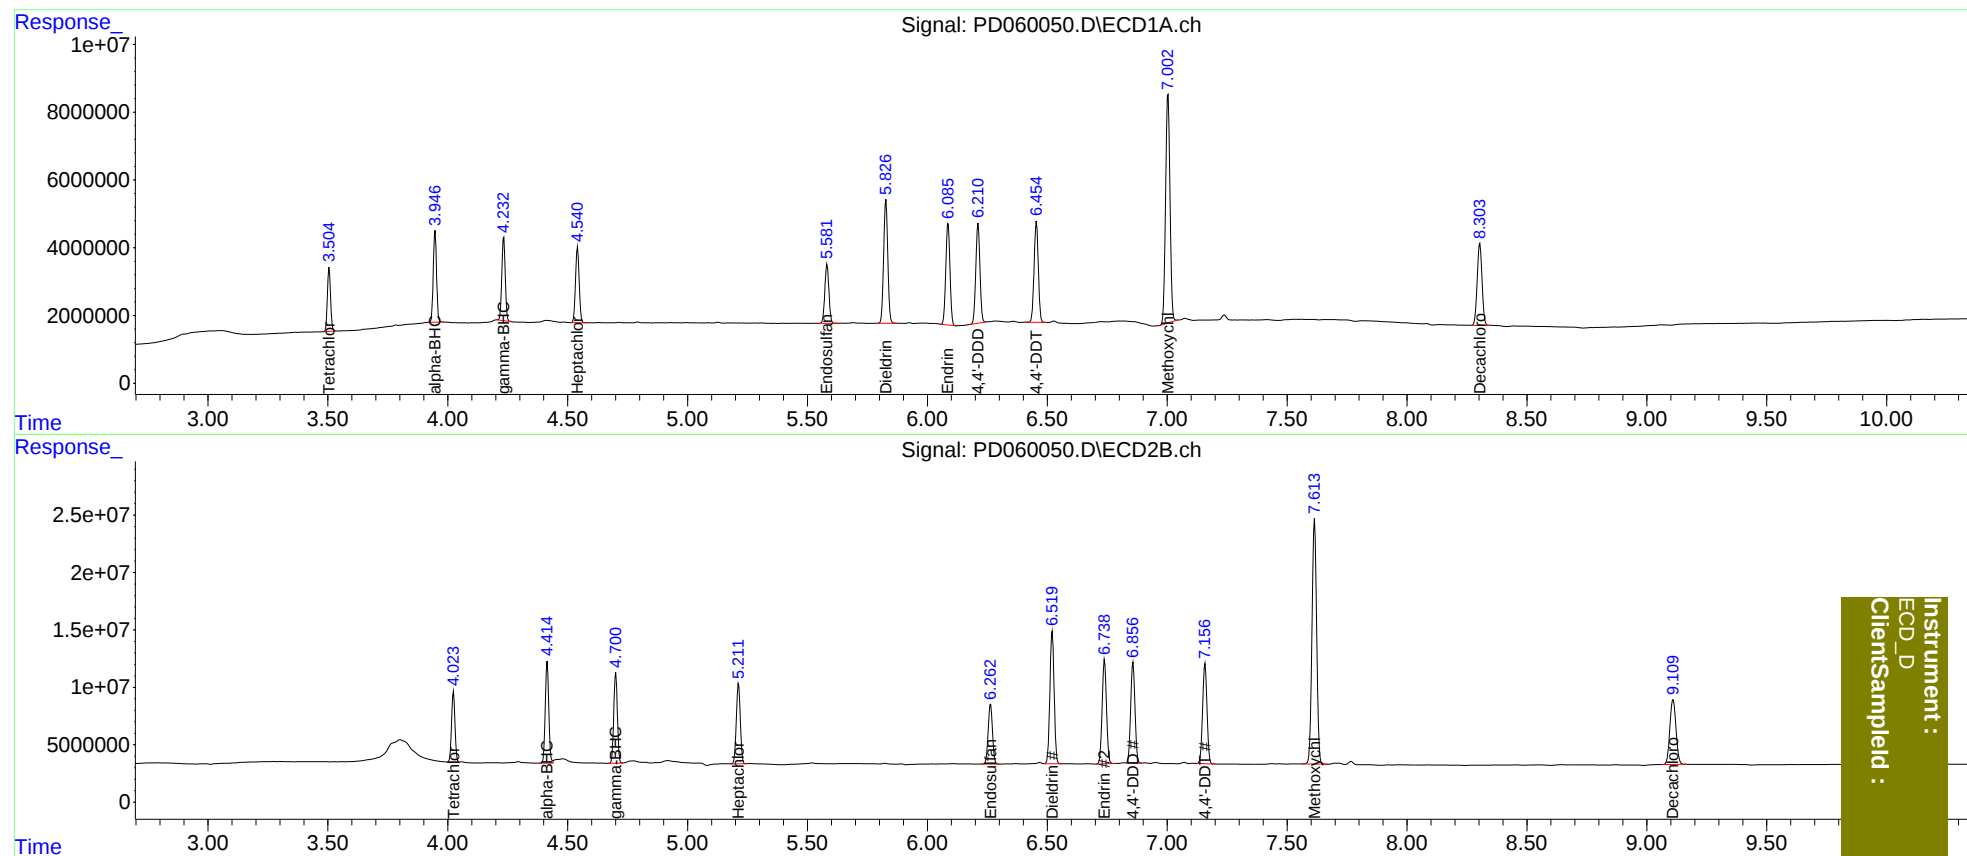


Instrument :
ECD_D
ClientSample :
INDA301

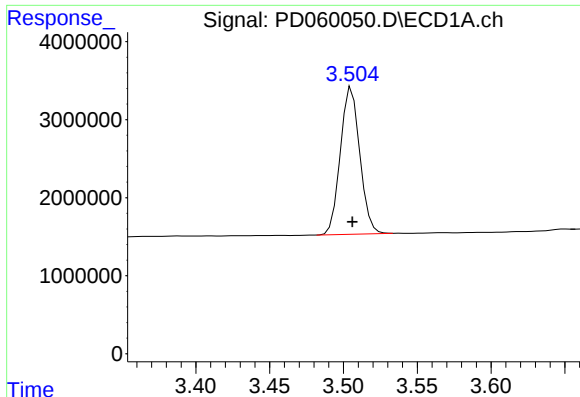

#1 Tetrachloro-m-xylene


R.T.: 3.506 min
Delta R.T.: 0.000 min
Response: 17275441
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

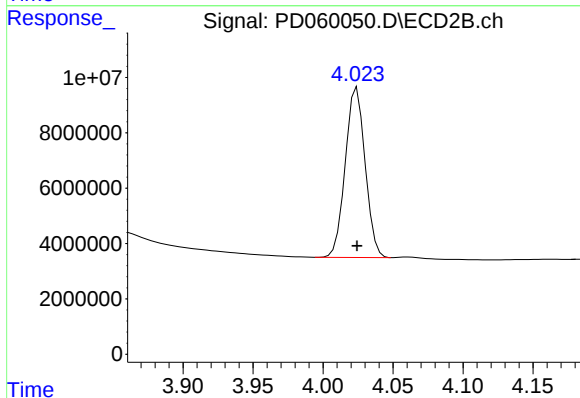


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 60629275
Conc: 20.00 ng/ml

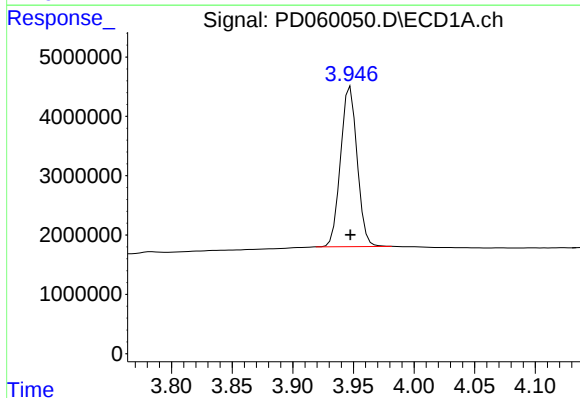


#2 alpha-BHC

R.T.: 3.948 min
Delta R.T.: 0.000 min
Response: 25690684
Conc: 20.00 ng/ml

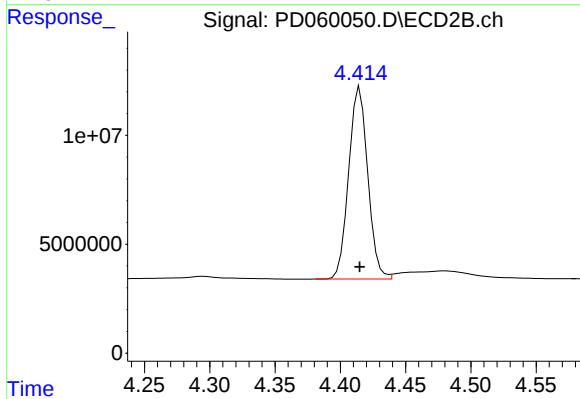

#2 alpha-BHC


R.T.: 4.415 min
Delta R.T.: 0.000 min
Response: 89712830
Conc: 20.00 ng/ml

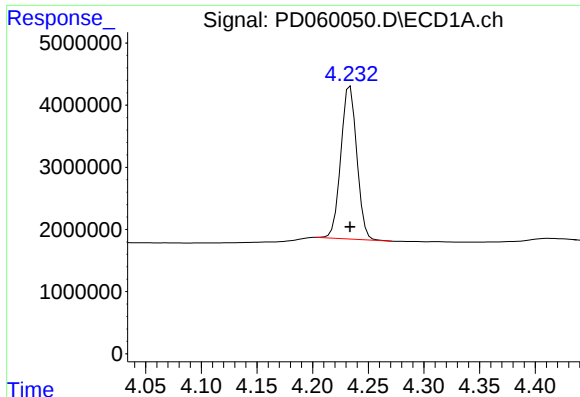

#3 gamma-BHC (Lindane)


R.T.: 4.234 min
Delta R.T.: 0.000 min
Response: 24508086
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

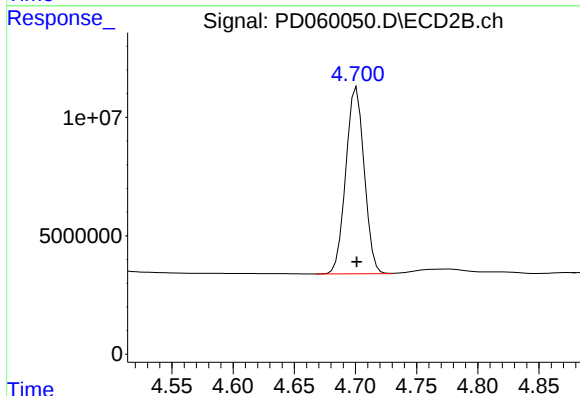


#3 gamma-BHC (Lindane)

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 82349301
Conc: 20.00 ng/ml

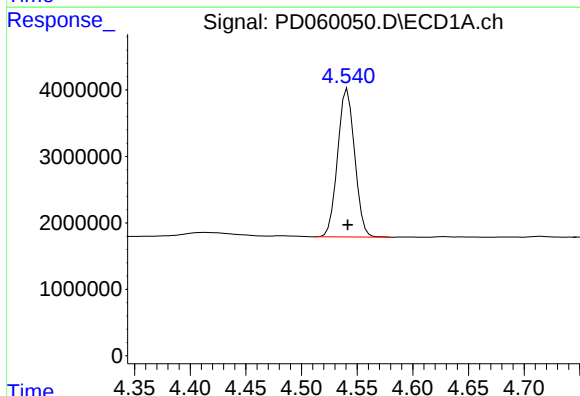


#4 Heptachlor

R.T.: 4.541 min
Delta R.T.: 0.000 min
Response: 23724338
Conc: 20.00 ng/ml

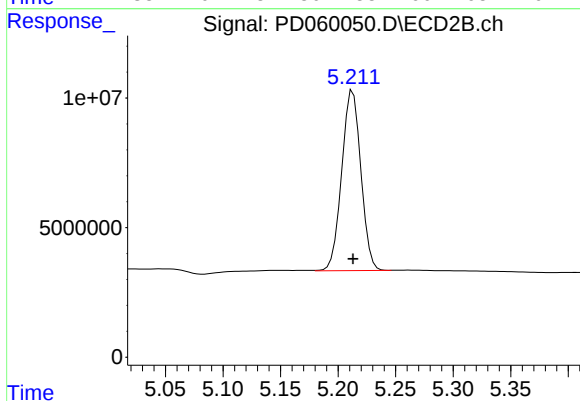

#4 Heptachlor


R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 80722312
Conc: 20.00 ng/ml

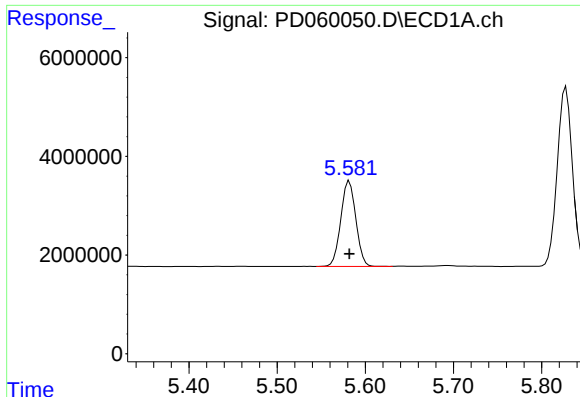

#9 Endosulfan I


R.T.: 5.582 min
Delta R.T.: 0.000 min
Response: 20539623
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

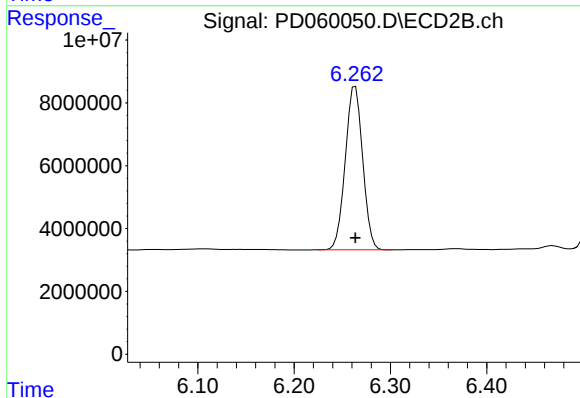


#9 Endosulfan I

R.T.: 6.264 min
Delta R.T.: 0.000 min
Response: 65008883
Conc: 20.00 ng/ml

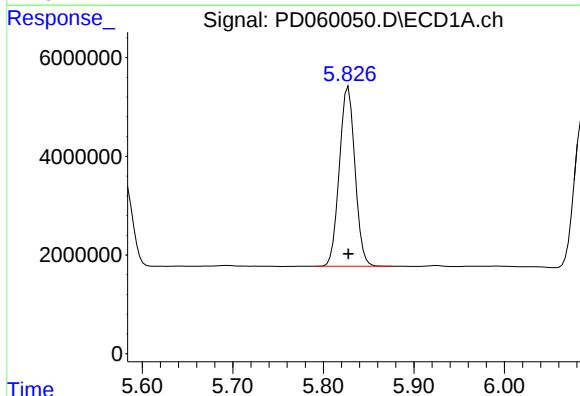


#13 Dieldrin

R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 43597481
Conc: 40.00 ng/ml

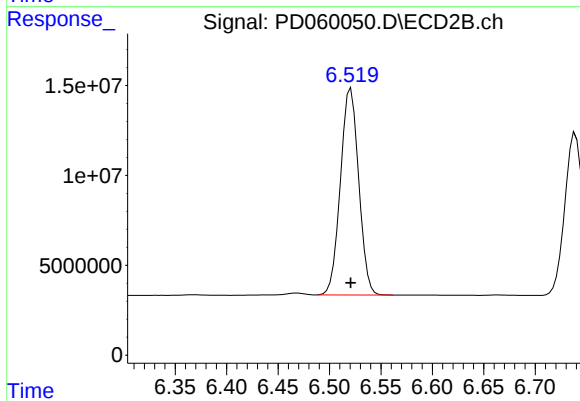

#13 Dieldrin


R.T.: 6.521 min
Delta R.T.: 0.000 min
Response: 142098106
Conc: 40.00 ng/ml

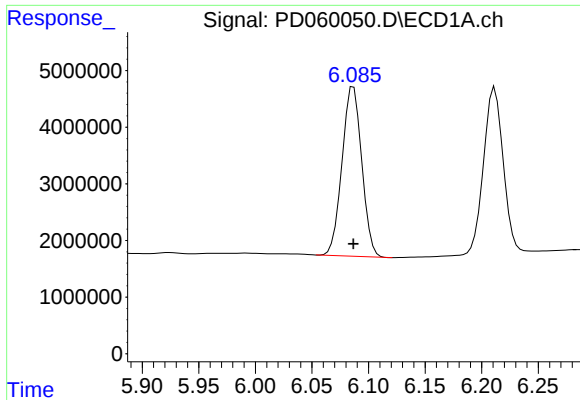

#14 Endrin


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 36316990
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

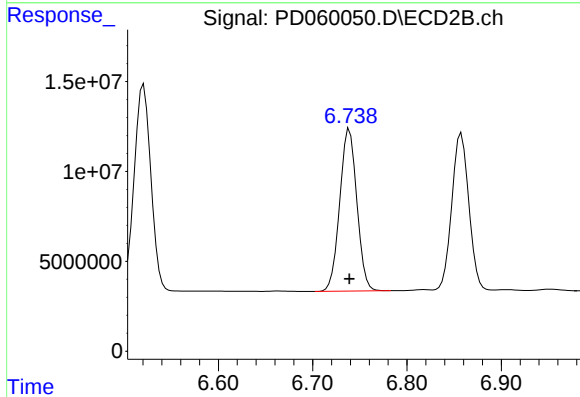


#14 Endrin

R.T.: 6.739 min
Delta R.T.: 0.000 min
Response: 113945542
Conc: 40.00 ng/ml

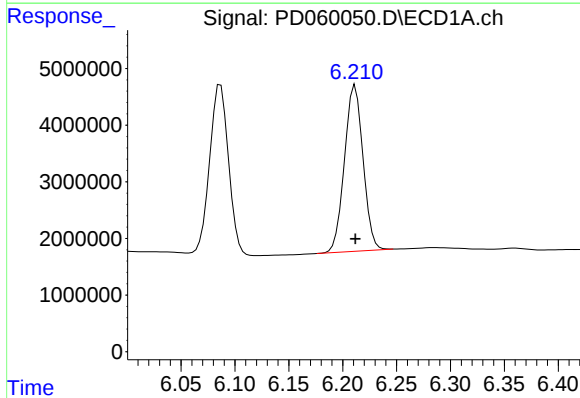


#16 4,4'-DDD

R.T.: 6.212 min
Delta R.T.: 0.000 min
Response: 35218724
Conc: 40.00 ng/ml

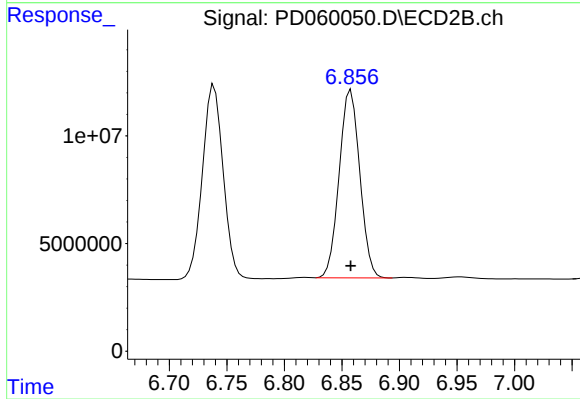

#16 4,4'-DDD


R.T.: 6.858 min
Delta R.T.: 0.000 min
Response: 109269723
Conc: 40.00 ng/ml

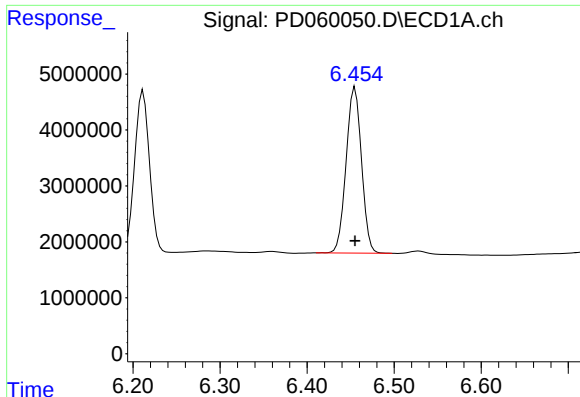

#17 4,4'-DDT


R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 36375685
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

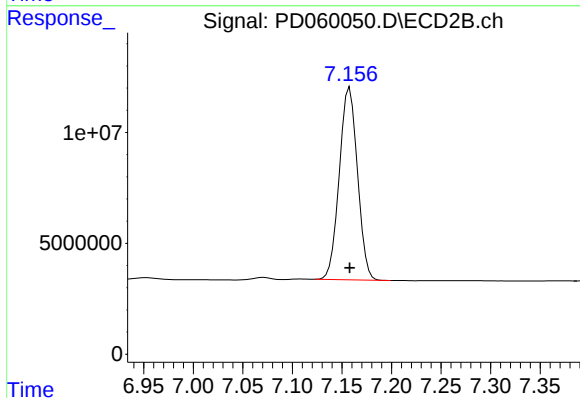


#17 4,4'-DDT

R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 110601014
Conc: 40.00 ng/ml

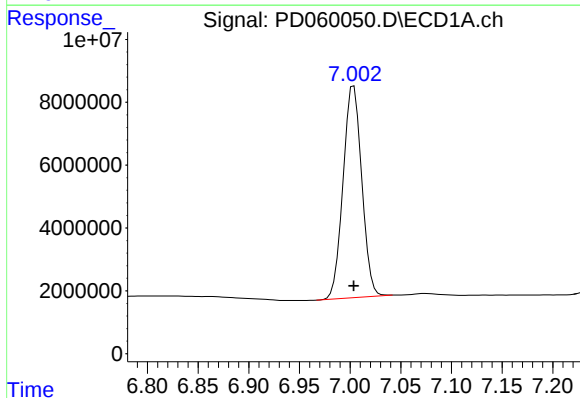


#20 Methoxychlor

R.T.: 7.004 min
Delta R.T.: 0.000 min
Response: 86132787
Conc: 200.00 ng/ml

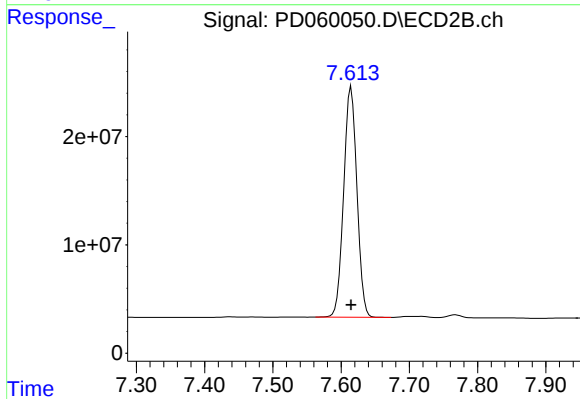

#20 Methoxychlor


R.T.: 7.615 min
Delta R.T.: 0.000 min
Response: 287515349
Conc: 200.00 ng/ml

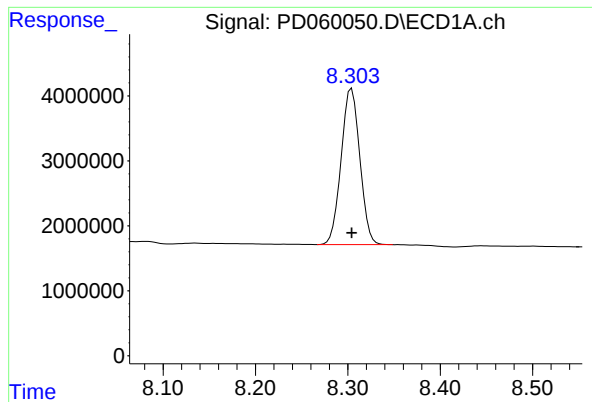

#27 Decachlorobiphenyl

R.T.: 8.304 min
Delta R.T.: 0.000 min
Response: 33795735
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

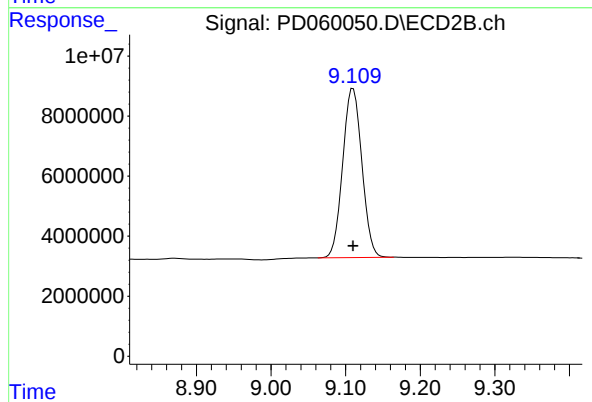

#27 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 100634522
Conc: 40.00 ng/ml