

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
 Data File : PD060052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 14:20
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 03:54:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 03:53:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.506	4.024	32212293	115.8E6	37.293	38.211
27)	SA Decachlor...	8.305	9.110	61114850	188.6E6	72.334	74.955
Target Compounds							
2)	A alpha-BHC	3.947	4.414	48706163	176.6E6	37.917	39.377
3)	MA gamma-BHC...	4.234	4.700	45647099	160.6E6	37.251	38.996
4)	MA Heptachlor	4.541	5.212	43964217	156.6E6	37.063	38.799
9)	A Endosulfan I	5.583	6.264	37924120	124.8E6	36.928	38.399
13)	MA Dieldrin	5.828	6.521	81902338	276.8E6	75.144	77.921
14)	MA Endrin	6.087	6.739	67839009	222.8E6	74.719	78.229
16)	A 4,4'-DDD	6.212	6.858	65557658	214.1E6	74.458	78.378
17)	MA 4,4'-DDT	6.455	7.158	68455038	219.5E6	75.276	79.400
20)	A Methoxychlor	7.004	7.615	160.0E6	543.1E6	371.465	377.768

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 14:20
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 03:54:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 03:53:19 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

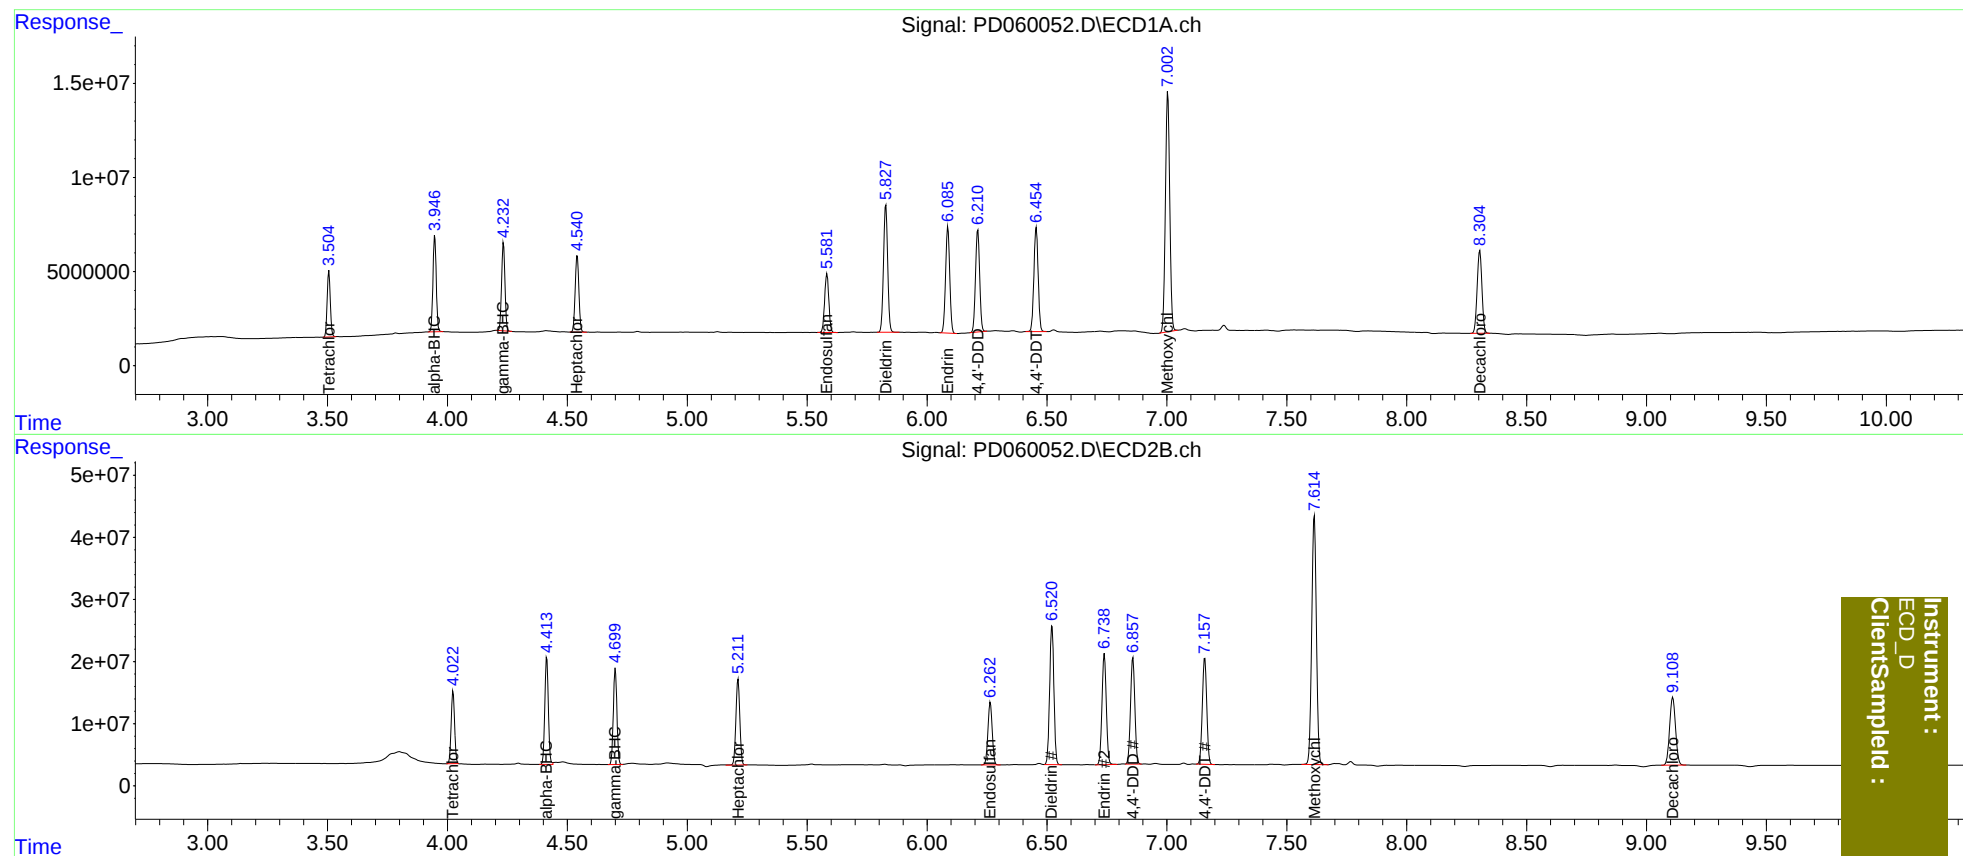


Instrument :
ECD_D
ClientSampled :

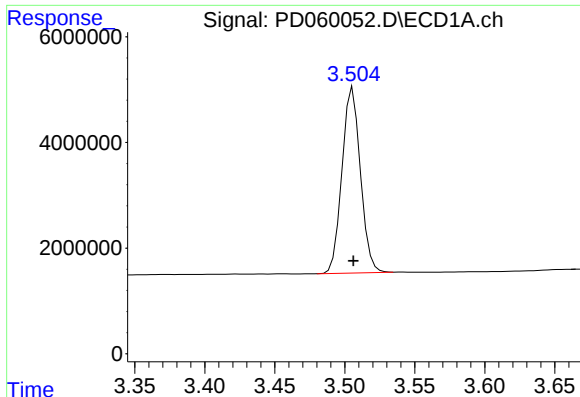

#1 Tetrachloro-m-xylene


R.T.: 3.506 min
Delta R.T.: 0.000 min
Response: 32212293
Conc: 37.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

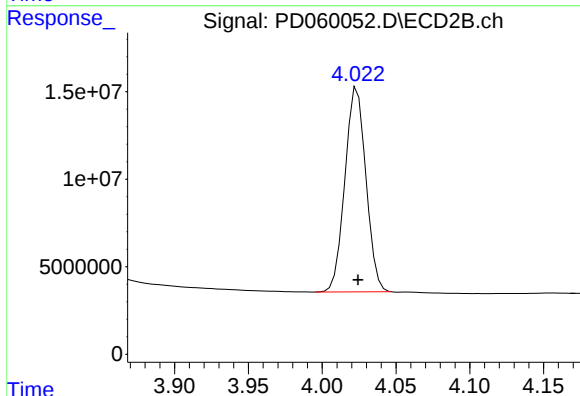


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 115835781
Conc: 38.21 ng/ml

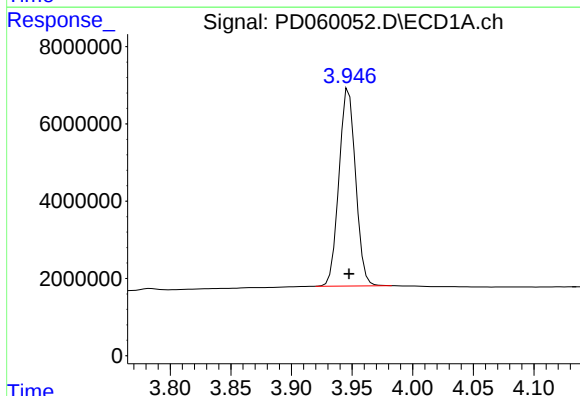


#2 alpha-BHC

R.T.: 3.947 min
Delta R.T.: 0.000 min
Response: 48706163
Conc: 37.92 ng/ml

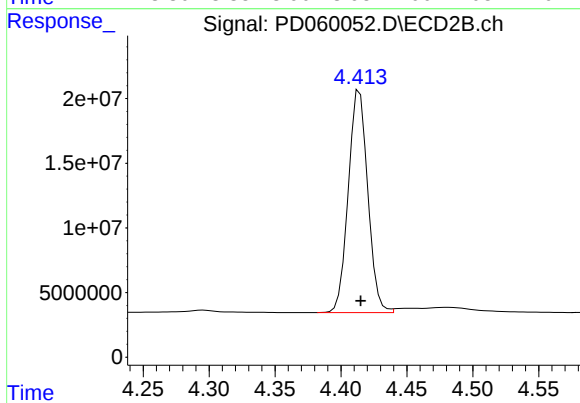

#2 alpha-BHC


R.T.: 4.414 min
Delta R.T.: 0.000 min
Response: 176630756
Conc: 39.38 ng/ml

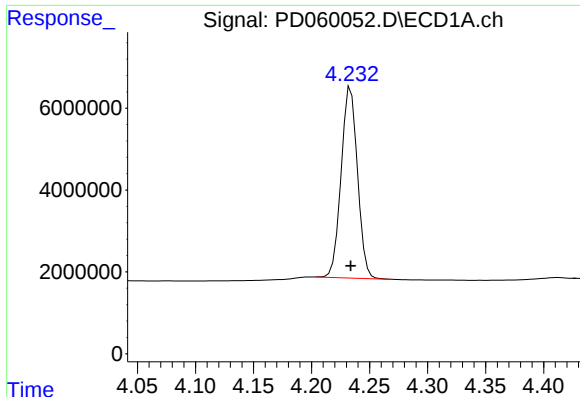

#3 gamma-BHC (Lindane)


R.T.: 4.234 min
Delta R.T.: 0.000 min
Response: 45647099
Conc: 37.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

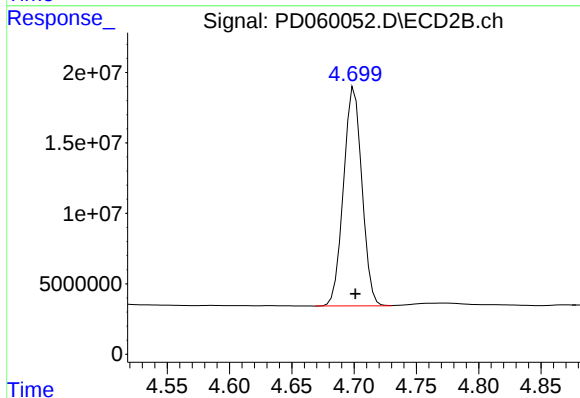


#3 gamma-BHC (Lindane)

R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 160565571
Conc: 39.00 ng/ml

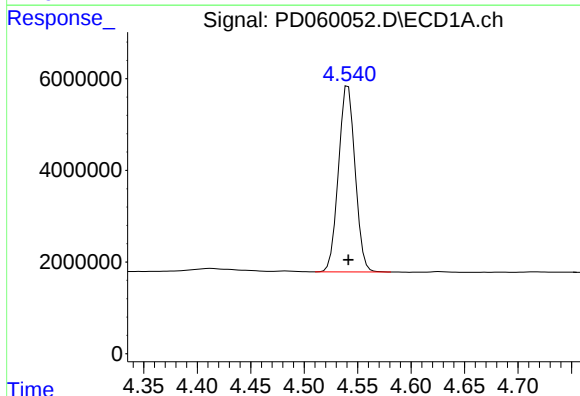


#4 Heptachlor

R.T.: 4.541 min
Delta R.T.: 0.000 min
Response: 43964217
Conc: 37.06 ng/ml

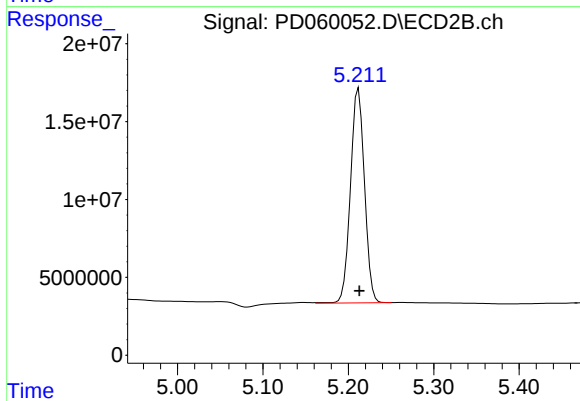

#4 Heptachlor


R.T.: 5.212 min
Delta R.T.: 0.000 min
Response: 156597990
Conc: 38.80 ng/ml

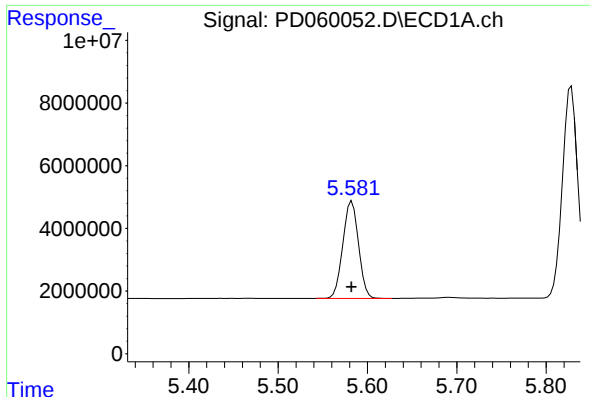

#9 Endosulfan I


R.T.: 5.583 min
Delta R.T.: 0.000 min
Response: 37924120
Conc: 36.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

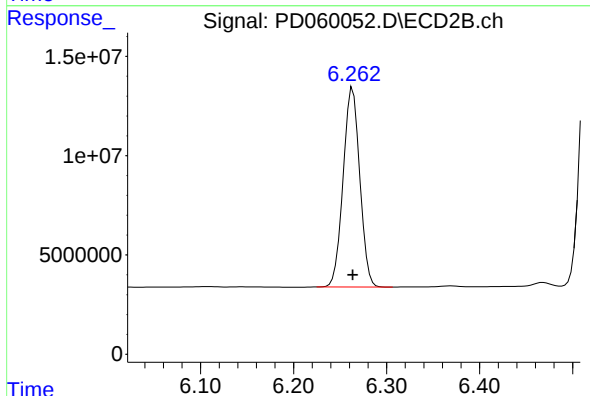


#9 Endosulfan I

R.T.: 6.264 min
Delta R.T.: 0.000 min
Response: 124812971
Conc: 38.40 ng/ml

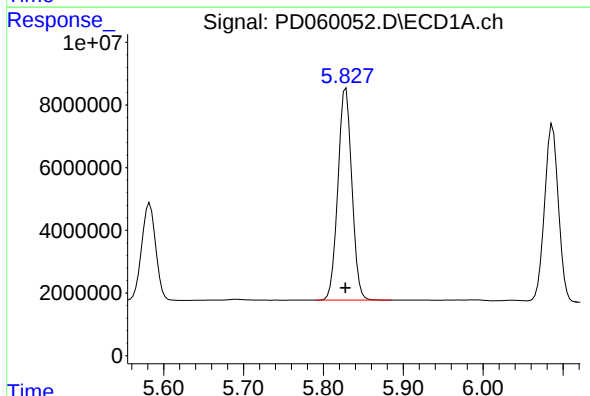


#13 Dieldrin

R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 81902338
Conc: 75.14 ng/ml

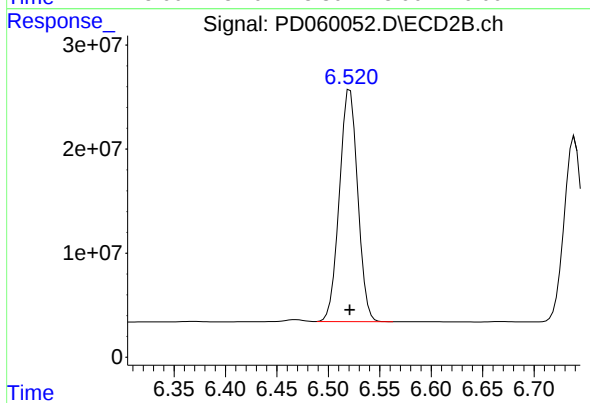

#13 Dieldrin


R.T.: 6.521 min
Delta R.T.: 0.000 min
Response: 276811931
Conc: 77.92 ng/ml

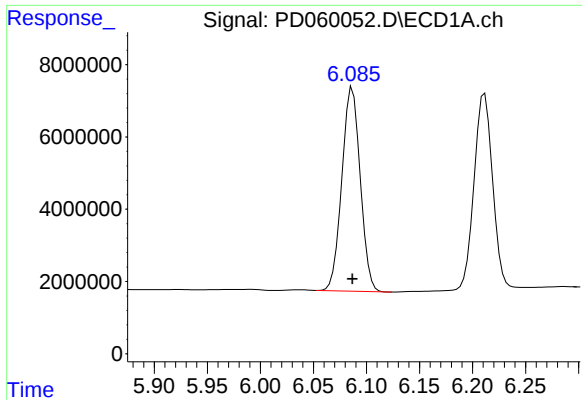

#14 Endrin


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 67839009
Conc: 74.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

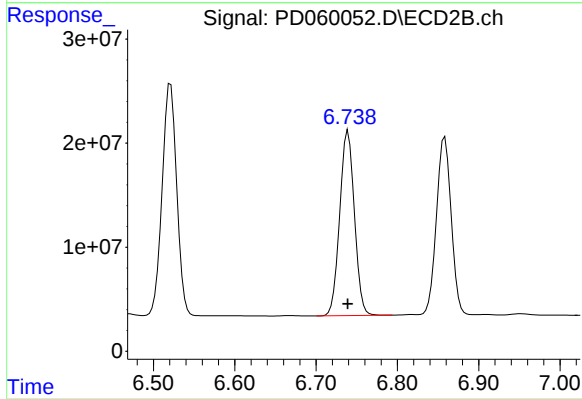


#14 Endrin

R.T.: 6.739 min
Delta R.T.: 0.000 min
Response: 222847529
Conc: 78.23 ng/ml

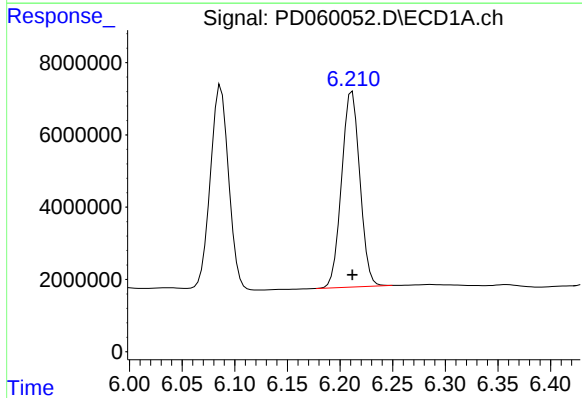


#16 4,4'-DDD

R.T.: 6.212 min
Delta R.T.: 0.000 min
Response: 65557658
Conc: 74.46 ng/ml

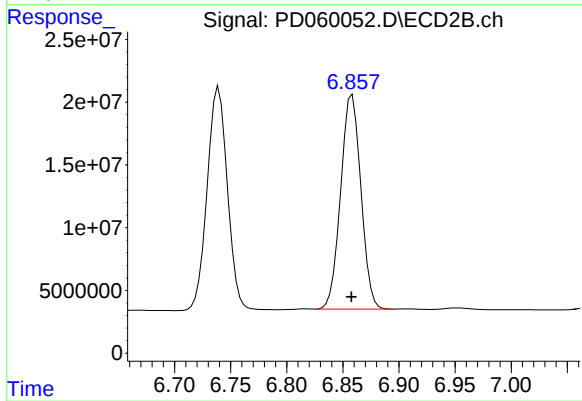

#16 4,4'-DDD


R.T.: 6.858 min
Delta R.T.: 0.000 min
Response: 214109181
Conc: 78.38 ng/ml

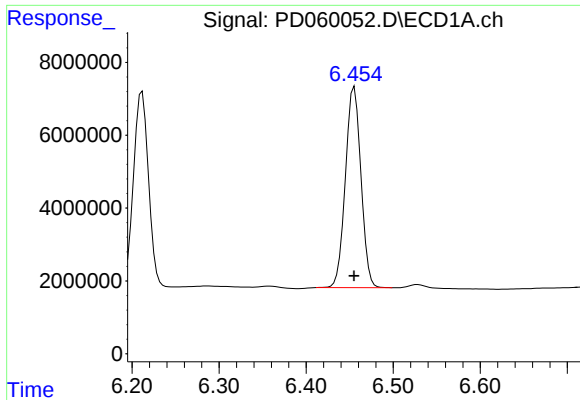

#17 4,4'-DDT


R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 68455038
Conc: 75.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

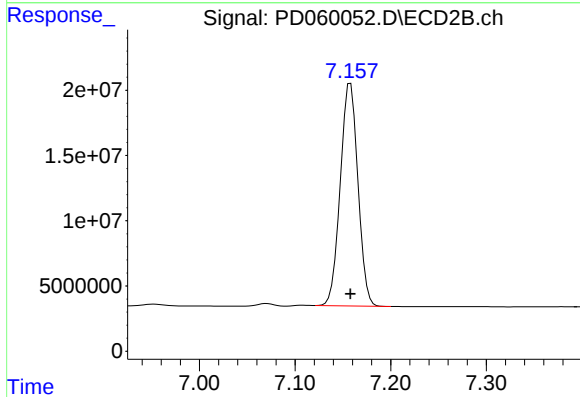


#17 4,4'-DDT

R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 219542742
Conc: 79.40 ng/ml

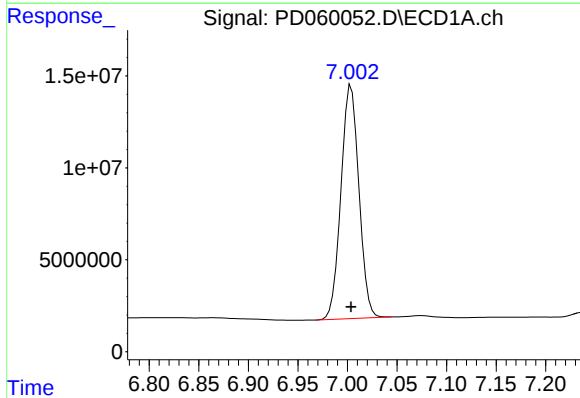


#20 Methoxychlor

R.T.: 7.004 min
Delta R.T.: 0.000 min
Response: 159976706
Conc: 371.47 ng/ml

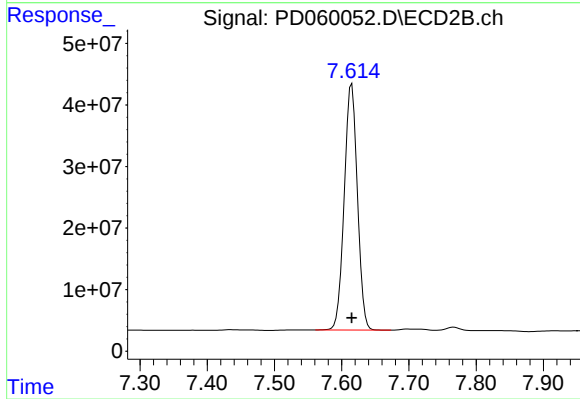

#20 Methoxychlor


R.T.: 7.615 min
Delta R.T.: 0.000 min
Response: 543070207
Conc: 377.77 ng/ml

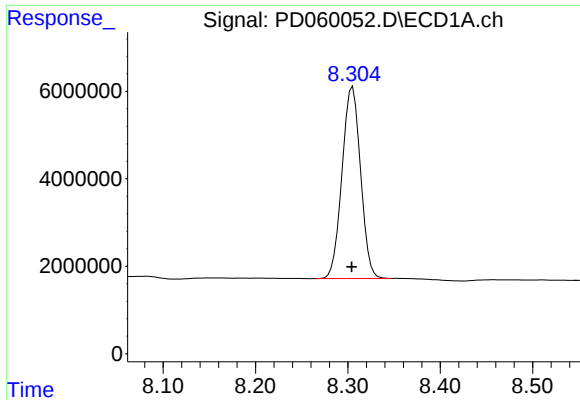

#27 Decachlorobiphenyl

R.T.: 8.305 min
Delta R.T.: 0.001 min
Response: 61114850
Conc: 72.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

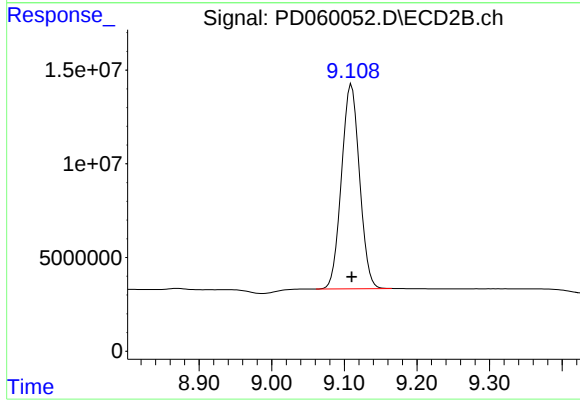

#27 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 188575275
Conc: 74.95 ng/ml