

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
 Data File : PD060054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 14:49
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 03:54:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 03:53:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.505	4.024	62312603	233.0E6	72.140	76.864
27)	SA Decachlor...	8.304	9.110	114.4E6	354.0E6	135.460	140.725
Target Compounds							
2)	A alpha-BHC	3.947	4.414	96304771	360.2E6	74.973	80.305
3)	MA gamma-BHC...	4.233	4.700	90131460	328.0E6	73.552	79.671
4)	MA Heptachlor	4.541	5.212	85119094	319.7E6	71.757	79.209
9)	A Endosulfan I	5.582	6.264	72505620	251.4E6	70.601	77.344
13)	MA Dieldrin	5.827	6.521	161.7E6	559.3E6	148.372	157.445
14)	MA Endrin	6.086	6.739	131.2E6	444.8E6	144.494	156.142
16)	A 4,4'-DDD	6.211	6.858	128.9E6	433.6E6	146.373	158.720
17)	MA 4,4'-DDT	6.455	7.158	135.0E6	442.6E6	148.491	160.068
20)	A Methoxychlor	7.003	7.615	304.9E6	1022.8E6	707.954	711.495

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 14:49
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 03:54:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 03:53:19 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

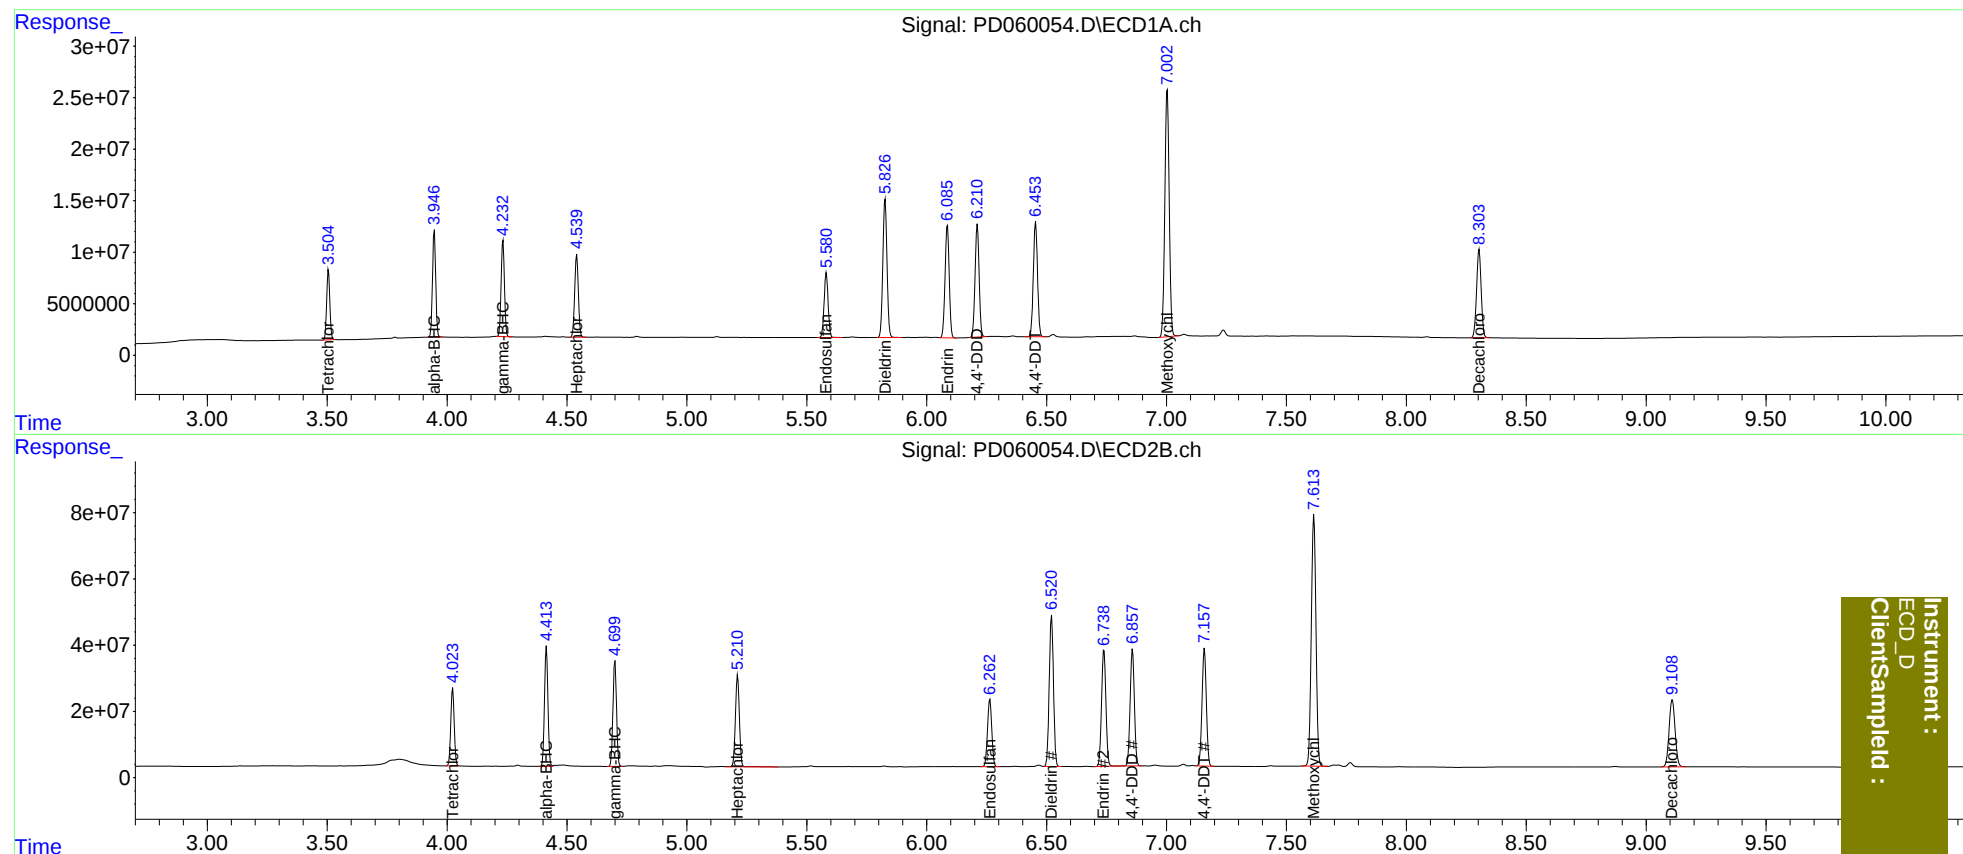


Instrument :
ECD_D
ClientSampled :

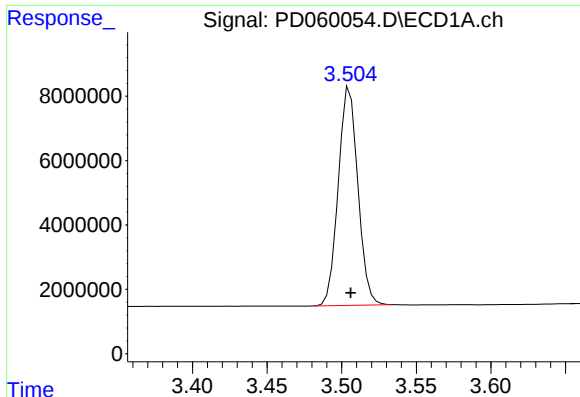

#1 Tetrachloro-m-xylene


R.T.: 3.505 min
Delta R.T.: 0.000 min
Response: 62312603
Conc: 72.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

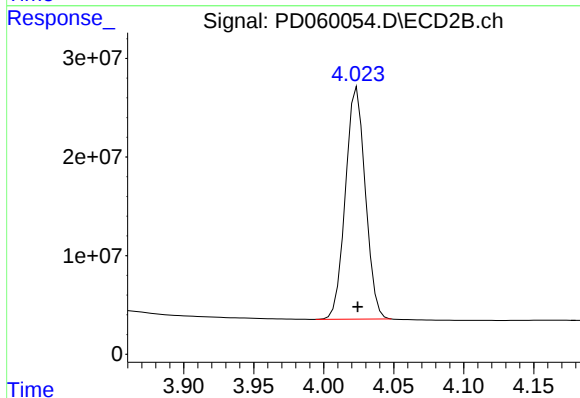


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 233011285
Conc: 76.86 ng/ml

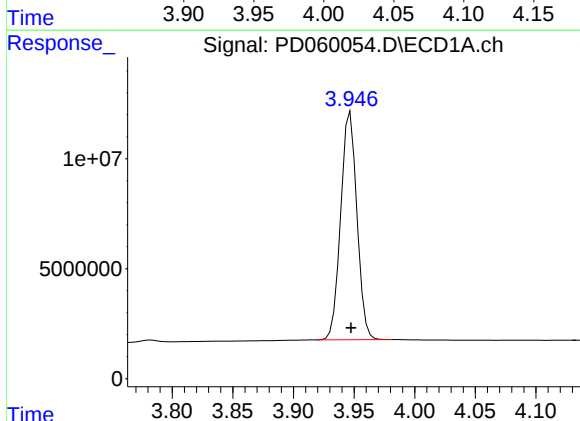


#2 alpha-BHC

R.T.: 3.947 min
Delta R.T.: 0.000 min
Response: 96304771
Conc: 74.97 ng/ml

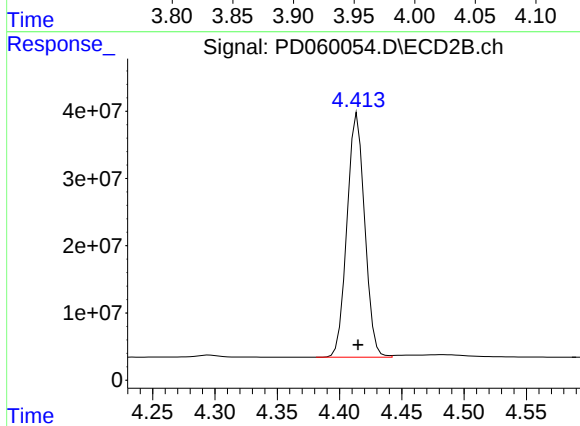

#2 alpha-BHC


R.T.: 4.414 min
Delta R.T.: 0.000 min
Response: 360220791
Conc: 80.31 ng/ml

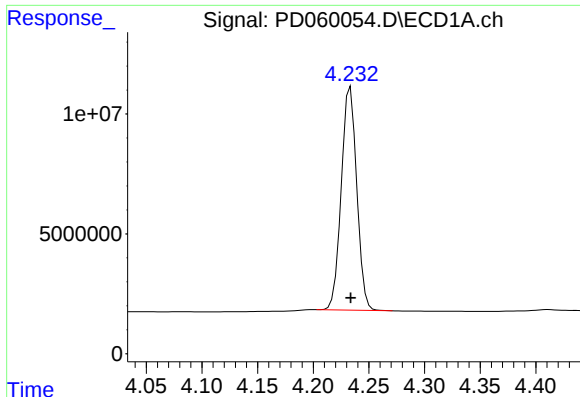

#3 gamma-BHC (Lindane)


R.T.: 4.233 min
Delta R.T.: 0.000 min
Response: 90131460
Conc: 73.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

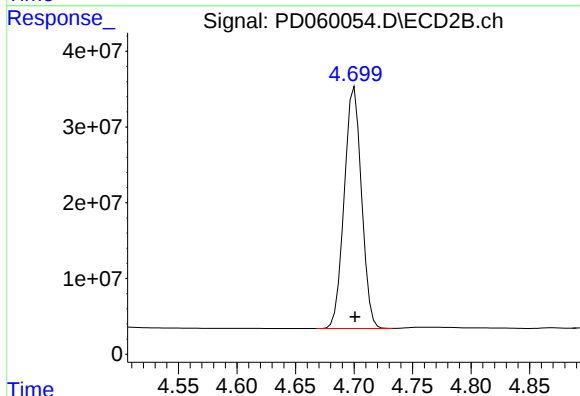


#3 gamma-BHC (Lindane)

R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 328043368
Conc: 79.67 ng/ml

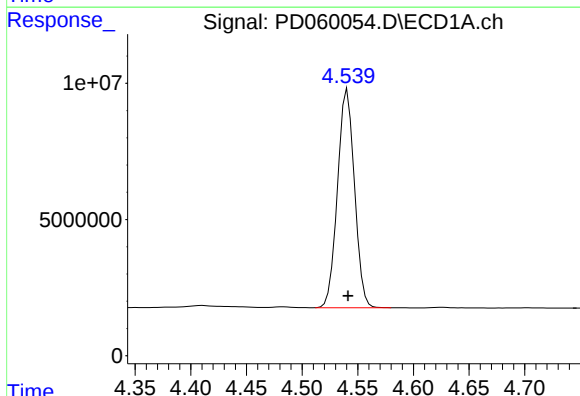


#4 Heptachlor

R.T.: 4.541 min
Delta R.T.: 0.000 min
Response: 85119094
Conc: 71.76 ng/ml

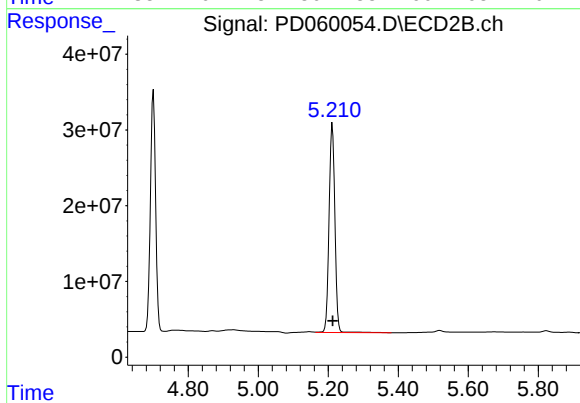

#4 Heptachlor


R.T.: 5.212 min
Delta R.T.: -0.001 min
Response: 319697802
Conc: 79.21 ng/ml

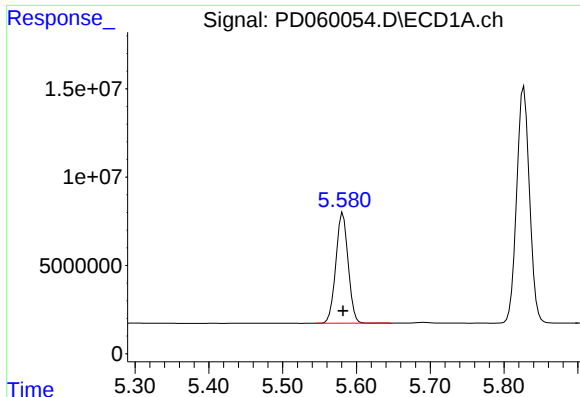

#9 Endosulfan I


R.T.: 5.582 min
Delta R.T.: 0.000 min
Response: 72505620
Conc: 70.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

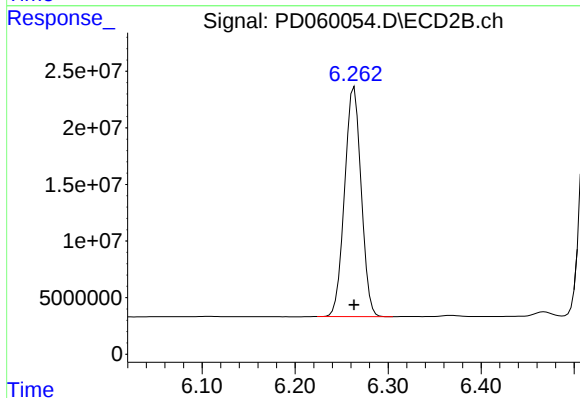


#9 Endosulfan I

R.T.: 6.264 min
Delta R.T.: 0.000 min
Response: 251401806
Conc: 77.34 ng/ml

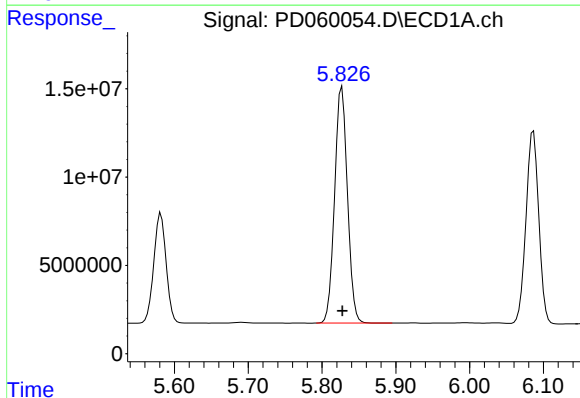


#13 Dieldrin

R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 161716218
Conc: 148.37 ng/ml

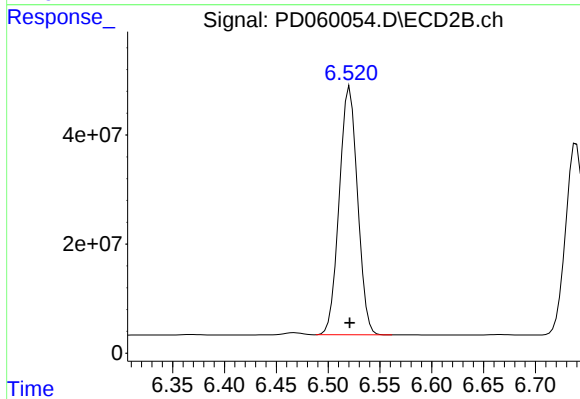

#13 Dieldrin


R.T.: 6.521 min
Delta R.T.: 0.000 min
Response: 559315458
Conc: 157.44 ng/ml

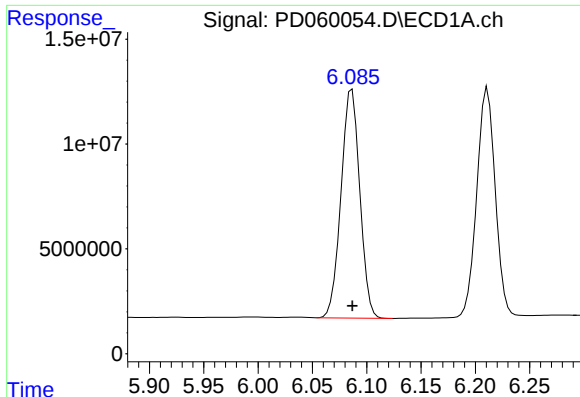

#14 Endrin


R.T.: 6.086 min
Delta R.T.: 0.000 min
Response: 131190078
Conc: 144.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

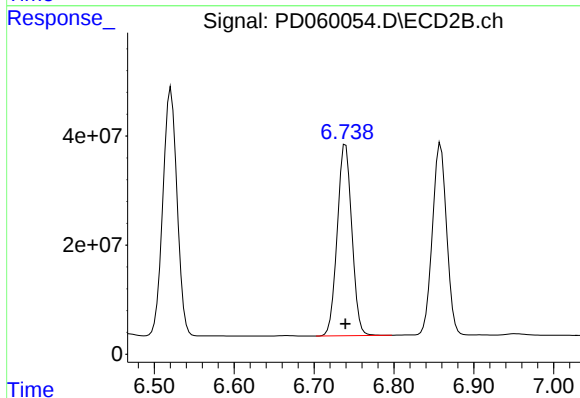


#14 Endrin

R.T.: 6.739 min
Delta R.T.: 0.000 min
Response: 444791637
Conc: 156.14 ng/ml

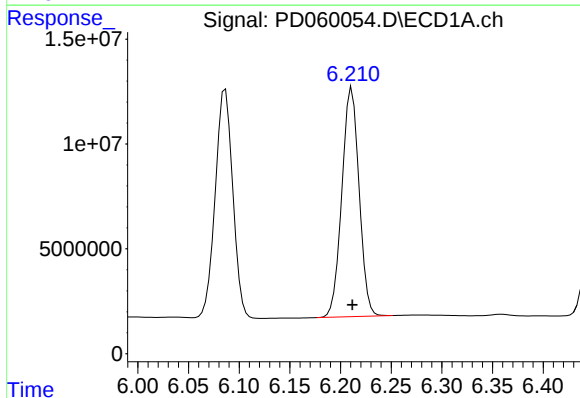


#16 4,4'-DDD

R.T.: 6.211 min
Delta R.T.: 0.000 min
Response: 128876675
Conc: 146.37 ng/ml

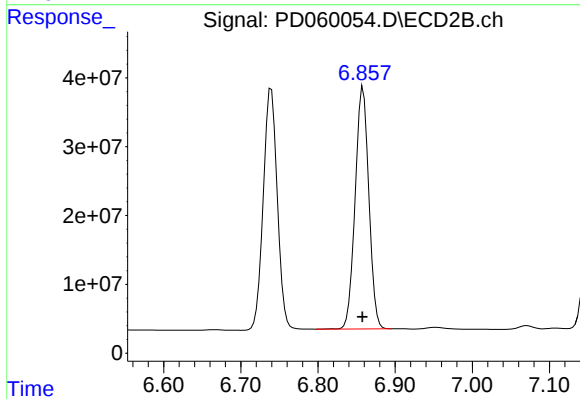

#16 4,4'-DDD


R.T.: 6.858 min
Delta R.T.: 0.000 min
Response: 433583150
Conc: 158.72 ng/ml

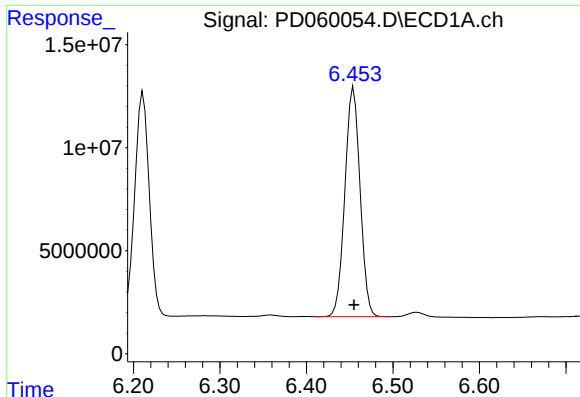

#17 4,4'-DDT


R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 135036973
Conc: 148.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

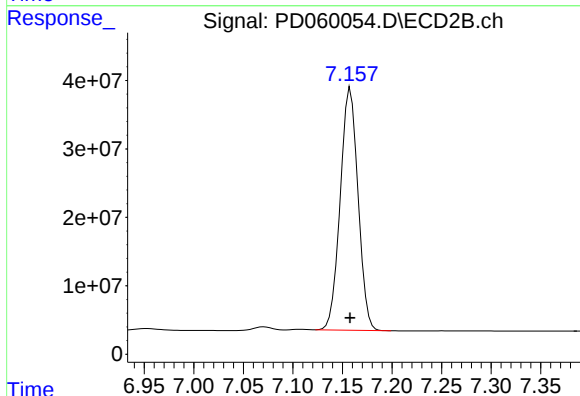


#17 4,4'-DDT

R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 442592701
Conc: 160.07 ng/ml

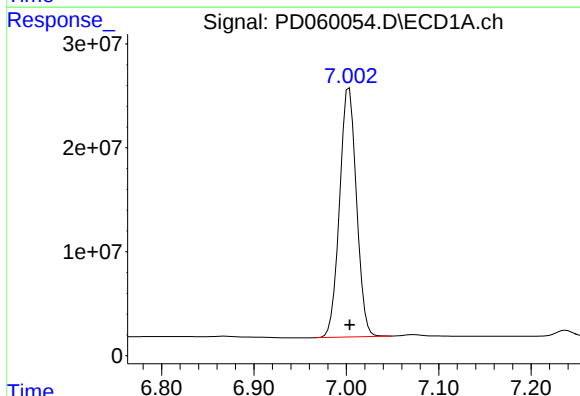


#20 Methoxychlor

R.T.: 7.003 min
Delta R.T.: 0.000 min
Response: 304890073
Conc: 707.95 ng/ml

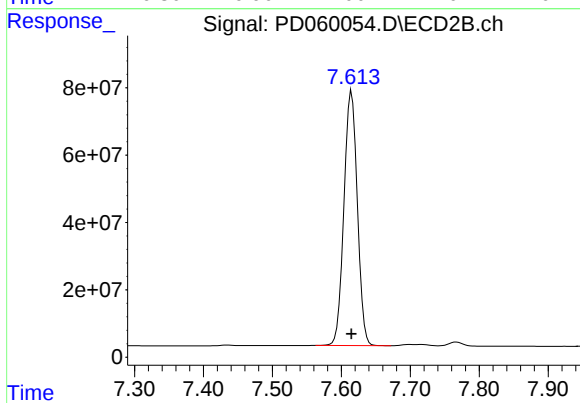

#20 Methoxychlor

R.T.: 7.615 min
Delta R.T.: 0.000 min
Response: 1022828604
Conc: 711.49 ng/ml

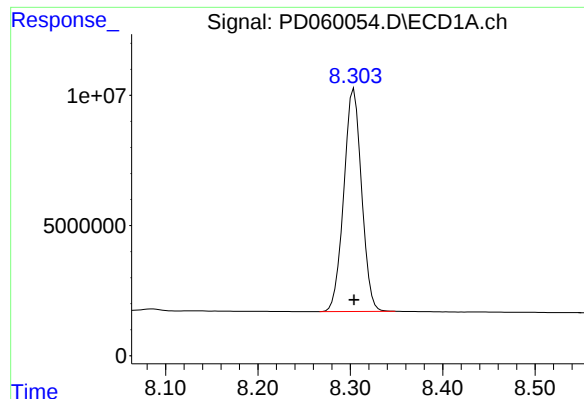

#27 Decachlorobiphenyl


R.T.: 8.304 min

Delta R.T.: 0.000 min

Response: 114449191

Conc: 135.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

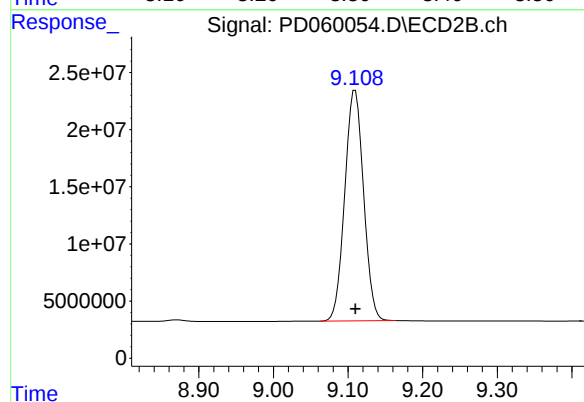

#27 Decachlorobiphenyl

R.T.: 9.110 min

Delta R.T.: 0.000 min

Response: 354044116

Conc: 140.72 ng/ml