

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 16:41
Operator : DD\AJ
Sample : L4586-03
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
C0AA5

Manual Integrations
APPROVED

Ankita
11/5/2020 11:17:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 04:10:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

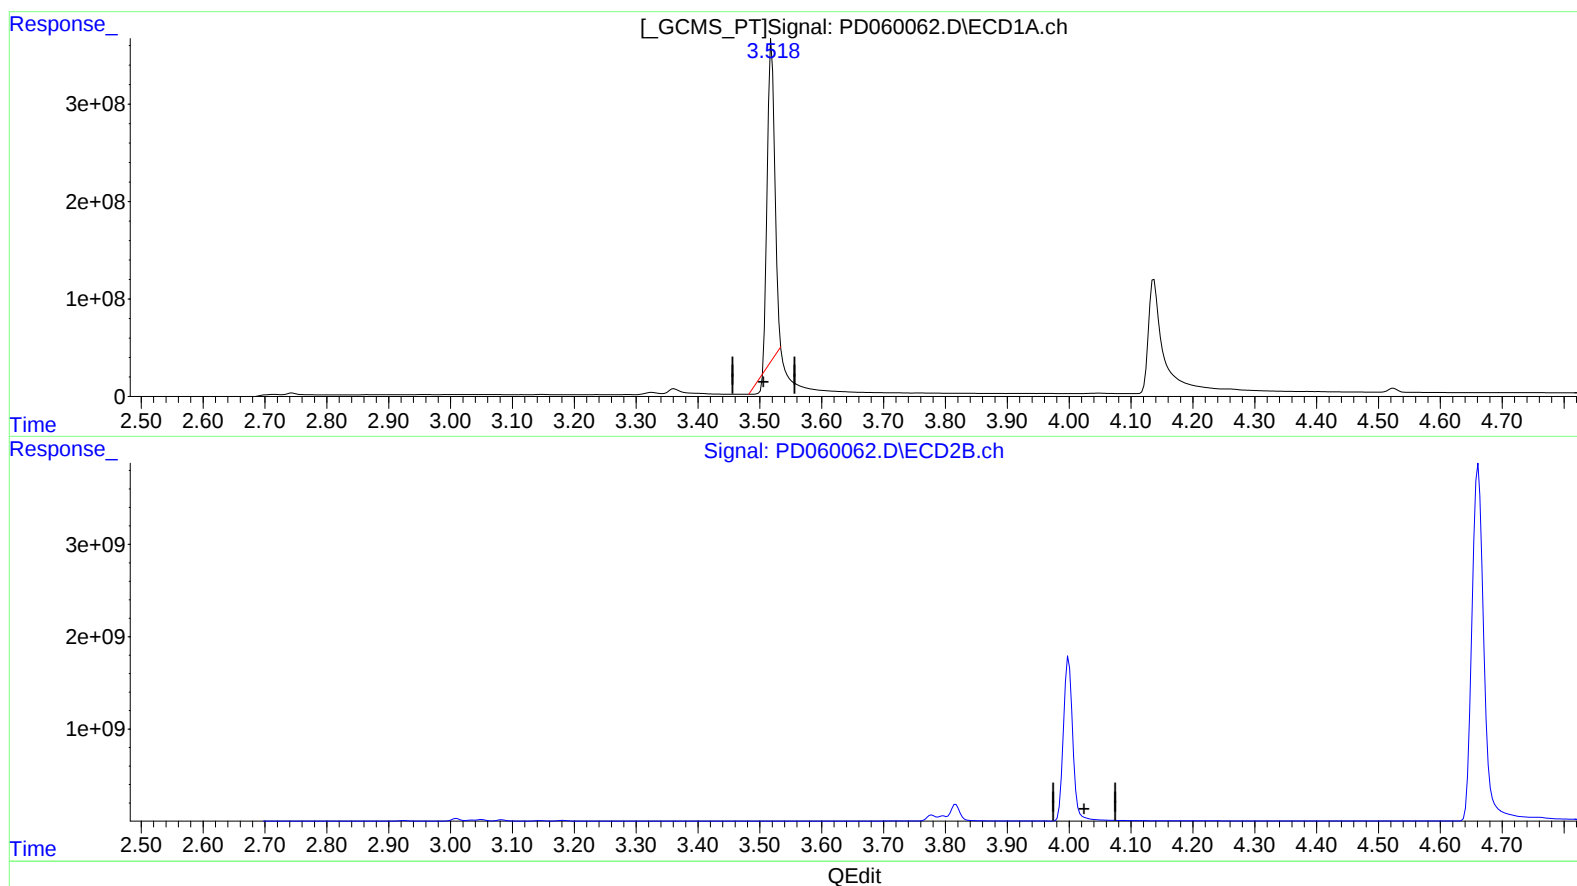

(1) Tetrachloro-m-xylene (SA)

3.519min 3159.943 ng/ml

response 2707961622

(1) Tetrachloro-m-xylene #2 (SA)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 16:41
Operator : DD\AJ
Sample : L4586-03
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
C0AA5

Manual Integrations
APPROVED

Ankita
11/5/2020 11:17:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 04:10:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

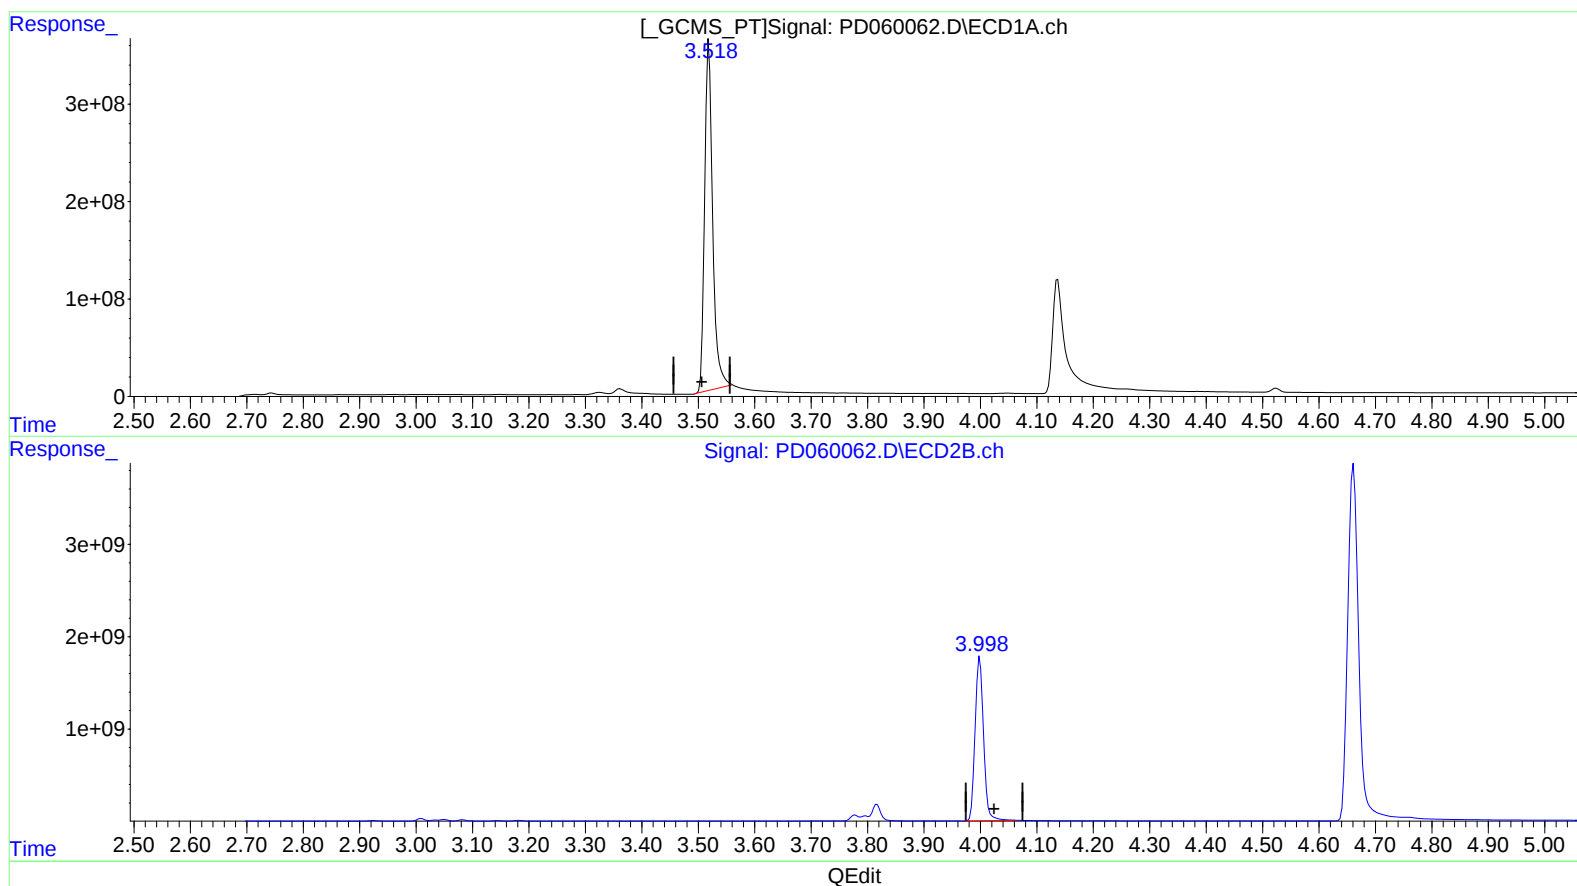

(1) Tetrachloro-m-xylene (SA)

3.518min 4128.141 ng/ml m

response 3537672827

(1) Tetrachloro-m-xylene #2 (SA)

3.998min 6195.759 ng/ml m

response 18468982800

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
 Data File : PD060062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 16:41
 Operator : DD\AJ
 Sample : L4583-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

Ankita
 11/5/2020 11:17:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 04:10:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.518	3.998f	3537.7E6	18469.0E6	4128.141m	6195.759m#
27) SA Decachlor...	8.304	9.109	24980530	77962072	30.065	31.691
Target Compounds						
13) MA Dieldrin	5.827	6.520	8524221	27444435	7.824	7.860
15) B Endosulfa...	6.360	6.928	3501362	7569203	3.883	2.678 #

AJ
 11/06/20

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.