

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 16:55
Operator : DD\AJ
Sample : L4583-04
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
C0AA7

Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 04:10:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

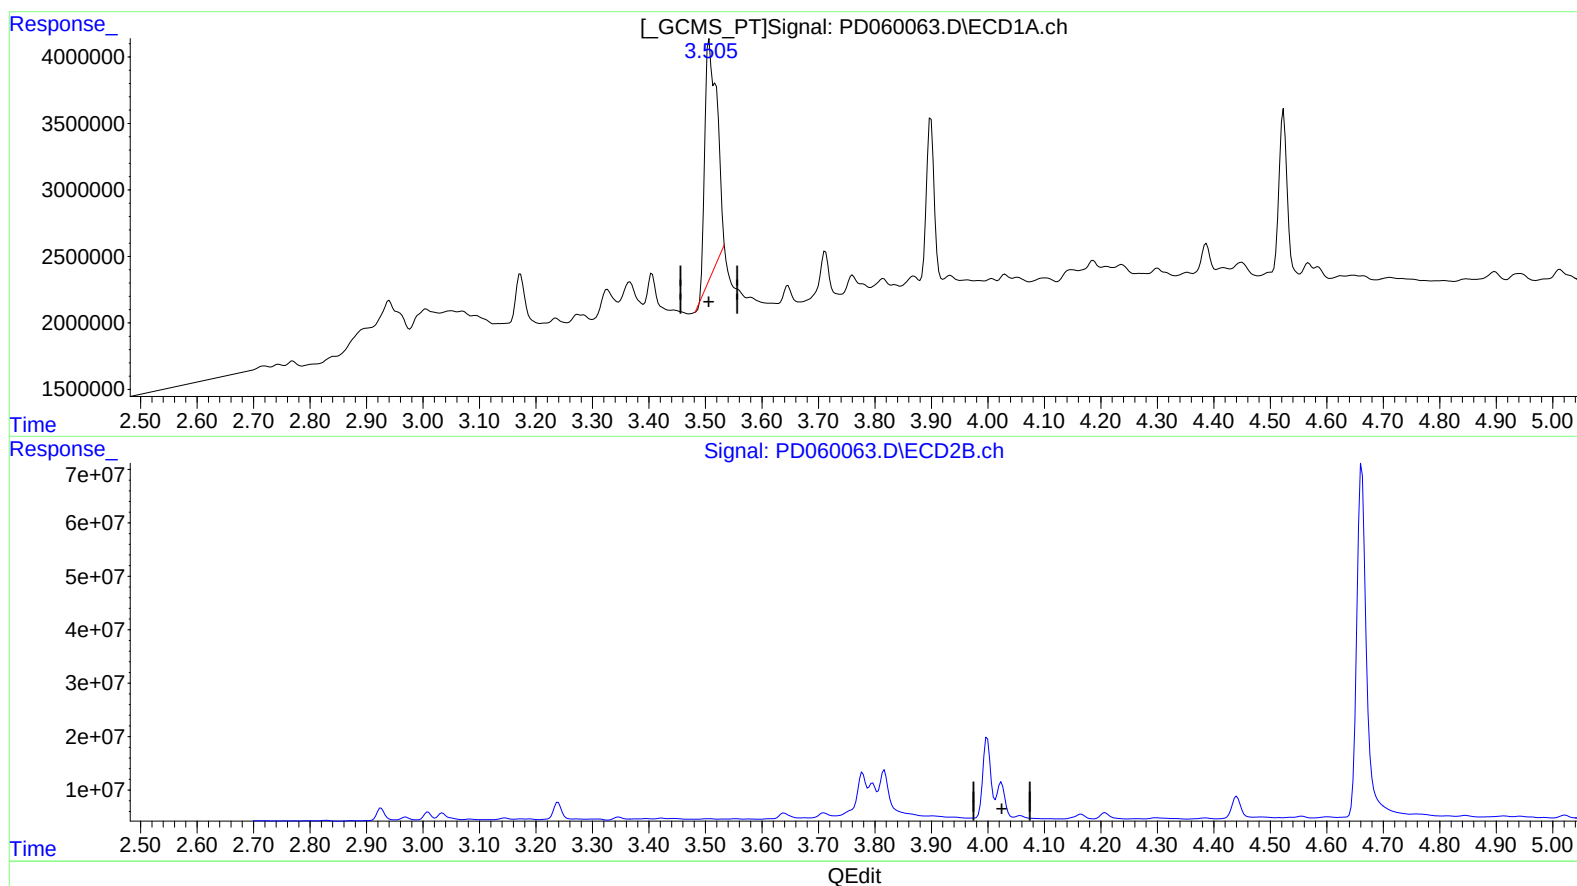

(1) Tetrachloro-m-xylene (SA)

3.507min 31.565 ng/ml

response 27050076

(1) Tetrachloro-m-xylene #2 (SA)

4.024min -26.484 ng/ml

response -78945618

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 16:55
Operator : DD\AJ
Sample : L4583-04
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
C0AA7

Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 04:10:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

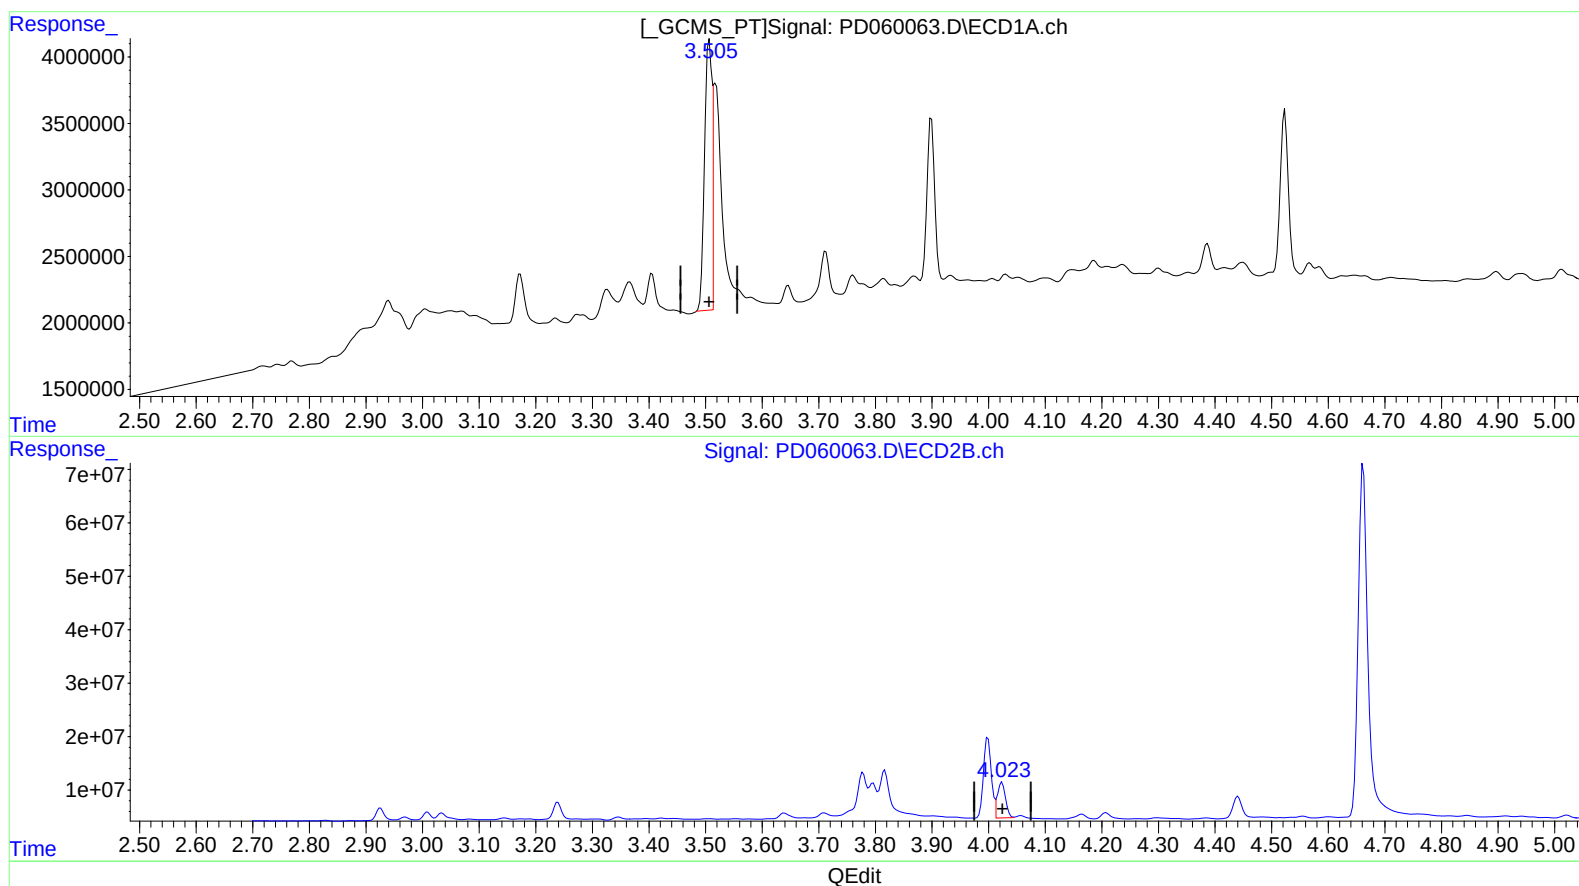

(1) Tetrachloro-m-xylene (SA)

3.505min 24.800 ng/ml m

response 21252864

(1) Tetrachloro-m-xylene #2 (SA)

4.023min 21.173 ng/ml m

response 63114690

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
 Data File : PD060063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 16:55
 Operator : DD\AJ
 Sample : L4583-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA7

Manual Integrations
 APPROVED

Ankita
 11/4/2020 4:56:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 04:10:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.505	4.023	21252864	63114690	24.800m	21.173m
27) SA Decachlor...	8.303	9.107	25763339	82066652	31.007	33.360
Target Compounds						
8) B Heptachlo...	5.238	5.897	2557155	7970270	2.421	2.420
13) MA Dieldrin	5.826	6.520	16817415	52904555	15.435	15.151

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AS
 11/06/20