

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 17:38
Operator : DD\AJ
Sample : L4583-07MS
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
C0AA9MS

Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 05:07:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

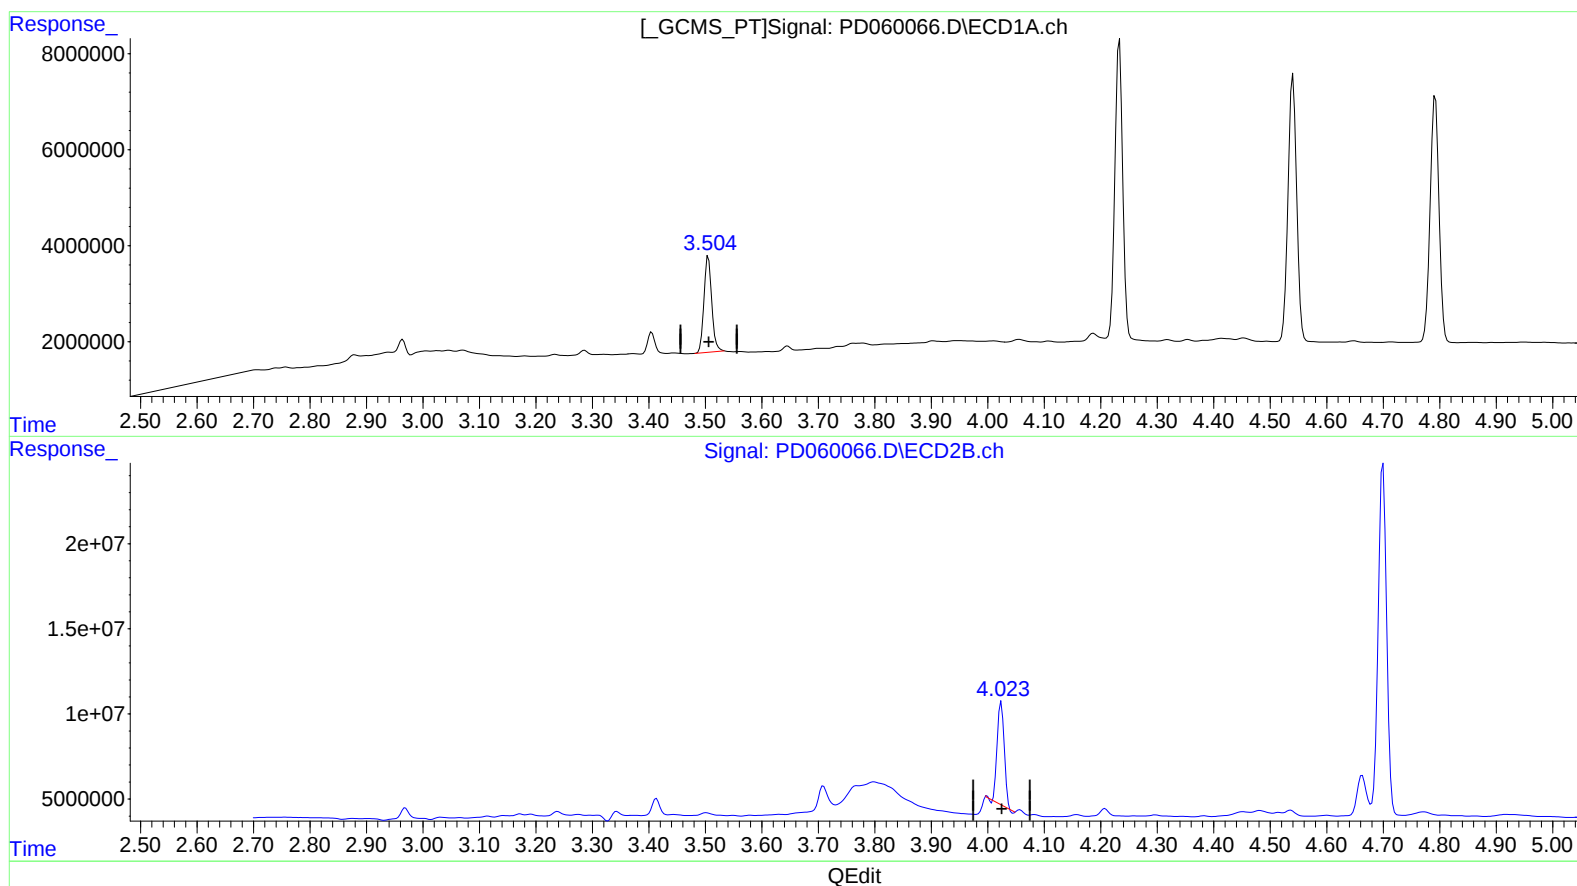

(1) Tetrachloro-m-xylene (SA)

3.505min 22.465 ng/ml

response 19252129

(1) Tetrachloro-m-xylene #2 (SA)

4.024min 17.227 ng/ml

response 51352578

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
Data File : PD060066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2020 17:38
Operator : DD\AJ
Sample : L4583-07MS
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
C0AA9MS

Manual Integrations
APPROVED

Ankita
11/4/2020 4:56:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 05:07:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

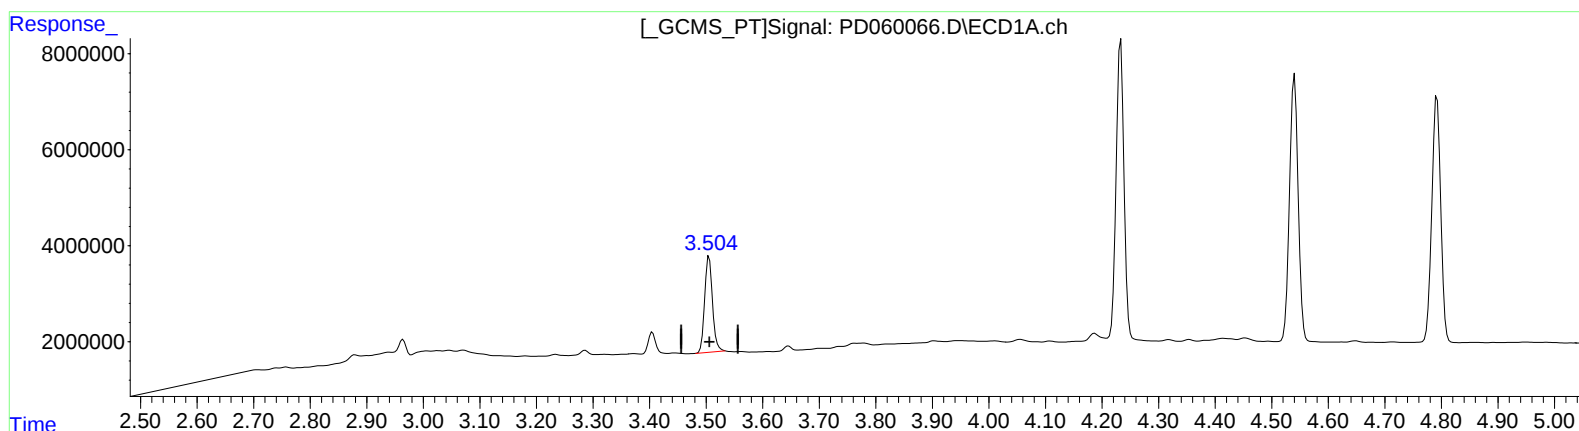

(1) Tetrachloro-m-xylene (SA)

3.505min 22.465 ng/ml

response 19252129

(1) Tetrachloro-m-xylene #2 (SA)

4.023min 22.015 ng/ml m

response 65624641

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110320\
 Data File : PD060066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2020 17:38
 Operator : DD\AJ
 Sample : L4583-07MS
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA9MS

Manual Integrations
 APPROVED

Ankita
 11/4/2020 4:56:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 05:07:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.505	4.023	19252129	65624641	22.465	22.015m
27) SA Decachlor...	8.302	9.108	29757630	90782501	35.814	36.903
Target Compounds						
3) MA gamma-BHC...	4.233	4.700	59902280	217.3E6	49.005	53.700
4) MA Heptachlor	4.540	5.212	59202266	212.7E6	50.440	53.651
5) MB Aldrin	4.792	5.518	56546850	196.9E6	49.253	53.065
13) MA Dieldrin	5.826	6.520	113.2E6	390.0E6	103.867	111.688
14) MA Endrin	6.086	6.738	95103763	315.5E6	105.419	112.689
17) MA 4,4'-DDT	6.453	7.157	89605223	294.2E6	99.698	108.099

> AJ
 11/06/20

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.